

? am 1/20/02 ref

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB *		600 mL		1 mL			1 mL	3A	71			
Ref					0.5 mL			2B				
1142								4B				
1139								1A				
1141								1B				
1140								3B				
1138								4A				
1136								2A				
LB had lower surrogate recovery; however it contained only those compounds typically attributable to the extracting solvents or column bleed. (WB)												
BATCH # EGCMS-17121												
Remarks 1140 and 1136 had dark yellow tints after being concentrated.												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type - <u>sepfun</u> Solv. lot# <u>V39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39H00</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	<u>91759</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>011602</u>											
LPC												
ENDRIN/DDT												


Analyst LF
revision 4/12/01

Verified by _____

Reviewed by DN
Date 2/27/02

Data File : C:\MSDCHEM\1\5973N\02FEB25\0225DF.D
 Acq On : 25 Feb 2002 8:37 am
 Sample : dftpp
 Misc : February 25, 2002
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\HP020702.M (RTE Integrator)
 Title : 508 scan method

Vial: 1
 Operator:
 Inst : Instrume
 Multiplr: 1.00

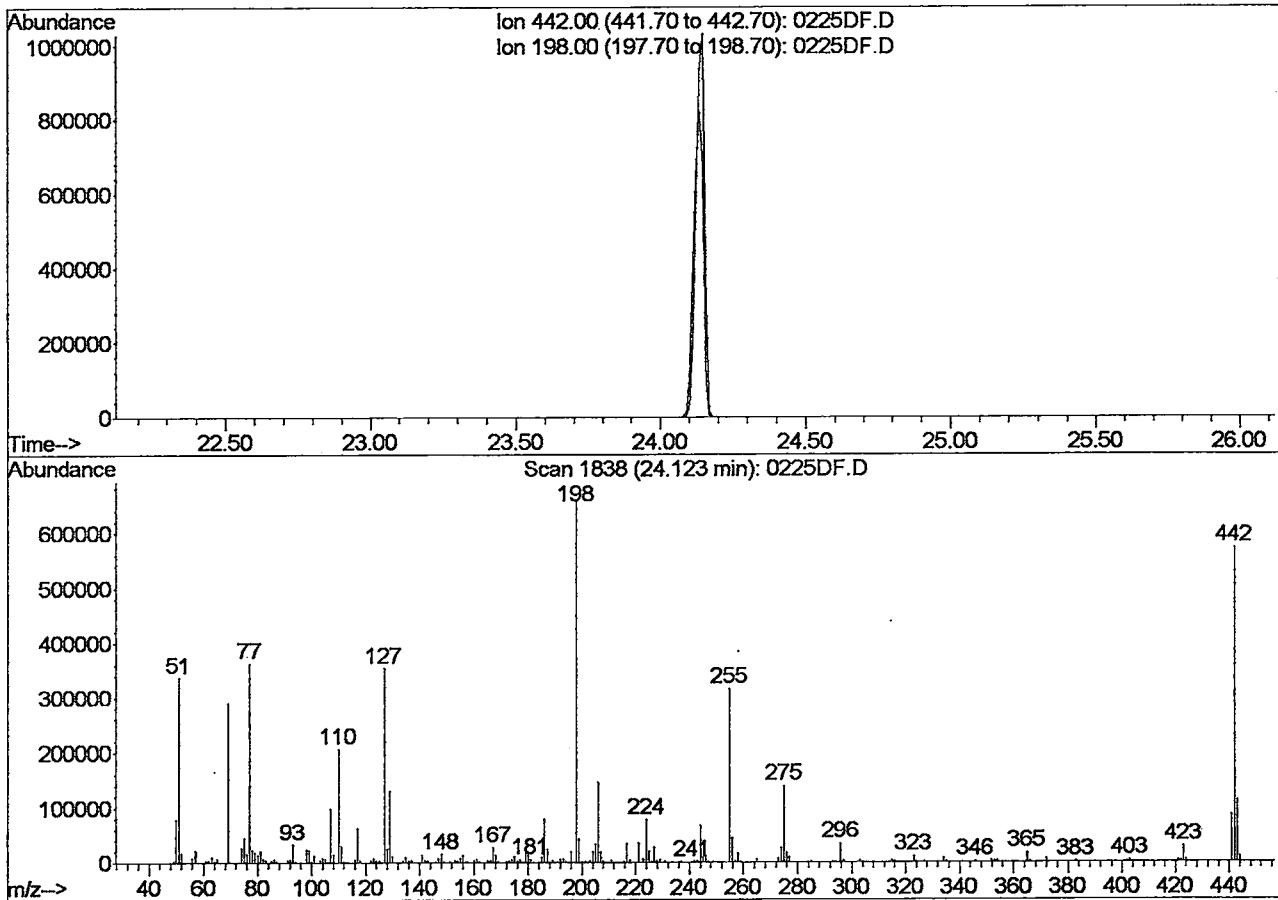

Spectrum Information: Scan 1838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	51.1	337728	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.0	291008	PASS
70	69	0.00	2	0.4	1044	PASS
127	198	40	60	53.7	354688	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	661056	PASS
199	198	5	9	6.7	44064	PASS
275	198	10	30	21.3	140608	PASS
365	198	1	99	2.8	18248	PASS
441	443	1	99	76.3	86856	PASS
442	198	40	110	86.8	573568	PASS
443	442	17	23	19.9	113904	PASS

0225DF.D HP020702.M

Mon Feb 25 10:13:45 2002