


2-Propanol, 1-(2-methoxy-1-methylethoxy) -

Entry Number 9238 from C:\DATABASE\nbs75k.1
 CAS 020324-32-7
 Melting Point -300
 Boiling Point -300
 Retention Index 0
 Mol Formula C7H16O3
 Mol Weight 148.109
 Company ID NIST 1992

Miscellaneous Information
 QI=57 Steroids; Alkaloids; Misc. Natural products;

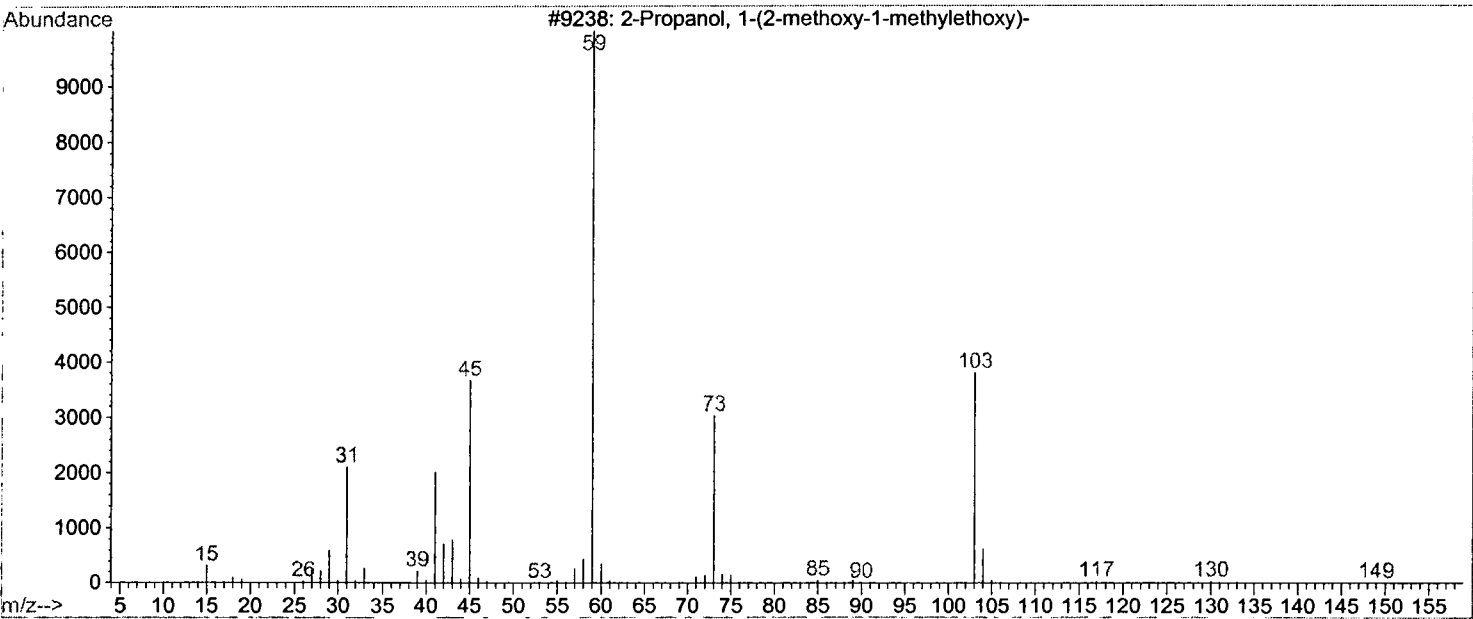

No structure available for 020324-32-7

Sequence Name: C:\HPCHEM\1\SEQUENCE\FEB2102.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\feb2102\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0208	
2	Sample	2	CAL40	GCMS0208	
3	Sample	29	SURR	GCMS0208	
4	Sample	3	LB	GCMS0208	gc/ms scan 1/22
5	Sample	4	REF	GCMS0208	gc/ms scan 1/22
6	Sample	5	1329	GCMS0208	gc/ms scan 1/22
7	Sample	6	472	GCMS0208	gc/ms scan 1/22
8	Sample	7	1435	GCMS0208	gc/ms scan 1/22
9	Sample	8	1436	GCMS0208	gc/ms scan 1/22
10	Sample	9	1437	GCMS0208	gc/ms scan 1/22
11	Sample	10	1438	GCMS0208	gc/ms scan 1/22
12	Sample	11	1439	GCMS0208	gc/ms scan 1/22
13	Sample	12	1440	GCMS0208	gc/ms scan 1/22
14	Sample	13	1441	GCMS0208	gc/ms scan 1/22
15	Sample	14	1442	GCMS0208	gc/ms scan 1/22
16	Sample	15	1462	GCMS0208	gc/ms scan 1/22
17	Sample	1	DFTPP2	GCMS0208	gc/ms scan 1/22
18	Sample	2	CAL40A	GCMS0208	gc/ms scan 1/22
19	Sample	16	LBA	GCMS0208	gc/ms scan 1/22
20	Sample	17	REFA	GCMS0208	gc/ms scan 1/22
21	Sample	18	1463	GCMS0208	gc/ms scan 1/22
22	Sample	19	1464	GCMS0208	gc/ms scan 1/22
23	Sample	20	1465	GCMS0208	gc/ms scan 1/22
24	Sample	21	1498	GCMS0208	gc/ms scan 1/22
25	Sample	22	1499	GCMS0208	gc/ms scan 1/22
26	Sample	23	1500	GCMS0208	gc/ms scan 1/22
27	Sample	24	1501	GCMS0208	gc/ms scan 1/22
28	Sample	25	1502	GCMS0208	gc/ms scan 1/22
29	Sample	26	1503	GCMS0208	gc/ms scan 1/22
30	Sample	27	1504	GCMS0208	gc/ms scan 1/22
31	Sample	28	1505	GCMS0208	gc/ms scan 1/22
32	Sample	30	LBB	GCMS0208	gc/ms scan 2/21
33	Sample	31	REFB	GCMS0208	gc/ms scan 2/21
34	Sample	32	REFB2	GCMS0208	gc/ms scan 2/21
35	Sample	33	31549	GCMS0208	gc/ms scan 2/21
36	Sample	34	31587	GCMS0208	gc/ms scan 2/21
37	Sample	35	31499	GCMS0208	gc/ms scan 2/21
38	Sample	36	31498	GCMS0208	gc/ms scan 2/21
39	Sample	37	31551	GCMS0208	gc/ms scan 2/21
40	Sample	38	31591	GCMS0208	gc/ms scan 2/21
41	Sample	39	31589	GCMS0208	gc/ms scan 2/21
42	Sample	40	31590	GCMS0208	gc/ms scan 2/21


Last Modified: Fri Feb 22 17:04:26 2002

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB2102\DFTPP2.D
 Acq On : 22 Feb 2002 4:52 am
 Sample : gc/ms scan 1/22
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

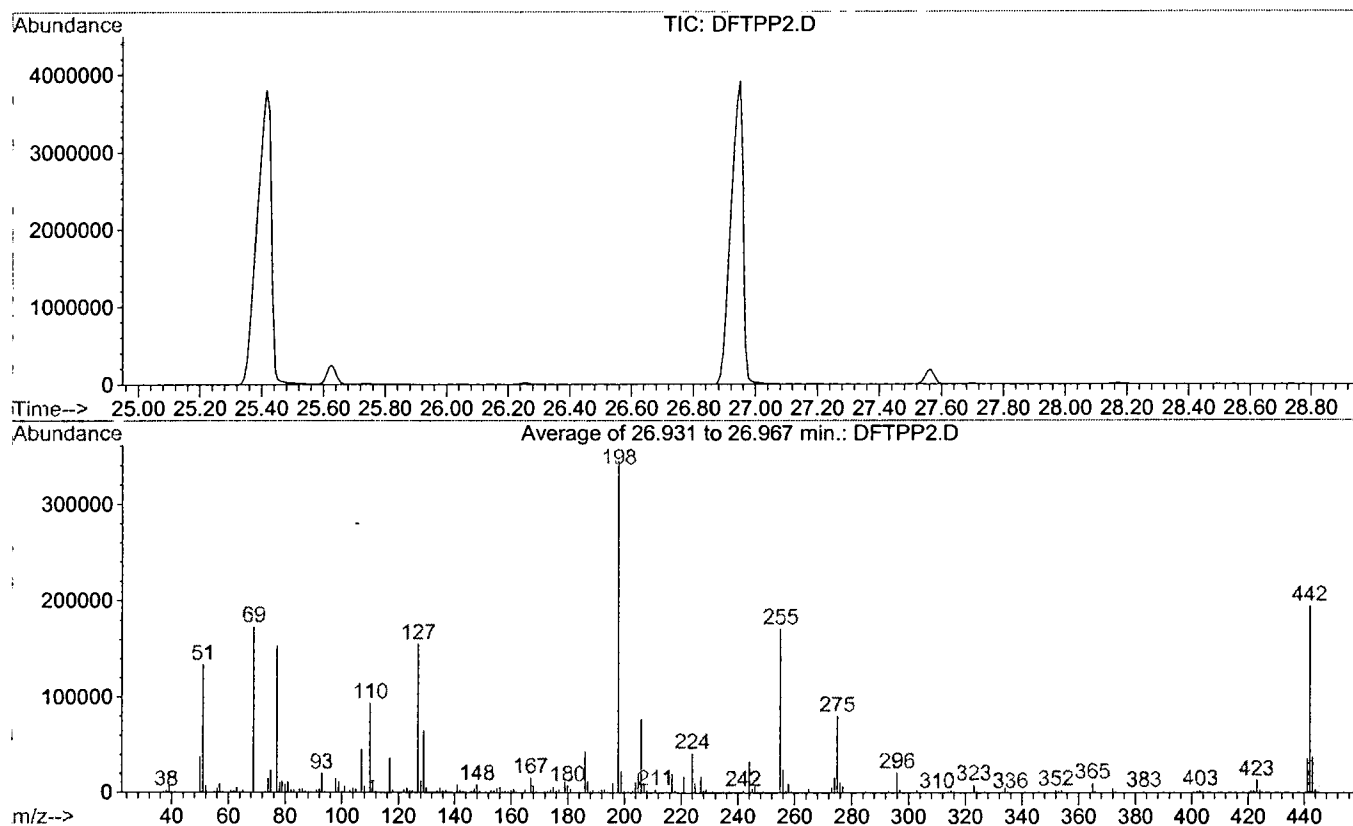

Spectrum Information: Average of 26.931 to 26.967 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	38.9	133754	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.3	172777	PASS
70	69	0.00	2	0.1	152	PASS
127	198	40	60	45.1	154979	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	343443	PASS
199	198	5	9	6.6	22571	PASS
275	198	10	30	23.1	79232	PASS
365	198	1	100	2.8	9599	PASS
441	443	0.01	100	95.5	35398	PASS
442	198	40	110	56.4	193866	PASS
443	442	17	23	19.1	37058	PASS