


Method 508 MOD.

Date Extracted 1-25-02

Page 47

Ref

#CCMS-17157

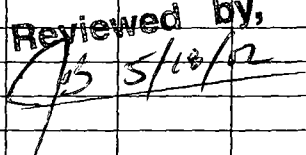Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
L.B.		500.00		1ml			1ml	3B	7	
Ref					0.5ml			9A		
1733								3A		
1734								10B		
1735	F.B.							1B		
1796								10A		
1797								1A		
1798								5A		
1799								2B		
1800								4A		
1801								2A		
1802								4B		
1803	F.B.	↓		↓			↓		↓	
Remarks										
Reviewed by,  5/18/02										
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - <u>Self Fan.</u> Solv.lot# <u>V 4/470</u> NaCl lot# <u>V 1599</u> Na2SO4 lot# <u>1599 08</u> STANDARD INT STD LOG# CALIBRATION <u>11/20/02</u> REF# <u>11/159</u> MDL Q. C INT. II <u>11/102</u> SURROGATE <u>GCHS 011602</u> LPC ENDRIN/DDT										

Analyst A.D.
Revision 4/12/01

Verified by mg

Reviewed by DN
Date 3/6/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\FEB2502.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\feb2502\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

(X) Full Method

() Reprocessing Only

On A Barcode Mismatch

(X) Inject Anyway

() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0208	
2	Sample	2	CAL25	GCMS0208	
3	Sample	3	LB	GCMS0208	gc/ms scan 1/25
4	Sample	4	REF	GCMS0208	gc/ms scan 1/25
5	Sample	5	1643	GCMS0208	gc/ms scan 1/25
6	Sample	6	1650	GCMS0208	gc/ms scan 1/25
7	Sample	7	1651	GCMS0208	gc/ms scan 1/25
8	Sample	8	1687	GCMS0208	gc/ms scan 1/25
9	Sample	9	1688	GCMS0208	gc/ms scan 1/25
10	Sample	10	1689	GCMS0208	gc/ms scan 1/25
11	Sample	11	1690	GCMS0208	gc/ms scan 1/25
12	Sample	12	1691	GCMS0208	gc/ms scan 1/25
13	Sample	13	1692	GCMS0208	gc/ms scan 1/25
14	Sample	14	1693	GCMS0208	gc/ms scan 1/25
15	Sample	15	1694	GCMS0208	gc/ms scan 1/25
16	Sample	16	1732	GCMS0208	gc/ms scan 1/25
17	Sample	17	LBA	GCMS0208	gc/ms scan 1/25
18	Sample	18	REFA	GCMS0208	gc/ms scan 1/25
19	Sample	19	1733	GCMS0208	gc/ms scan 1/25
20	Sample	20	1734	GCMS0208	gc/ms scan 1/25
21	Sample	21	1735	GCMS0208	gc/ms scan 1/25 fb
22	Sample	22	1796	GCMS0208	gc/ms scan 1/25
23	Sample	23	1797	GCMS0208	gc/ms scan 1/25
24	Sample	24	1798	GCMS0208	gc/ms scan 1/25
25	Sample	25	1799	GCMS0208	gc/ms scan 1/25
26	Sample	1	DFTPP1	GCMS0208	
27	Sample	2	CAL25A	GCMS0208	
28	Sample	26	1800	GCMS0208	gc/ms scan 1/25
29	Sample	27	1801	GCMS0208	gc/ms scan 1/25
30	Sample	28	1802	GCMS0208	gc/ms scan 1/25
31	Sample	29	1803	GCMS0208	gc/ms scan 1/25 fb
32	Sample	30	LBB	GCMS0208	gc/ms scan 1/29
33	Sample	31	REFB	GCMS0208	gc/ms scan 1/29
34	Sample	32	1960	GCMS0208	gc/ms scan 1/29
35	Sample	33	1961	GCMS0208	gc/ms scan 1/29
36	Sample	34	1962	GCMS0208	gc/ms scan 1/29
37	Sample	35	1963	GCMS0208	gc/ms scan 1/29
38	Sample	36	1964	GCMS0208	gc/ms scan 1/29
39	Sample	37	1965	GCMS0208	gc/ms scan 1/29
40	Sample	38	1966	GCMS0208	gc/ms scan 1/29
41	Sample	39	1967	GCMS0208	gc/ms scan 1/29
42	Sample	40	1968	GCMS0208	gc/ms scan 1/29


Last Modified: Tue Feb 26 12:24:47 2002

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB2502\DFTPP.D
 Acq On : 25 Feb 2002 10:41 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

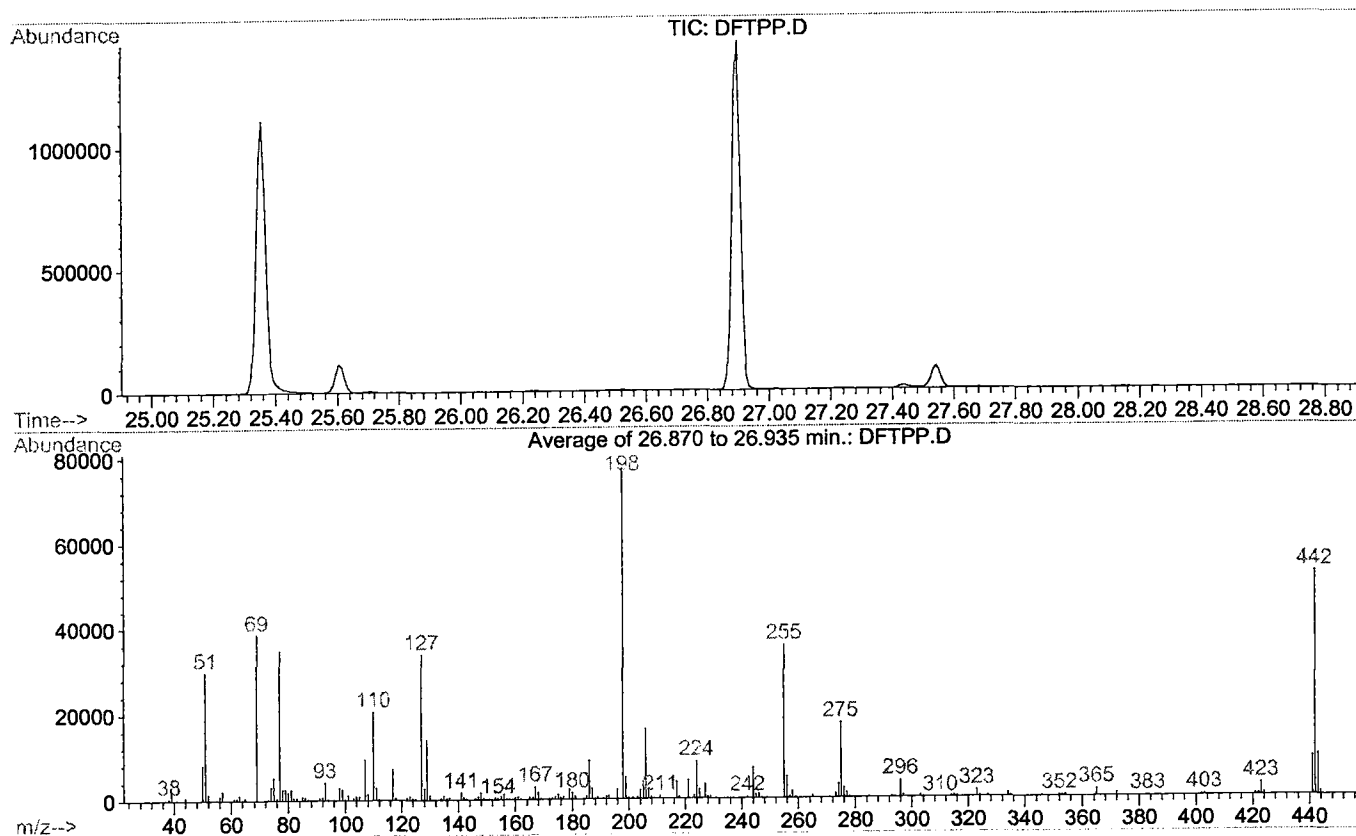

Spectrum Information: Average of 26.870 to 26.935 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	38.7	29889	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.0	38574	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	43.9	33901	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	77178	PASS
199	198	5	9	6.6	5123	PASS
275	198	10	30	22.7	17482	PASS
365	198	1	100	2.4	1860	PASS
441	443	0.01	100	93.7	9178	PASS
442	198	40	110	67.4	52030	PASS
443	442	17	23	18.8	9798	PASS

DFTPP.D GCMS0208.M

Thu Feb 28 11:11:13 2002

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB2502\DFTPP1.D

Acq On : 26 Feb 2002 12:34 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

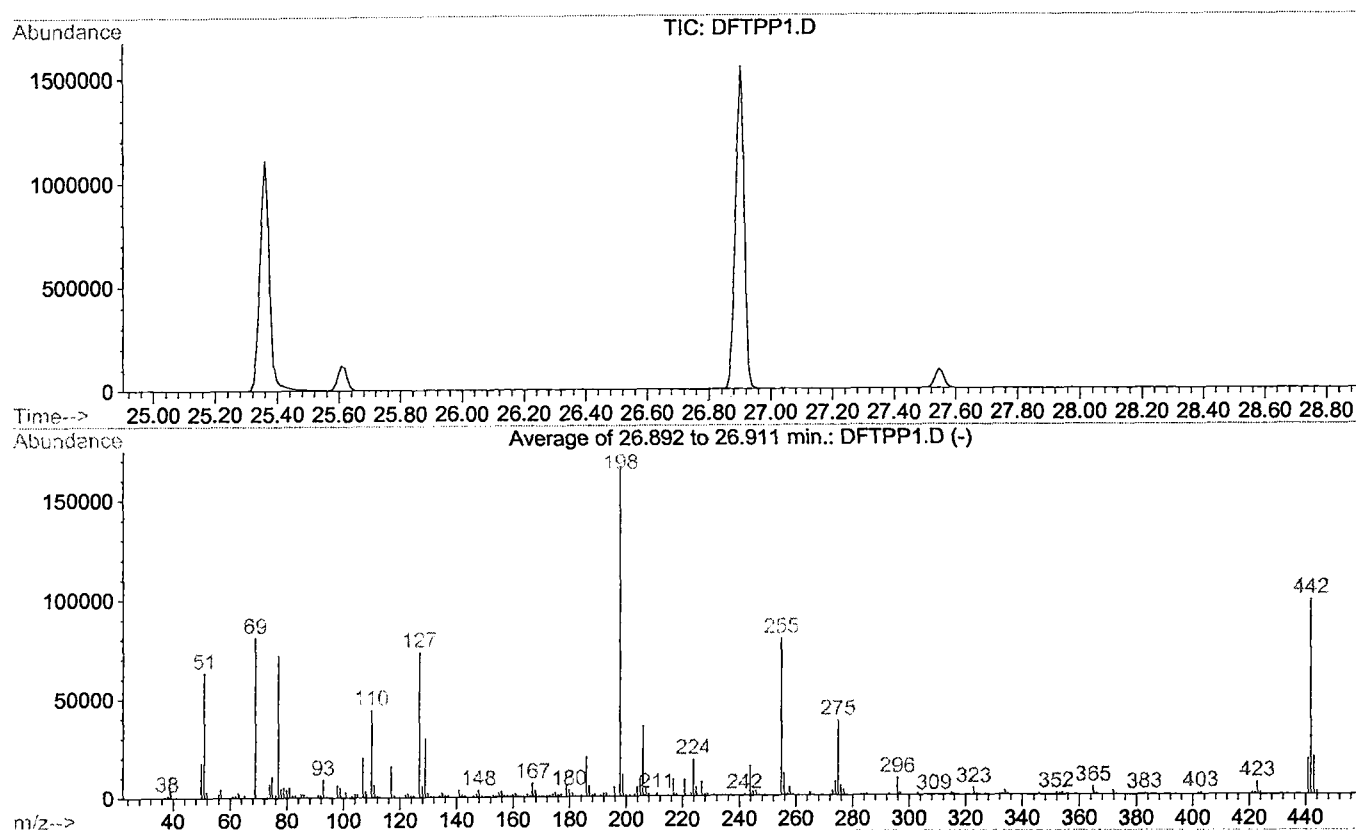

Spectrum Information: Average of 26.892 to 26.911 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	38.1	63291	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.7	81024	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	44.2	73563	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	166251	PASS
199	198	5	9	6.8	11343	PASS
275	198	10	30	23.1	38427	PASS
365	198	1	100	2.4	4049	PASS
441	443	0.01	100	93.7	17882	PASS
442	198	40	110	59.5	98845	PASS
443	442	17	23	19.3	19092	PASS

DFTPP1.D GCMS0208.M

Thu Feb 28 11:11:56 2002