

Sequence Name: C:\HPCHEM\1\SEQUENCE\FEB0802.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\feb0802\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch

(X) Full Method (X) Inject Anyway

() Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------

1	Sample	1	DFTPP	GCMS0103	
2	Sample	2	SURR	GCMS0208	
3	Sample	3	CALCHK	GCMS0208	
4	Sample	4	CAL40	GCMS0208	
5	Sample	5	LB	GCMS0208	GC/MS SCAN 2/8
6	Sample	6	REF	GCMS0208	GC/MS SCAN 2/8
7	Sample	7	31586	GCMS0208	GC/MS SCAN 2/4
8	Sample	8	31640	GCMS0208	GC/MS SCAN 2/4
9	Sample	9	30646	GCMS0208	GC/MS SCAN 2/4
10	Sample	10	00831	GCMS0208	GC/MS SCAN 2/4
11	Sample	11	00845	GCMS0208	GC/MS SCAN 2/4
12	Sample	12	31252	GCMS0208	GC/MS SCAN 2/4
13	Sample	13	31129	GCMS0208	GC/MS SCAN 2/4
14	Sample	14	31132	GCMS0208	GC/MS SCAN 2/4
15	Sample	15	LBA	GCMS0208	GC/MS SCAN 1/28
16	Sample	16	REFA	GCMS0208	GC/MS SCAN 1/28
17	Sample	17	1937	GCMS0208	GC/MS SCAN 1/28
18	Sample	18	1938	GCMS0208	GC/MS SCAN 1/28
19	Sample	19	1939	GCMS0208	GC/MS SCAN 1/28
20	Sample	20	1940	GCMS0208	GC/MS SCAN 1/28
21	Sample	21	1941	GCMS0208	GC/MS SCAN 1/28
22	Sample	22	1942	GCMS0208	GC/MS SCAN 1/28
23	Sample	23	1943	GCMS0208	GC/MS SCAN 1/28
24	Sample	24	28049	GCMS0208	GC/MS SCAN 1/28 FB
25	Sample	25	31341	GCMS0208	RE-EXTRACT 1/28
26	Sample	26	DFTPP1	GCMS0208	
27	Sample	27	CAL40A	GCMS0208	
28	Sample	28	LBB	GCMS0208	GC/MS SCAN 2/7
29	Sample	29	REFB	GCMS0208	GC/MS SCAN 2/7
30	Sample	30	2966	GCMS0208	GC/MS SCAN 2/7
31	Sample	31	2967	GCMS0208	GC/MS SCAN 2/7
32	Sample	32	2968	GCMS0208	GC/MS SCAN 2/7
33	Sample	33	2969	GCMS0208	GC/MS SCAN 2/7
34	Sample	34	2970	GCMS0208	GC/MS SCAN 2/7
35	Sample	35	2971	GCMS0208	GC/MS SCAN 2/7
36	Sample	36	2972	GCMS0208	GC/MS SCAN 2/7
37	Sample	37	2973	GCMS0208	GC/MS SCAN 2/7FB
38	Sample	38	3014	GCMS0208	GC/MS SCAN 2/7
39	Sample	39	3015	GCMS0208	GC/MS SCAN 2/7
40	Sample	40	31344	GCMS0208	RE-EXTRACT 2/7
41	Sample	41	31136	GCMS0208	RE-EXTRACT 2/7 FB
42	Sample	42	LBC	GCMS0208	GC/MS SCAN 2/8

Last Modified: Fri Feb 08 16:33:57 2002

Page: 1

43 Sample

43 REFC

GCMS0208 GC/MS SCAN 2/8

Sequence Name: C:\HPCHEM\1\SEQUENCE\FEB0802.S

Line	Type	Vial	DataFile	Method	Sample Name
44	Sample	44	REFC2	GCMS0208 GC/MS	SCAN 2/8
45	Sample	45	30641	GCMS0208 GC/MS	SCAN 2/8
46	Sample	46	30650	GCMS0208 GC/MS	SCAN 2/8
47	Sample	47	30649	GCMS0208 GC/MS	SCAN 2/8
48	Sample	48	30651	GCMS0208 GC/MS	SCAN 2/8
49	Sample	49	30703	GCMS0208 GC/MS	SCAN 2/8
50	Sample	26	DFTPP2	GCMS0208	
51	Sample	27	CAL40B	GCMS0208	
52	Sample	50	30707	GCMS0208 GC/MS	SCAN 2/8
53	Sample	51	30708	GCMS0208 GC/MS	SCAN 2/8
54	Sample	52	30709	GCMS0208 GC/MS	SCAN 2/8
55	Sample	53	30710	GCMS0208 GC/MS	SCAN 2/8
56	Sample	54	31464	GCMS0208 GC/MS	SCAN 2/8

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB0802\DFTPP.D

Acq On : 8 Feb 2002 9:14 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

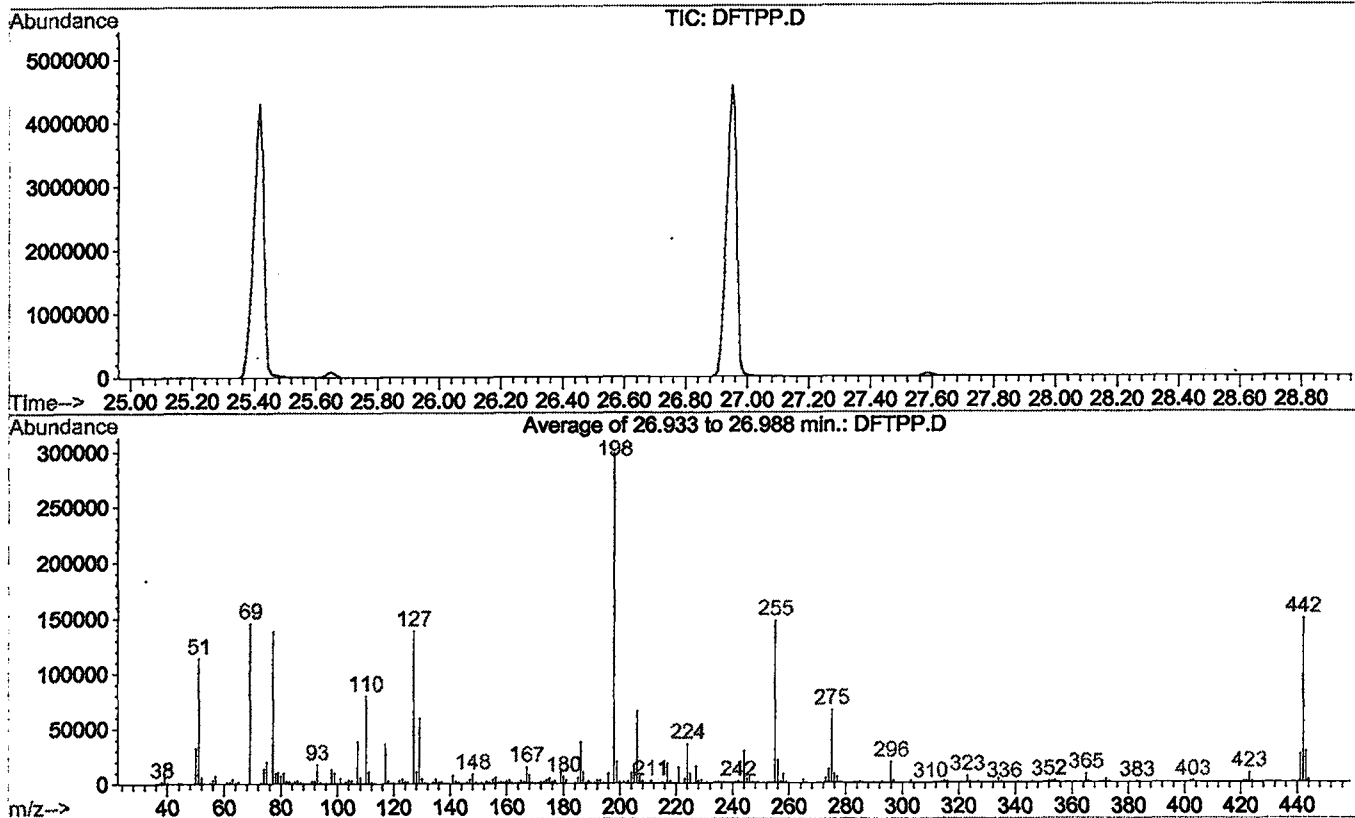

Spectrum Information: Average of 26.933 to 26.988 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	38.2	113807	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.0	146046	PASS
70	69	0.00	2	0.1	125	PASS
127	198	40	60	46.6	138906	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	298168	PASS
199	198	5	9	6.7	19968	PASS
275	198	10	30	22.4	66806	PASS
365	198	1	100	2.7	8159	PASS
441	443	0.01	100	91.7	26161	PASS
442	198	40	110	50.0	149137	PASS
443	442	17	23	19.1	28528	PASS