

NYC-WTC_000005355

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAR0702.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\MAR0702\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch

(X) Full Method (X) Inject Anyway

() Reprocessing Only () Don't Inject


Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------

1	Sample	1	DFTPP	GCMS0208	
2	Sample	2	CAL5	GCMS0208	
3	Sample	3	CAL10	GCMS0208	
4	Sample	4	CAL25	GCMS0208	
5	Sample	5	CAL40	GCMS0208	
6	Sample	6	CAL80	GCMS0208	
7	Sample	7	CAL100	GCMS0208	
8	Sample	8	B5	GCMS0208	
9	Sample	9	B10	GCMS0208	
10	Sample	10	B25	GCMS0208	
11	Sample	11	B40	GCMS0208	
12	Sample	12	B80	GCMS0208	
13	Sample	13	B100	GCMS0208	
14	Sample	14	SURR	GCMS0208	
15	Sample	15	LB	GCMS0208	gc/ms scan 2/5
16	Sample	16	REF	GCMS0208	gc/ms scan 2/5
17	Sample	17	2604	GCMS0208	gc/ms scan 2/5 fb
18	Sample	18	2645	GCMS0208	gc/ms scan 2/5
19	Sample	19	2646	GCMS0208	gc/ms scan 2/5
20	Sample	20	2647	GCMS0208	gc/ms scan 2/5
21	Sample	21	2710	GCMS0208	gc/ms scan 2/5
22	Sample	22	2711	GCMS0208	gc/ms scan 2/5
23	Sample	23	2712	GCMS0208	gc/ms scan 2/5
24	Sample	24	2581	GCMS0208	re-extract

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR0702\DFTPP.D
 Acq On : 7 Mar 2002 1:43 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

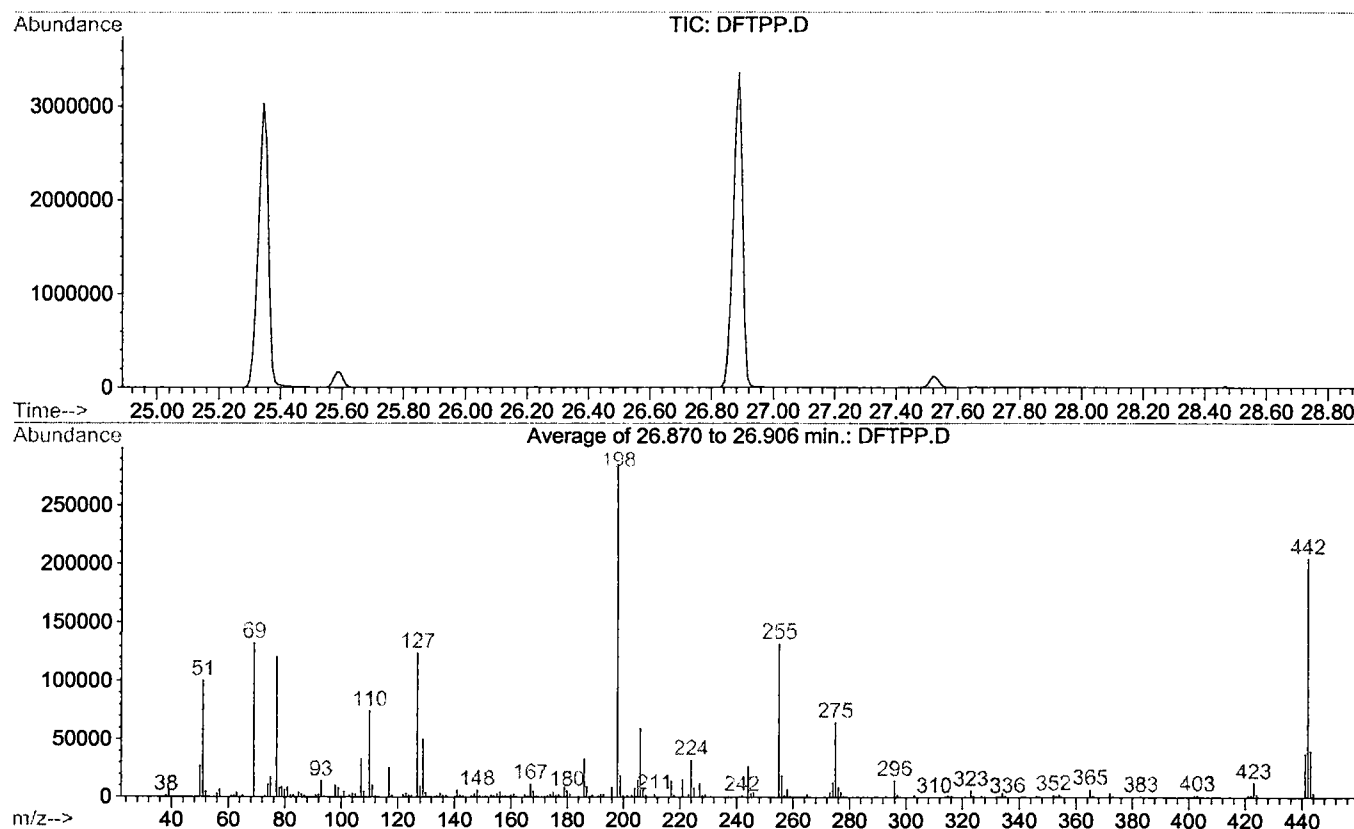

Spectrum Information: Average of 26.870 to 26.906 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.3	100574	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.5	132605	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	43.5	123966	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	285003	PASS
199	198	5	9	6.6	18724	PASS
275	198	10	30	22.6	64458	PASS
365	198	1	100	2.4	6887	PASS
441	443	0.01	100	93.8	37456	PASS
442	198	40	110	71.8	204600	PASS
443	442	17	23	19.5	39922	PASS