

Method 508 modified Date Extracted 2/6/02Page 72

REF

#GCM S - 17225

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	SpK add	IS add	Final vol.	T.V. pos.	pH	Count											
LB		500ml		1ml			1ml	6B	7												
REF					5ml			9A													
2701								10B													
2783								7B													
2784								8A													
2785								9B													
2786								8B													
2787								7A													
2788								6A													
2789	FB							10A													
27																					
Remarks																					
Reviewed by, <u>JOS 5/27/02</u>																					
drip rate must be between 5-15 ml/min for liq-liq extractors																					
drip rate -																					
Extraction type <u>Sep Fun</u>		Solv. lot# <u>V41470</u>		NaCl lot# <u>V39618</u>		Na2SO4 lot# <u>V39400</u>															
STANDARD	INT STD LOG#																				
CALIBRATION	<u>HP 01300v</u>																				
REF SPIKE	<u>91759</u>																				
MDL/MDRF																					
Q. CHECK																					
INT. STD.	<u>022702</u>																				
SURROGATE	<u>GEMS 020102</u>																				
LPC																					
ENDRIN/DDT																					

Analyst EA
Revision 4/12/01Verified by naReviewed by DW
Date 3/11/02

Sequence Name: C:\HPCHEM\1\DATA\MAR0102\

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\MAR0102\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

(X) Full Method

(X) Inject Anyway

() Reprocessing Only

() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------

1	Sample	1	DFTPP	GCMS0208	
2	Sample	2	CAL10	GCMS0208	
3	Sample	3	LB	GCMS0208	gc/ms scan 2/5
4	Sample	4	REF	GCMS0208	gc/ms scan 2/5
5	Sample	5	2595	GCMS0208	gc/ms scan 2/5
6	Sample	6	2596	GCMS0208	gc/ms scan 2/5
7	Sample	7	2597	GCMS0208	gc/ms scan 2/5
8	Sample	8	2598	GCMS0208	gc/ms scan 2/5
9	Sample	9	2599	GCMS0208	gc/ms scan 2/5
10	Sample	10	2600	GCMS0208	gc/ms scan 2/5
11	Sample	11	2601	GCMS0208	gc/ms scan 2/5 fb
12	Sample	12	2602	GCMS0208	gc/ms scan 2/5
13	Sample	13	2603	GCMS0208	gc/ms scan 2/5
14	Sample	14	LBA	GCMS0208	gc/ms scan 2/6
15	Sample	15	REFA	GCMS0208	gc/ms scan 2/6
16	Sample	16	2761	GCMS0208	gc/ms scan 2/6
17	Sample	17	2783	GCMS0208	gc/ms scan 2/6
18	Sample	18	2784	GCMS0208	gc/ms scan 2/6
19	Sample	19	2785	GCMS0208	gc/ms scan 2/6
20	Sample	20	2786	GCMS0208	gc/ms scan 2/6
21	Sample	21	2787	GCMS0208	gc/ms scan 2/6
22	Sample	22	2788	GCMS0208	gc/ms scan 2/6
23	Sample	23	2789	GCMS0208	gc/ms scan 2/6 fb
24	Sample	1	DFTPP2	GCMS0208	
25	Sample	2	CAL10A	GCMS0208	
26	Sample	24	LBB	GCMS0208	gc/ms scan 2/12
27	Sample	25	REF1	GCMS0208	gc/ms scan 2/12
28	Sample	26	REF2	GCMS0208	gc/ms scan 2/12
29	Sample	27	3075	GCMS0208	gc/ms scan 2/12
30	Sample	28	3076	GCMS0208	gc/ms scan 2/12
31	Sample	29	3077	GCMS0208	gc/ms scan 2/12
32	Sample	30	3078	GCMS0208	gc/ms scan 2/12
33	Sample	31	3178	GCMS0208	gc/ms scan 2/12
34	Sample	32	3179	GCMS0208	gc/ms scan 2/12
35	Sample	33	3180	GCMS0208	gc/ms scan 2/12
36	Sample	34	3181	GCMS0208	gc/ms scan 2/12
37	Sample	35	3182	GCMS0208	gc/ms scan 2/12
38	Sample	36	3183	GCMS0208	gc/ms scan 2/12
39	Sample	1	DFTPP3	GCMS0208	
40	Sample	2	CAL10B	GCMS0208	
41	Sample	37	LBC	GCMS0208	gc/ms scan 2/4
42	Sample	38	REFC	GCMS0208	gc/ms scan 2/4


Last Modified: Sat Mar 02 13:23:03 2002

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR0102\DFTPP.D
 Acq On : 1 Mar 2002 8:21 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0305.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

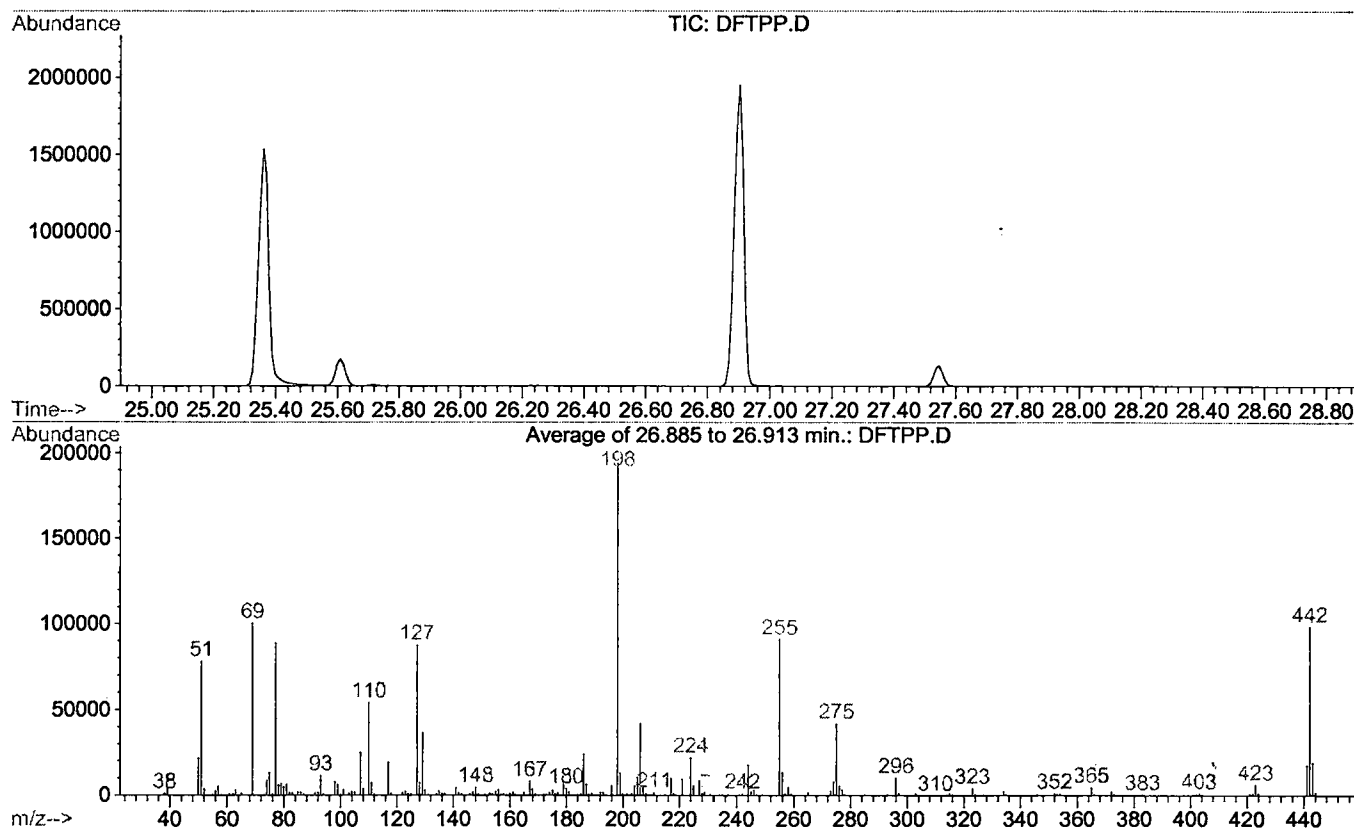

Spectrum Information: Average of 26.885 to 26.913 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	40.3	78150	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	51.8	100470	PASS
70	69	0.00	2	0.1	122	PASS
127	198	40	60	45.2	87670	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	193782	PASS
199	198	5	9	6.8	13100	PASS
275	198	10	30	21.7	42126	PASS
365	198	1	100	2.4	4688	PASS
441	443	0.01	100	93.4	17728	PASS
442	198	40	110	50.8	98494	PASS
443	442	17	23	19.3	18973	PASS

DFTPP.D GCMS0305.M Tue Mar 05 10:18:24 2002