

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 03/11/2002 Time: 16:03:39

Sample: AE02784
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 3/11/02 16:03 Ended: 3/11/02 16:03 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		112		5.0

Comments for Sample AE02784 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-11-2002 Time: 16:03:43

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

The recovery for 1 of the 43 compounds in the LCS Standard was below its acceptance range.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR0102\2784.D

Vial: 18

Acq On : 2 Mar 2002 1:05 am

Operator:

Sample : gc/ms scan 2/6

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 5 10:32 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 27 11:30:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.31	152	319913	20.00	ug/l	-0.04
10) Naphthalene-d8	15.95	136	1244134	20.00	ug/l	-0.04
17) Acenaphthene-d10	21.27	164	659118	20.00	ug/l	-0.04
29) Phenanthrene-d10	25.71	188	948935	20.00	ug/l	-0.05
38) Chrysene-d12	33.78	240	662153	20.00	ug/l	-0.06
44) Perylene-d12	38.05	264	456363	20.00	ug/l	-0.07

System Monitoring Compounds

37) 2,4-DDD	30.79	235	55730	5.62	ug/mL	0.29
Spiked Amount	5.000		Recovery	=	112.40%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	16.02	128	495	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	22.74	149	404	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#) = qualifier out of range (m) = manual integration

2784.D GCMS0208.M Tue Mar 05 10:32:59 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR0102\2784.D

Vial: 18

Acq On : 2 Mar 2002 1:05 am

Operator:

Sample : gc/ms scan 2/6

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 5 10:32 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 27 11:30:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	27.69	149	14550	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.78	228	1505	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.98	149	1357	N.D.		
43) Chrysene	33.78	228	1505	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.05	252	1721	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

2784.D GCMS0208.M Tue Mar 05 10:33:03 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAR0102\2784.D
Acq On : 2 Mar 2002 1:05 am
Sample : gc/ms scan 2/6
Misc :
MS Integration Params: GOOFY.P
Quant Time: Mar 5 10:32 2002

Vial: 18
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 27 11:30:15 2002
Response via : Initial Calibration

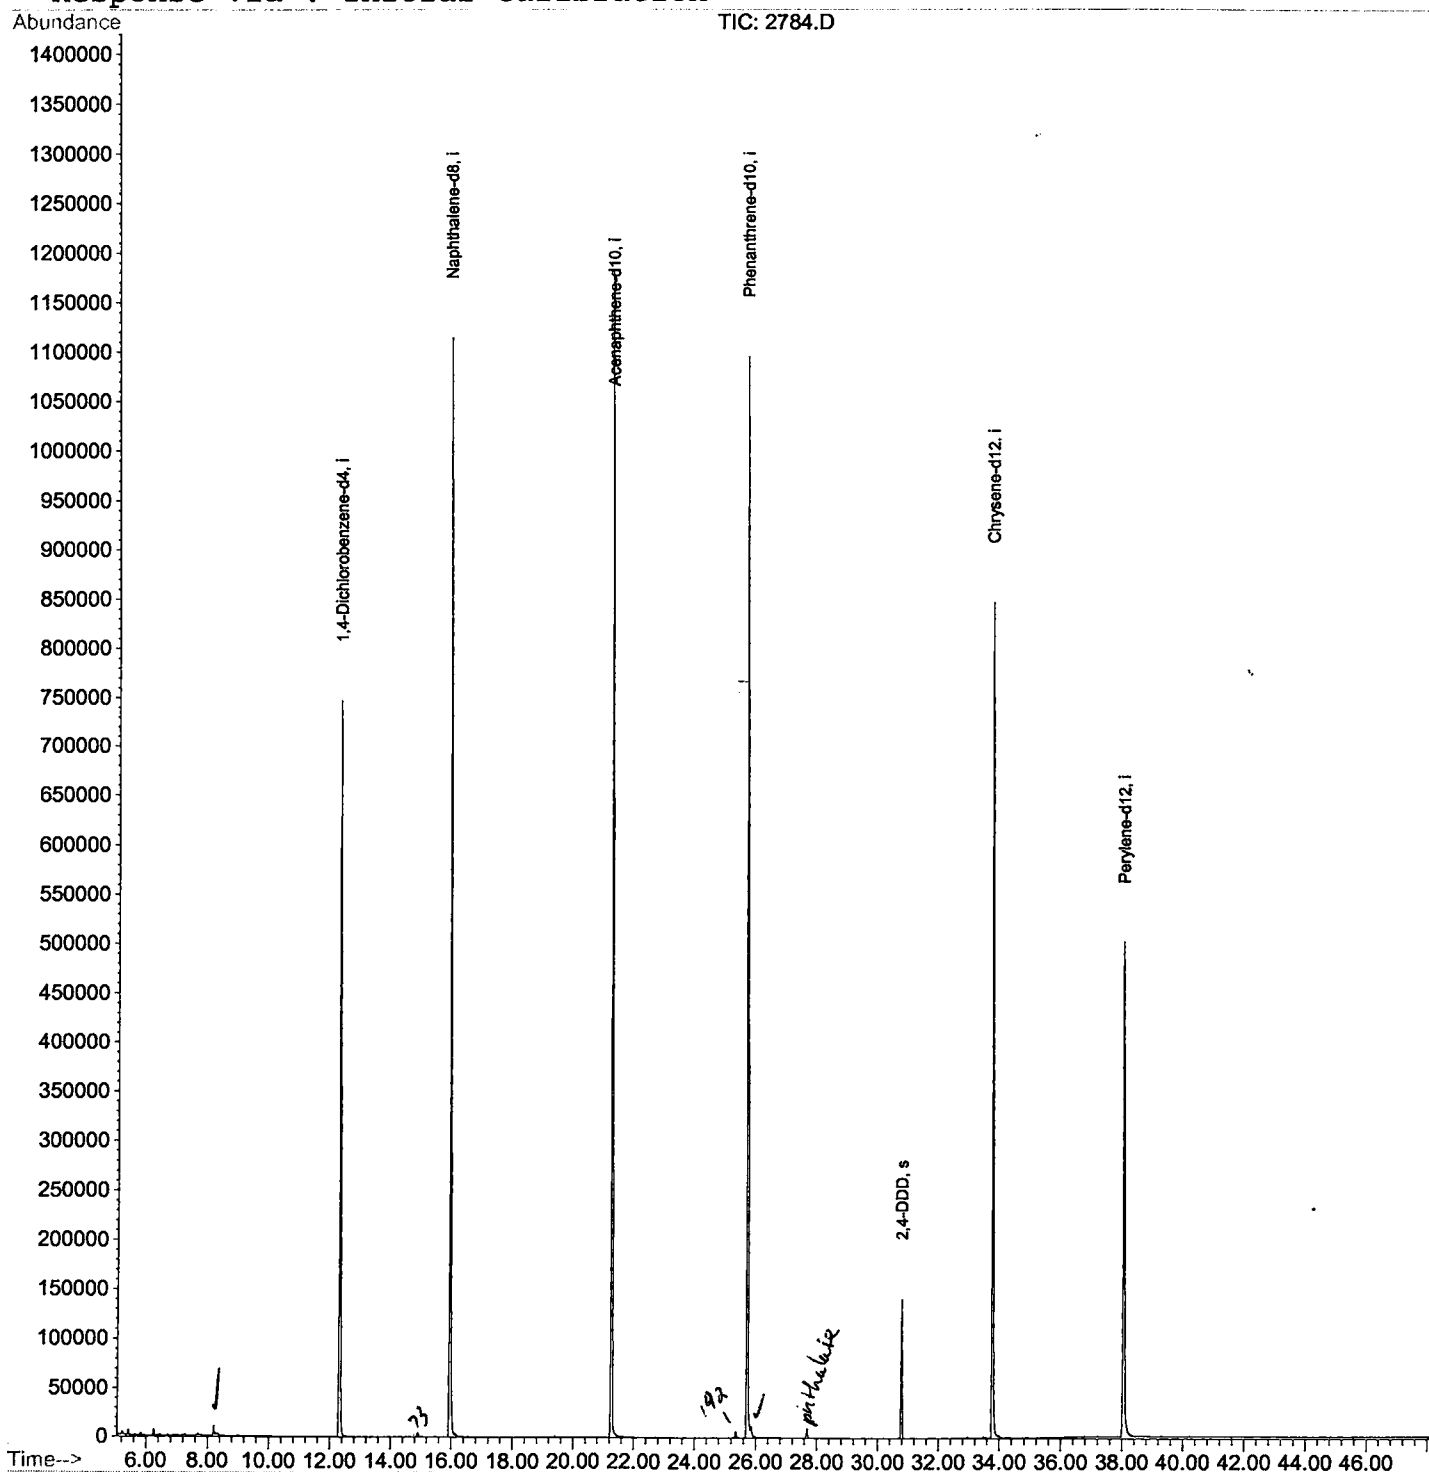

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAR0102\2784.D

Vial: 18

Acq On : 2 Mar 2002 1:05 am

Operator:

Sample : gc/ms scan 2/6

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.197	338	344	351	rBV	10421	26222	1.00%	0.197%
2	12.310	787	792	808	rBV	746729	1815281	69.57%	13.661%
3	15.954	1183	1189	1206	rBV	1114454	2417284	92.65%	18.192%
4	21.270	1761	1768	1788	rBV	1183239	2609170	100.00%	19.636%
5	25.713	2245	2252	2264	rBV2	1095987	2493561	95.57%	18.766%
6	25.851	2264	2267	2274	rVB	10056	26783	1.03%	0.202%
7	30.790	2800	2805	2814	rVB	141596	286058	10.96%	2.153%
8	33.783	3124	3131	3148	rBV2	847620	2005601	76.87%	15.093%
9	38.051	3585	3596	3617	rBV2	501283	1607957	61.63%	12.101%




Sum of corrected areas: 13287917

2784.D GCMS0208.M

Tue Mar 05 10:47:55 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAR0102\2784.D
 Operator :
 Acquired : 2 Mar 2002 1:05 am using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 2/6
 Misc Info :
 Vial Number: 18
 Quant File :GCMS0208.RES (RTE Integrator)

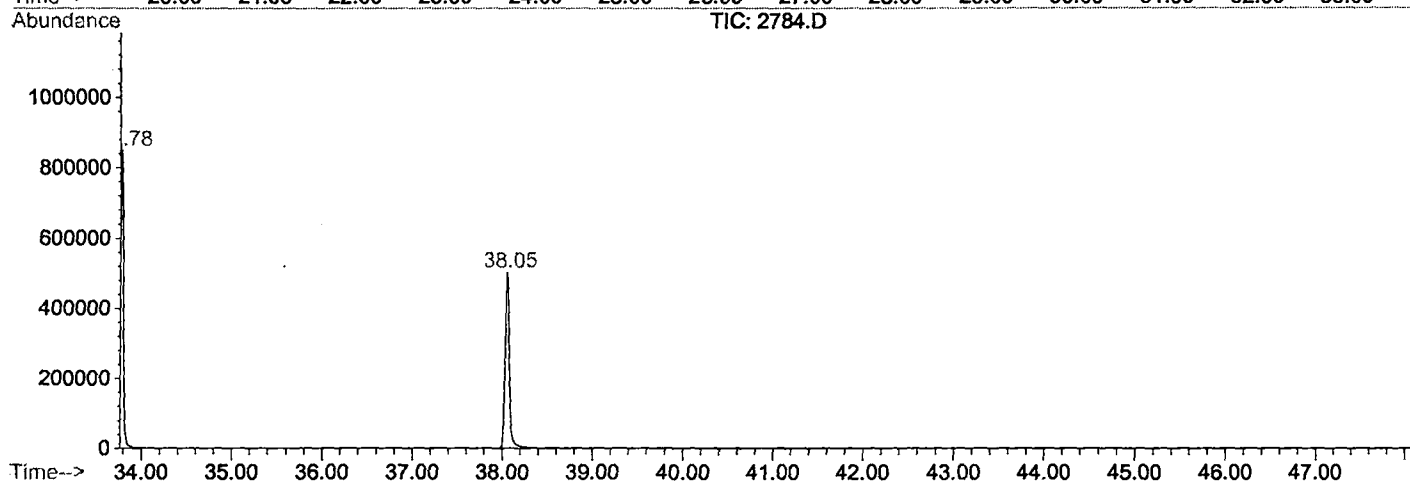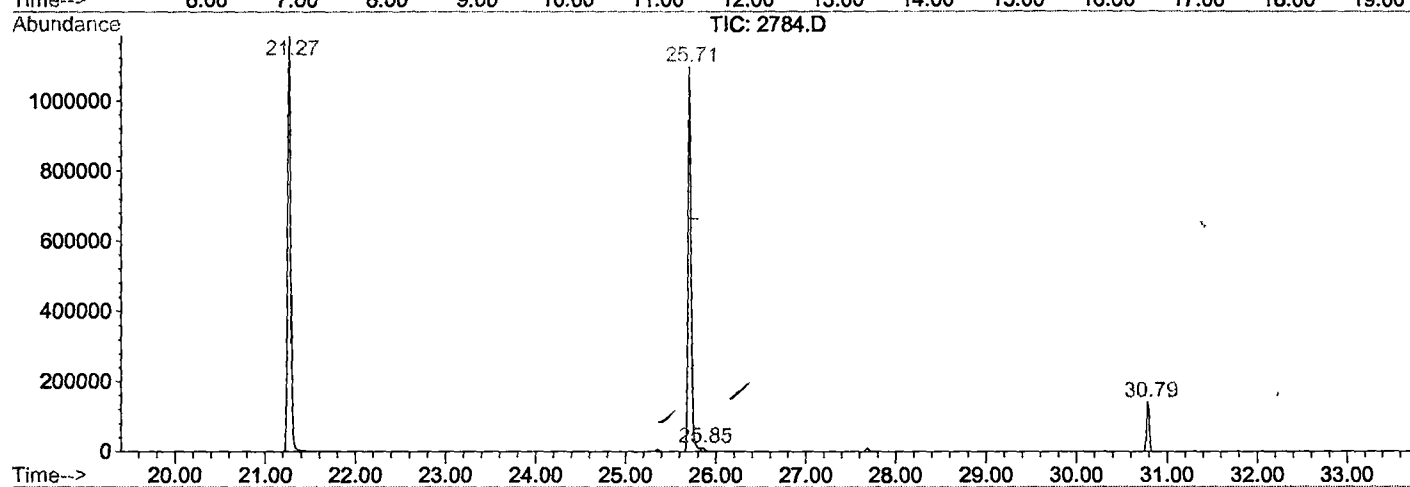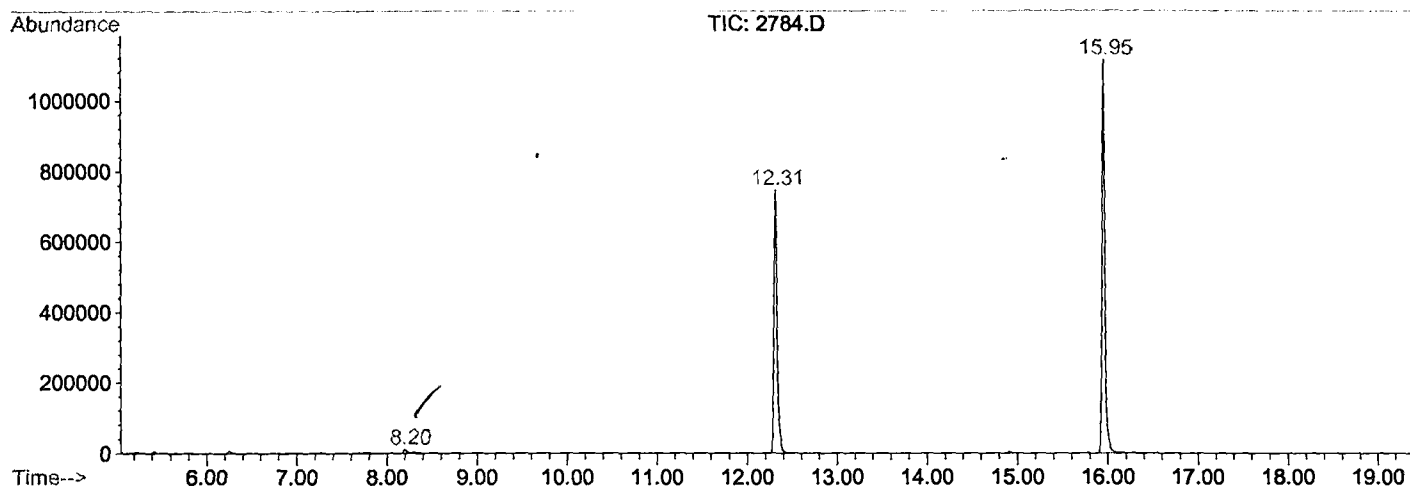

2784.D GCMS0208.M Tue Mar 05 10:48:01 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR0102\2784.D
 Acq On : 2 Mar 2002 1:05 am
 Sample : gc/ms scan 2/6
 Misc :
 MS Integration Params: LSCINT.P








Vial: 18
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 1,3-Dioxolane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.20	0.29 ug/l	26222	1,4-Dichlorobenzene-d4	12.31

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Dioxolane	74	C3H6O2	000646-06-0	7
2		N-Ethylformamide	73	C3H7NO	000627-45-2	5
3		Formamide, N,N-dimethyl-	73	C3H7NO	000068-12-2	5
4		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	4

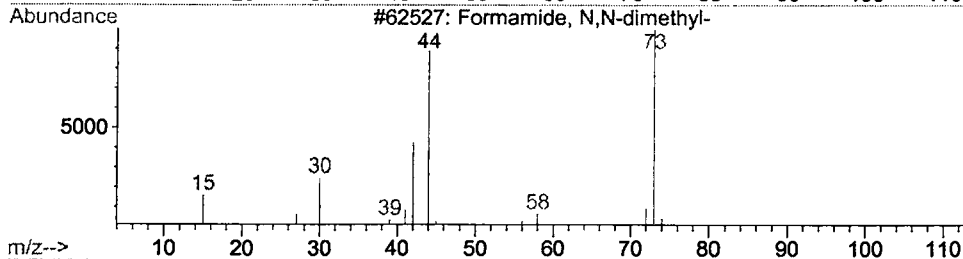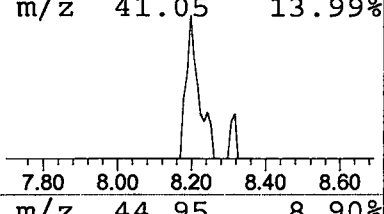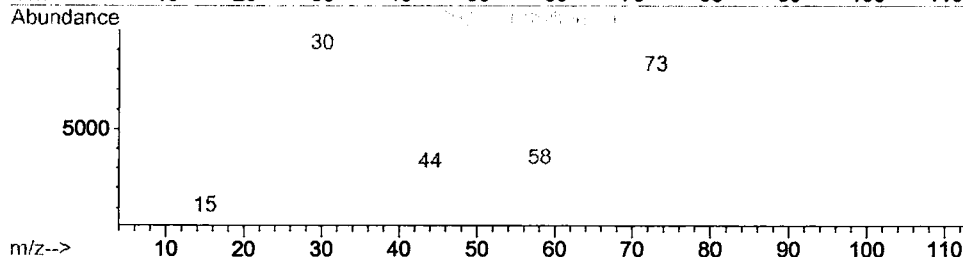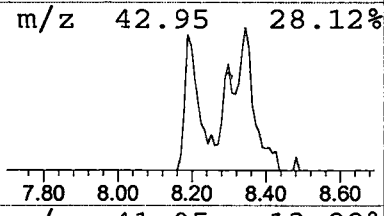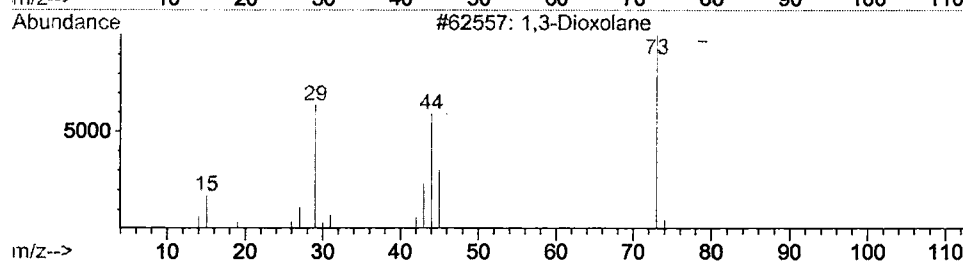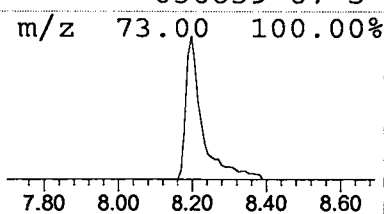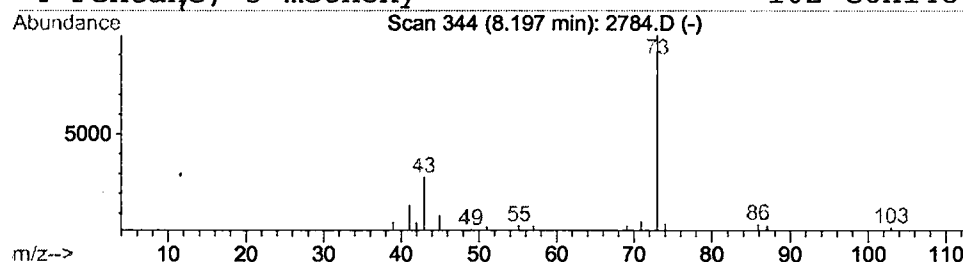

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR0102\2784.D
 Acq On : 2 Mar 2002 1:05 am
 Sample : gc/ms scan 2/6
 Misc :
 MS Integration Params: LSCINT.P


Vial: 18
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Anthracene-d10- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.85	0.21 ug/l	26783	Phenanthrene-d10	25.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Anthracene-d10-	188	C14D10	001719-06-8	72
2		Phenanthrene-d10	188	C14D10	001517-22-2	64
3		Naphthalene, 1,7-dimethoxy-	188	C12H12O2	005309-18-2	42
4		2-Quinolinecarboxaldehyde, 8-hydrox	188	C10H8N2O2	005603-22-5	40

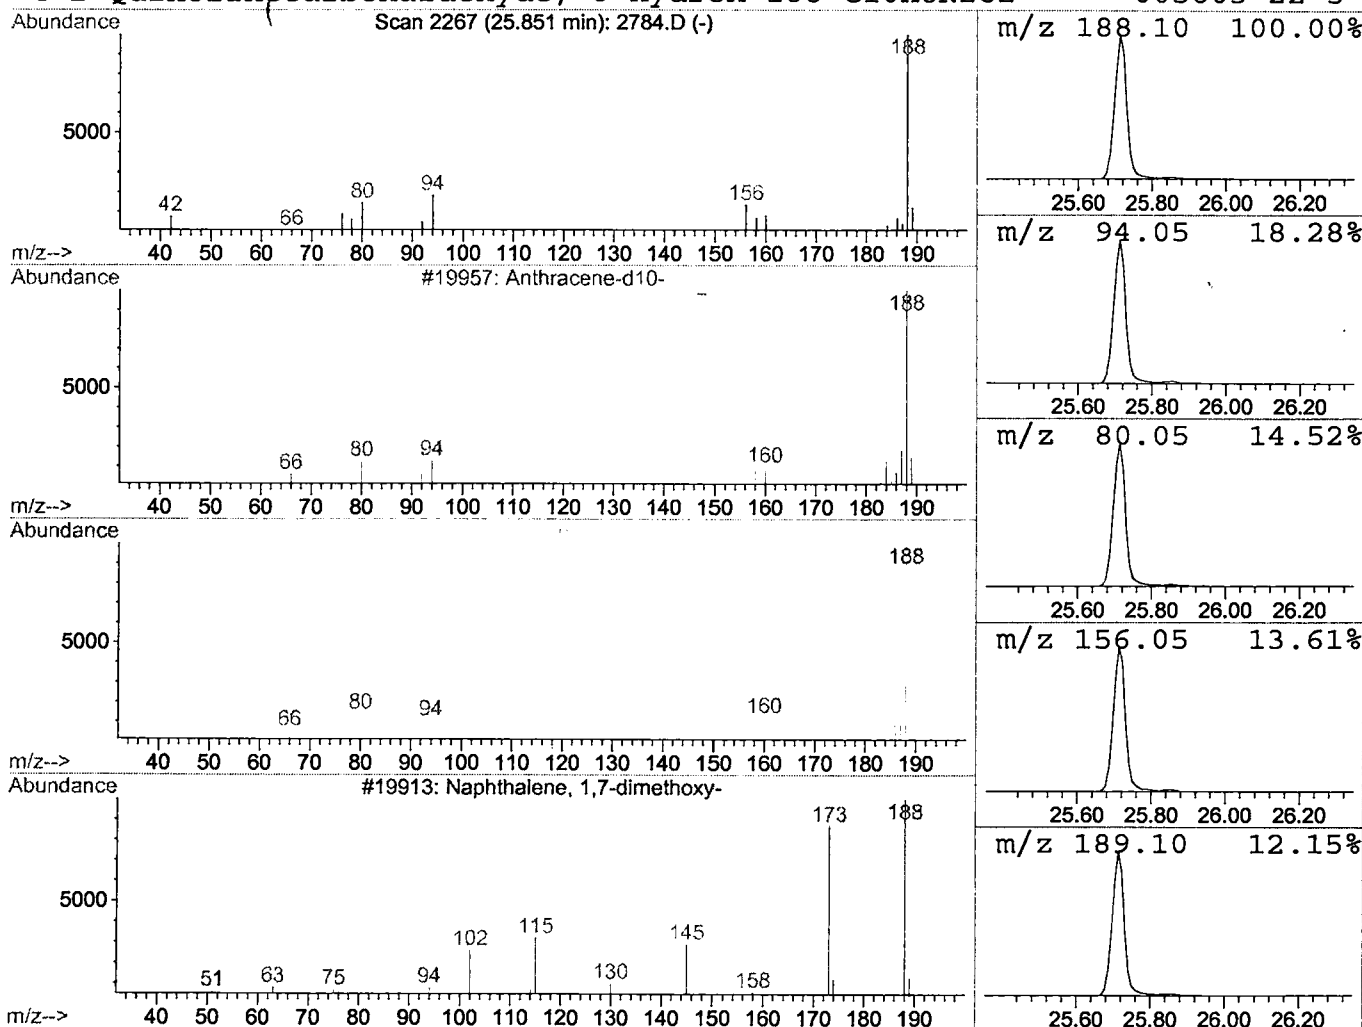

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 2 Mar 2002 1:05 am

Data File: C:\HPCHEM\1\DATA\MAR0102\2784.D

Name: gc/ms scan 2/6

Misc:

Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title: 209 625/TCLP calibration table

Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc Units	Area	IntStd	ISRT	ISArea	ISConc
1,3-Dioxolane	8.20	0.3 ug/l	26222	ISTD01	12.31	1815280	20.0
Anthracene-d10-	25.85	0.2 ug/l	26783	ISTD04	25.71	2493560	20.0

2784.D GCMS0208.M Tue Mar 05 10:48:14 2002