

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 03/11/2002 Time: 16:06:43

Sample: AE02786
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 3/11/02 16:06 Ended: 3/11/02 16:06 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		105		5.0

Comments for Sample AE02786 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-11-2002 Time: 16:06:48

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

The recovery for 1 of the 43 compounds in the LCS Standard was below its acceptance range.

Data File : C:\HPCHEM\1\DATA\MAR0102\2786.D

Vial: 20

Acq On : 2 Mar 2002 3:02 am

Operator:

Sample : gc/ms scan 2/6

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 5 10:38 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 27 11:30:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.32	152	314103	20.00	ug/l	-0.04
10) Naphthalene-d8	15.95	136	1232626	20.00	ug/l	-0.05
17) Acenaphthene-d10	21.27	164	657511	20.00	ug/l	-0.05
29) Phenanthrene-d10	25.72	188	956859m	20.00	ug/l	-0.05
38) Chrysene-d12	33.78	240	669682	20.00	ug/l	-0.07
44) Perylene-d12	38.06	264	460315	20.00	ug/l	-0.07

System Monitoring Compounds

37) 2,4-DDD	30.80	235	52434	5.25	ug/mL	0.30
Spiked Amount	5.000		Recovery	=	105.00%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	16.01	128	493	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	22.74	149	389	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)=qualifier out of range (m)=manual integration

2786.D GCMS0208.M Tue Mar 05 10:39:12 2002

Page 1

Data File : C:\HPCHEM\1\DATA\MAR0102\2786.D

Vial: 20

Acq On : 2 Mar 2002 3:02 am

Operator:

Sample : gc/ms scan 2/6

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 5 10:38 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 27 11:30:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	27.68	149	17384	N.D.		
36) Fluoranthene	29.44	202	188	N.D.		
39) Pyrene	30.11	202	335	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.79	228	1599	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.99	149	1754	N.D.		
43) Chrysene	33.79	228	1600	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.05	252	1644	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

2786.D GCMS0208.M Tue Mar 05 10:39:15 2002

Page 2


QUANTIFICATION REPORT

Data File : C:\HPCHEM\1\DATA\MAR0102\2786.D
Acq On : 2 Mar 2002 3:02 am
Sample : gc/ms scan 2/6
Misc :
MS Integration Params: GOOFY.P
Quant Time: Mar 5 10:38 2002

Vial: 20
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 27 11:30:15 2002
Response via : Initial Calibration

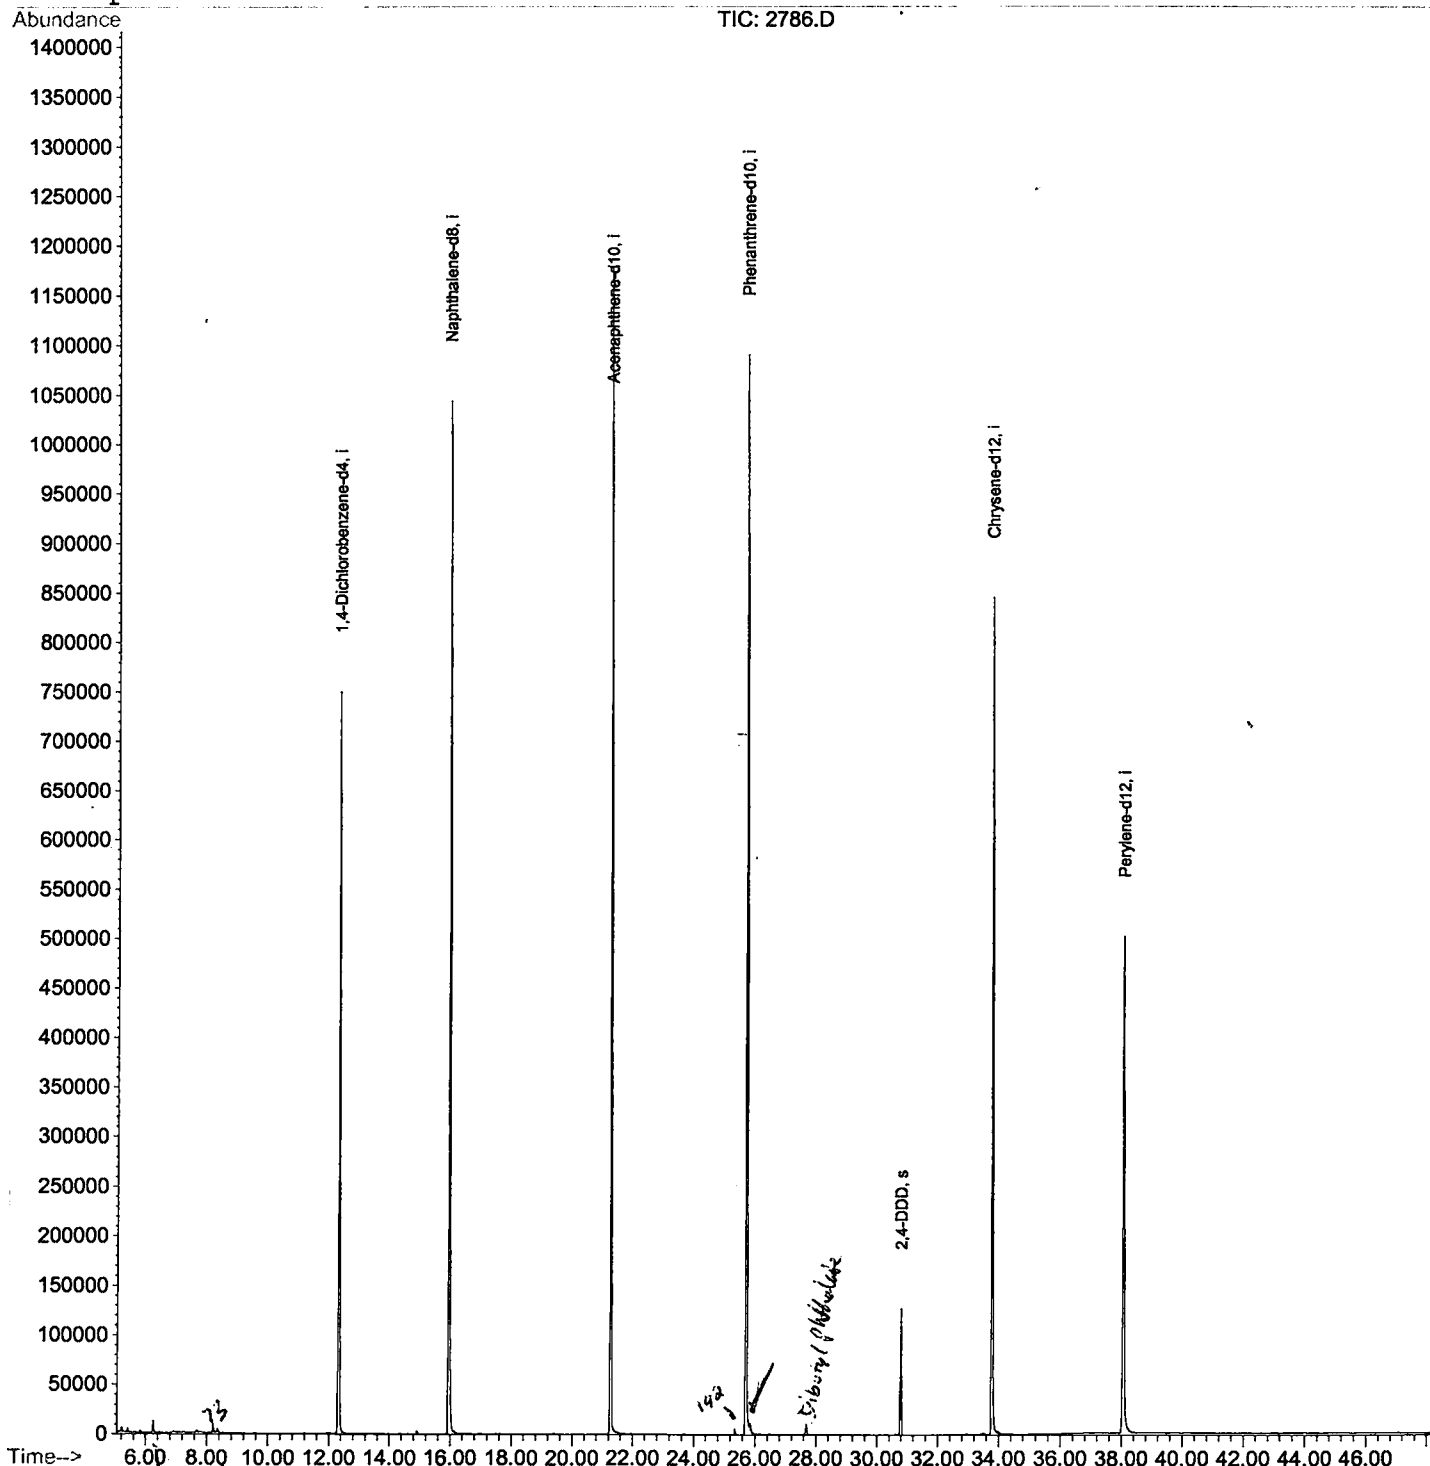

2786.D GCMS0208.M

Tue Mar 05 10:39:22 2002

Page 3

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAR0102\2786.D
Acq On : 2 Mar 2002 3:02 am
Sample : gc/ms scan 2/6
Misc :
MS Integration Params: LSCINT.P

Vial: 20
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.315	786	792	814	rVB	749294	1772873	68.99%	13.427%
2	15.950	1182	1188	1204	rBV	1043578	2385283	92.83%	18.065%
3	21.266	1761	1767	1780	rBV	1179166	2569573	100.00%	19.460%
4	25.718	2245	2252	2263	rBV2	1090617	2510577	97.70%	19.014%
5	25.856	2263	2267	2274	rVB	10057	30848	1.20%	0.234%
6	30.795	2800	2805	2813	rBV	127734	271670	10.57%	2.057%
7	33.779	3123	3130	3149	rBV2	845371	2038517	79.33%	15.438%
8	38.057	3587	3596	3613	rBV2	500752	1624794	63.23%	12.305%

Sum of corrected areas: 13204135

2786.D GCMS0208.M Tue Mar 05 10:51:44 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAR0102\2786.D
 Operator :
 Acquired : 2 Mar 2002 3:02 am using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 2/6
 Misc Info :
 Vial Number: 20
 Quant File :GCMS0208.RES (RTE Integrator)

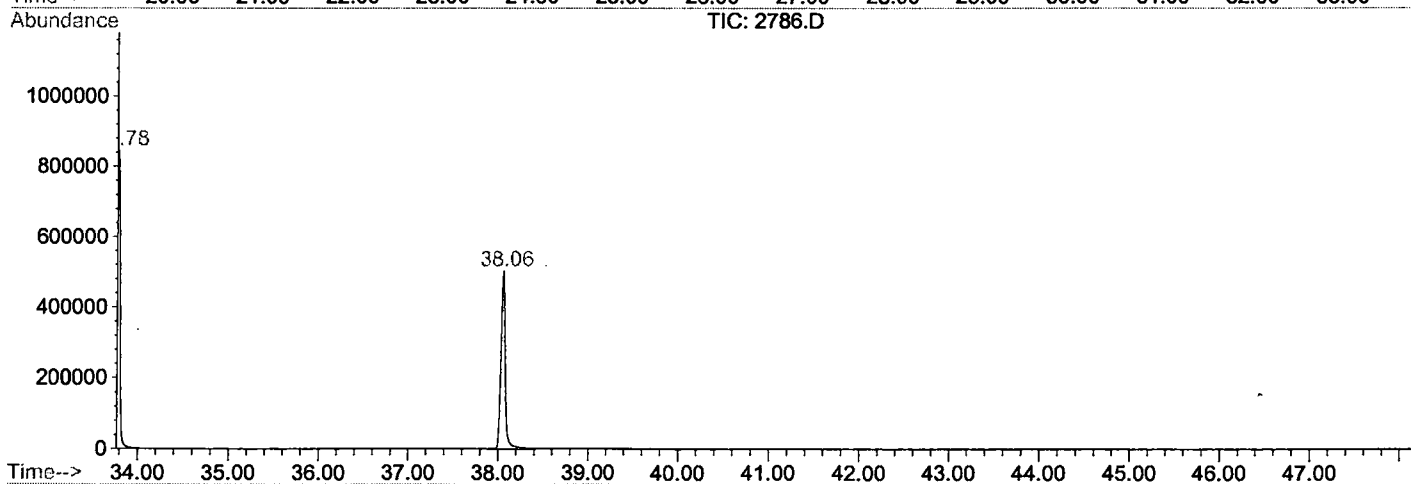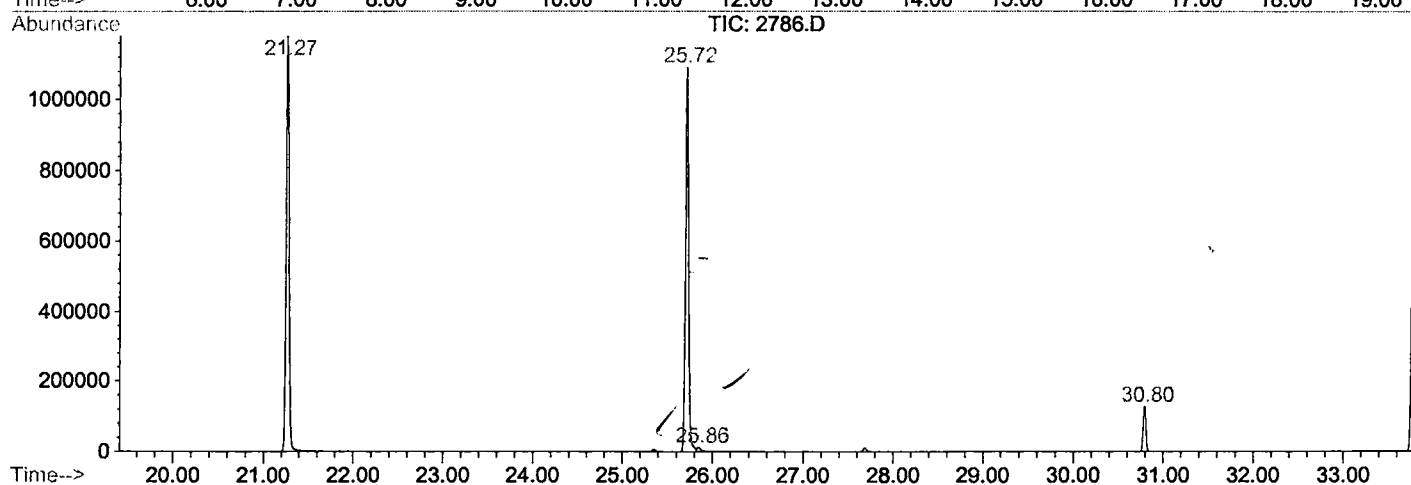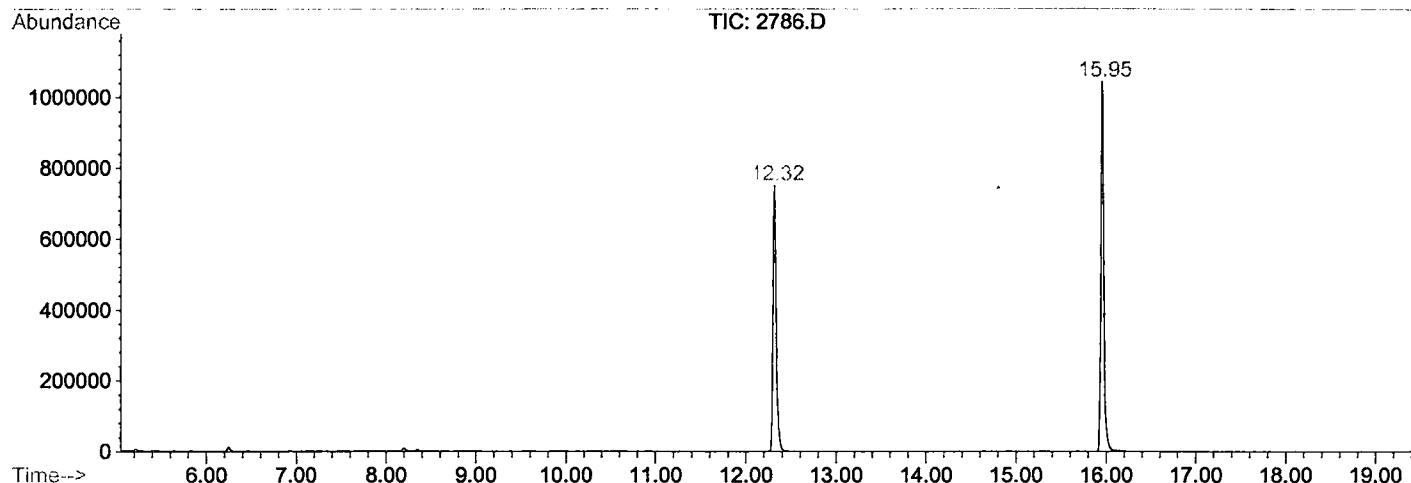

2786.D GCMS0208.M

Tue Mar 05 10:51:50 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR0102\2786.D
 Acq On : 2 Mar 2002 3:02 am
 Sample : gc/ms scan 2/6
 Misc :
 MS Integration Params: LSCINT.P










Vial: 20
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 Naphthalene, 1,7-dimethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.86	0.25 ug/l	30848	Phenanthrene-d10	25.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Naphthalene, 1,7-dimethoxy-	188	C12H12O2	005309-18-2	45
2		4-Fluoro-6-methyl-2-phenylpyrimidin	188	C11H9FN2	000000-00-0	42
3		Phenanthrene-d10	188	C14D10	001517-22-2	40
4		Anthracene-d10-	188	C14D10	001719-06-8	39

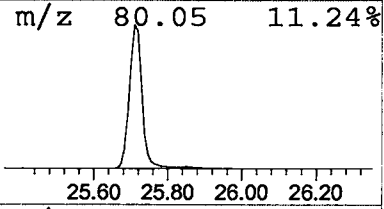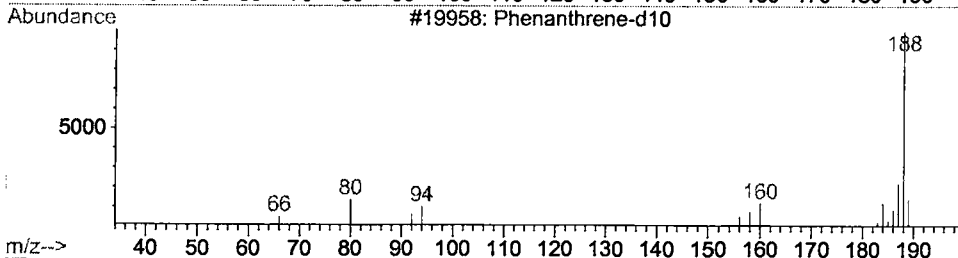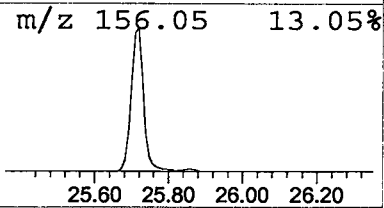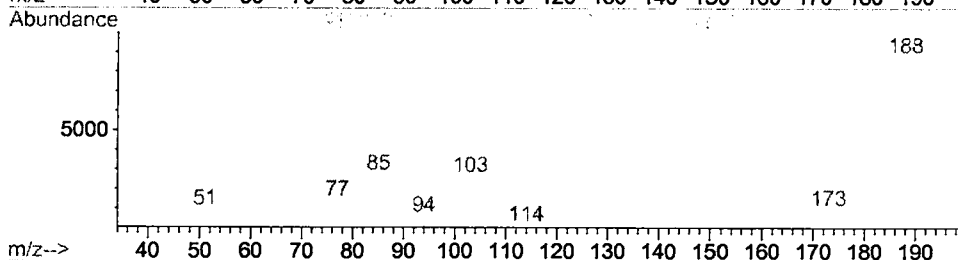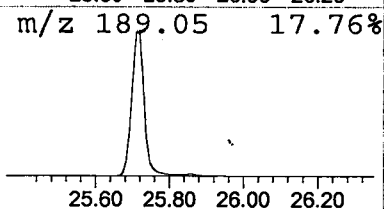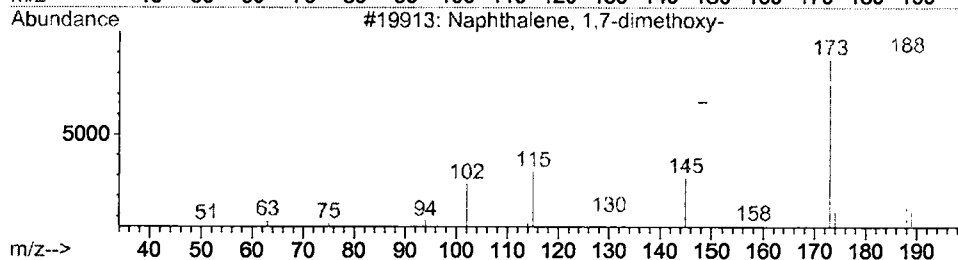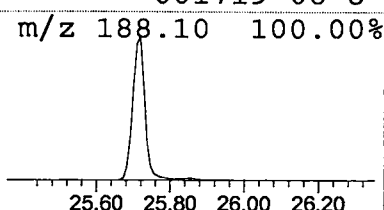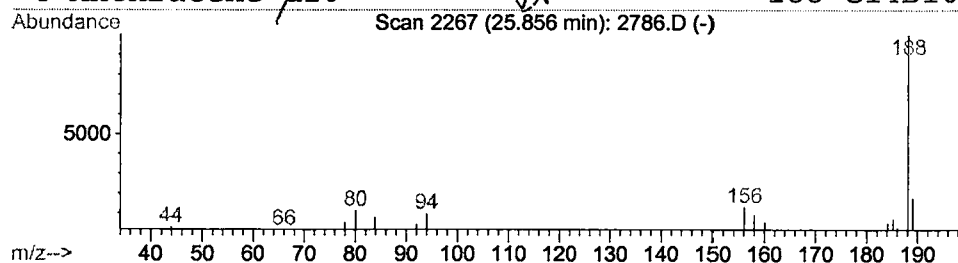

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 2 Mar 2002 3:02 am
 Data File: C:\HPCHEM\1\DATA\MAR0102\2786.D
 Name: gc/ms scan 2/6
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

Naphthalene, 1,7-dim	25.86	0.2	ug/l	30848	ISTD04	25.72	2510580	20.0
2786.D GCMS0208.M	Tue Mar 05 10:51:59 2002							

Library Searched : C:\DATABASE\nbs75k.1
 Quality : 9
 ID : 1,3-Dioxane

