

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 03/11/2002 Time: 16:09:45

Sample: AE02789
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 3/11/02 16:09 Ended: 3/11/02 16:09 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		79		5.0

Comments for Sample AE02789 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-11-2002 Time: 16:09:48

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

The recovery for 1 of the 43 compounds in the LCS Standard was below its acceptance range.

Data File : C:\HPCHEM\1\DATA\MAR0102\2789.D

Vial: 23

Acq On : 2 Mar 2002 5:58 am

Operator:

Sample : gc/ms scan 2/6 fb

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 5 10:43 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 27 11:30:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.31	152	314554	20.00	ug/l	-0.04
10) Naphthalene-d8	15.96	136	1225615	20.00	ug/l	-0.04
17) Acenaphthene-d10	21.27	164	653149	20.00	ug/l	-0.04
29) Phenanthrene-d10	25.71	188	952651	20.00	ug/l	-0.05
38) Chrysene-d12	33.78	240	626909	20.00	ug/l	-0.06
44) Perylene-d12	38.05	264	417337	20.00	ug/l	-0.07

System Monitoring Compounds

37) 2,4-DDD	30.79	235	39286	3.95	ug/mL	0.29
Spiked Amount	5.000		Recovery	=	79.00%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	0.00	128	0	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	22.75	149	207	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)=qualifier out of range (m)=manual integration

2789.D GCMS0208.M Tue Mar 05 10:44:04 2002

Page 1

Data File : C:\HPCHEM\1\DATA\MAR0102\2789.D

Vial: 23

Acq On : 2 Mar 2002 5:58 am

Operator:

Sample : gc/ms scan 2/6 fb

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 5 10:43 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 27 11:30:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	27.69	149	8606	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.77	228	1324	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.99	149	2620	N.D.		
43) Chrysene	33.77	228	1324	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.05	252	1447	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

2789.D GCMS0208.M

Tue Mar 05 10:44:07 2002


Page 2

Data File : C:\HPCHEM\1\DATA\MAR0102\2789.D
Acq On : 2 Mar 2002 5:58 am
Sample : gc/ms scan 2/6 fb
Misc :
MS Integration Params: GOOFY.P
Quant Time: Mar 5 10:43 2002

Vial: 23
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 27 11:30:15 2002
Response via : Initial Calibration

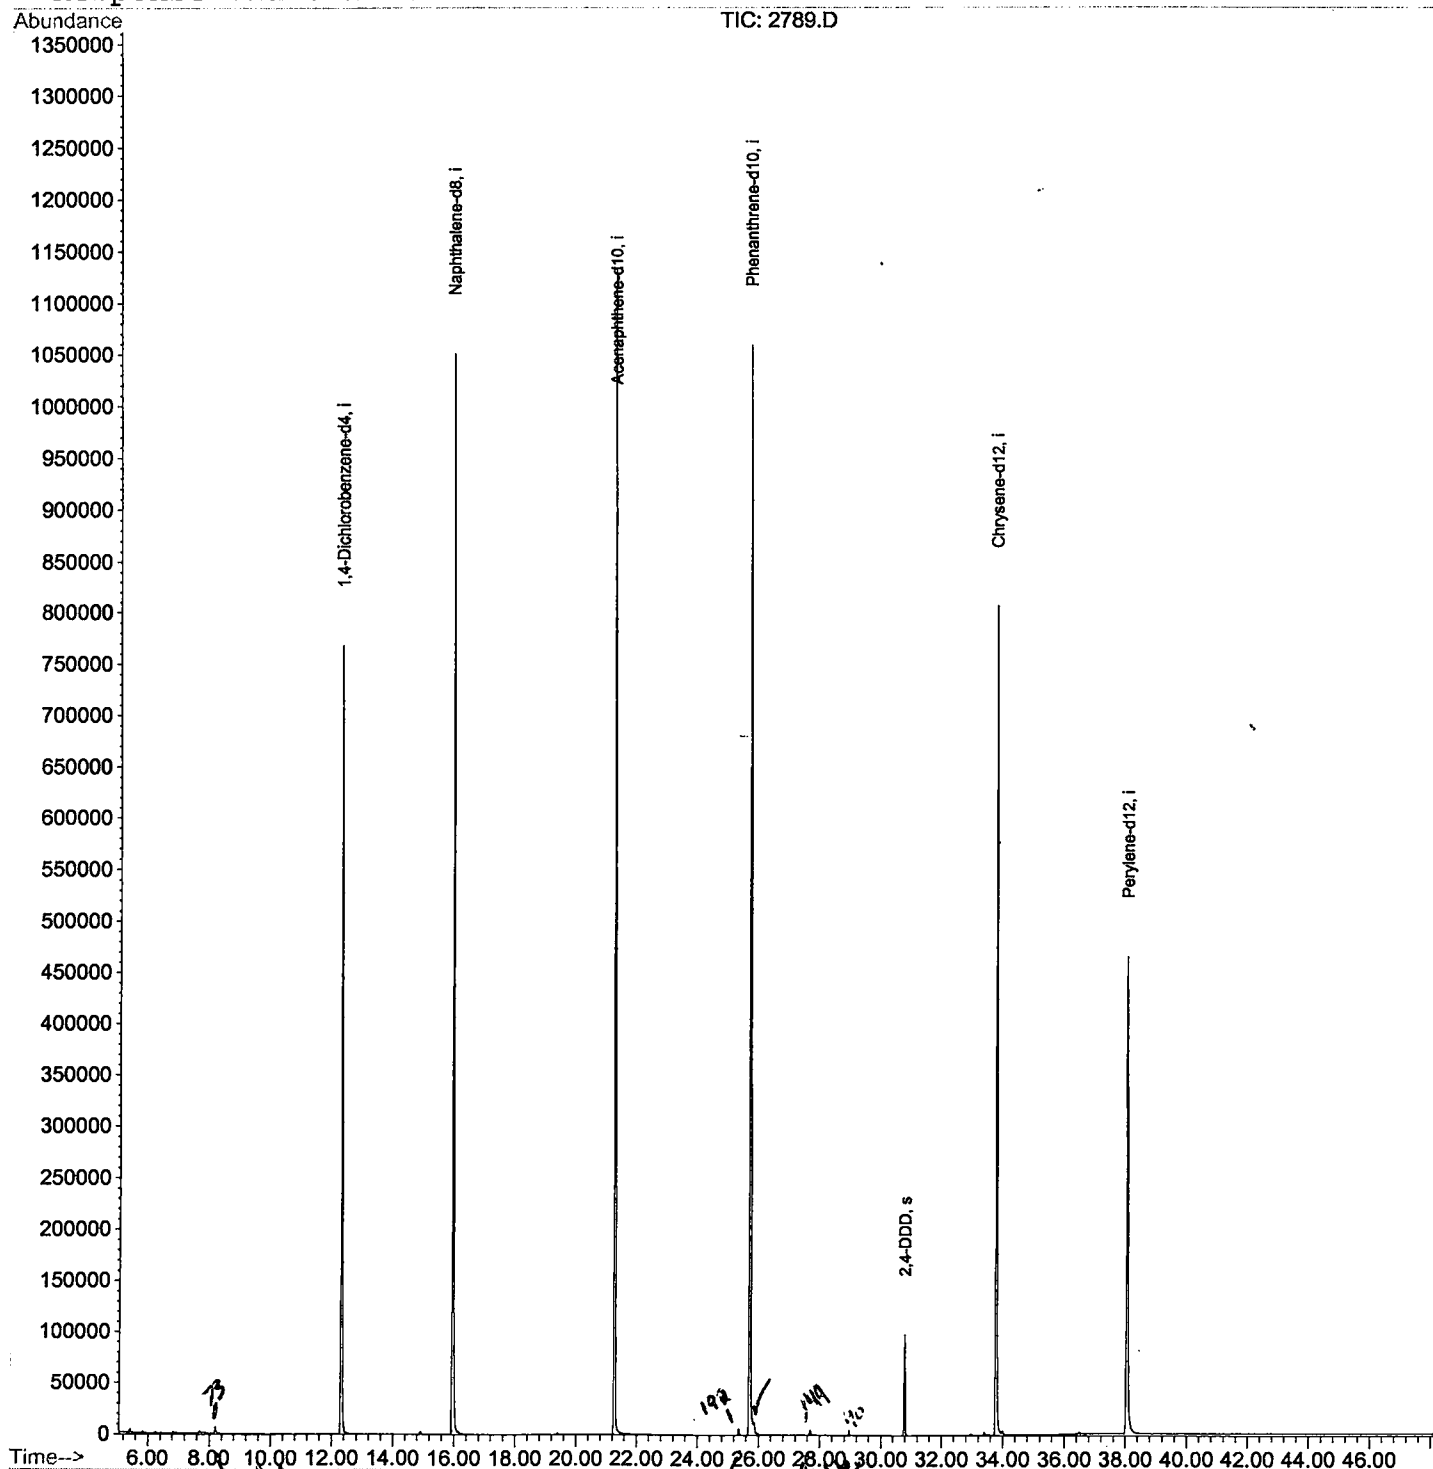

2789.D GCMS0208.M

Tue Mar 05 10:14 2002

Page 3

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAR0102\2789.D

Vial: 23

Acq On : 2 Mar 2002 5:58 am

Operator:

Sample : gc/ms scan 2/6 fb

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.311	787	792	809	rBV	768088	1775159	69.26%	13.920%
2	15.956	1183	1189	1207	rBV	1051008	2373541	92.61%	18.613%
3	21.271	1761	1768	1780	rBV	1134324	2562884	100.00%	20.097%
4	25.714	2245	2252	2264	rBV2	1059394	2430546	94.84%	19.060%
5	25.852	2264	2267	2274	rVB2	10438	30300	1.18%	0.238%
6	30.791	2800	2805	2812	rBV	98384	195809	7.64%	1.535%
7	33.784	3124	3131	3148	rBV	806707	1907155	74.41%	14.955%
8	38.053	3587	3596	3619	rBV2	464142	1476984	57.63%	11.582%


Sum of corrected areas: 12752378

2789.D GCMS0208.M

Tue Mar 05 10:54:06 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAR0102\2789.D
 Operator :
 Acquired : 2 Mar 2002 5:58 am using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 2/6 fb
 Misc Info :
 Vial Number: 23
 Quant File :GCMS0208.RES (RTE Integrator)

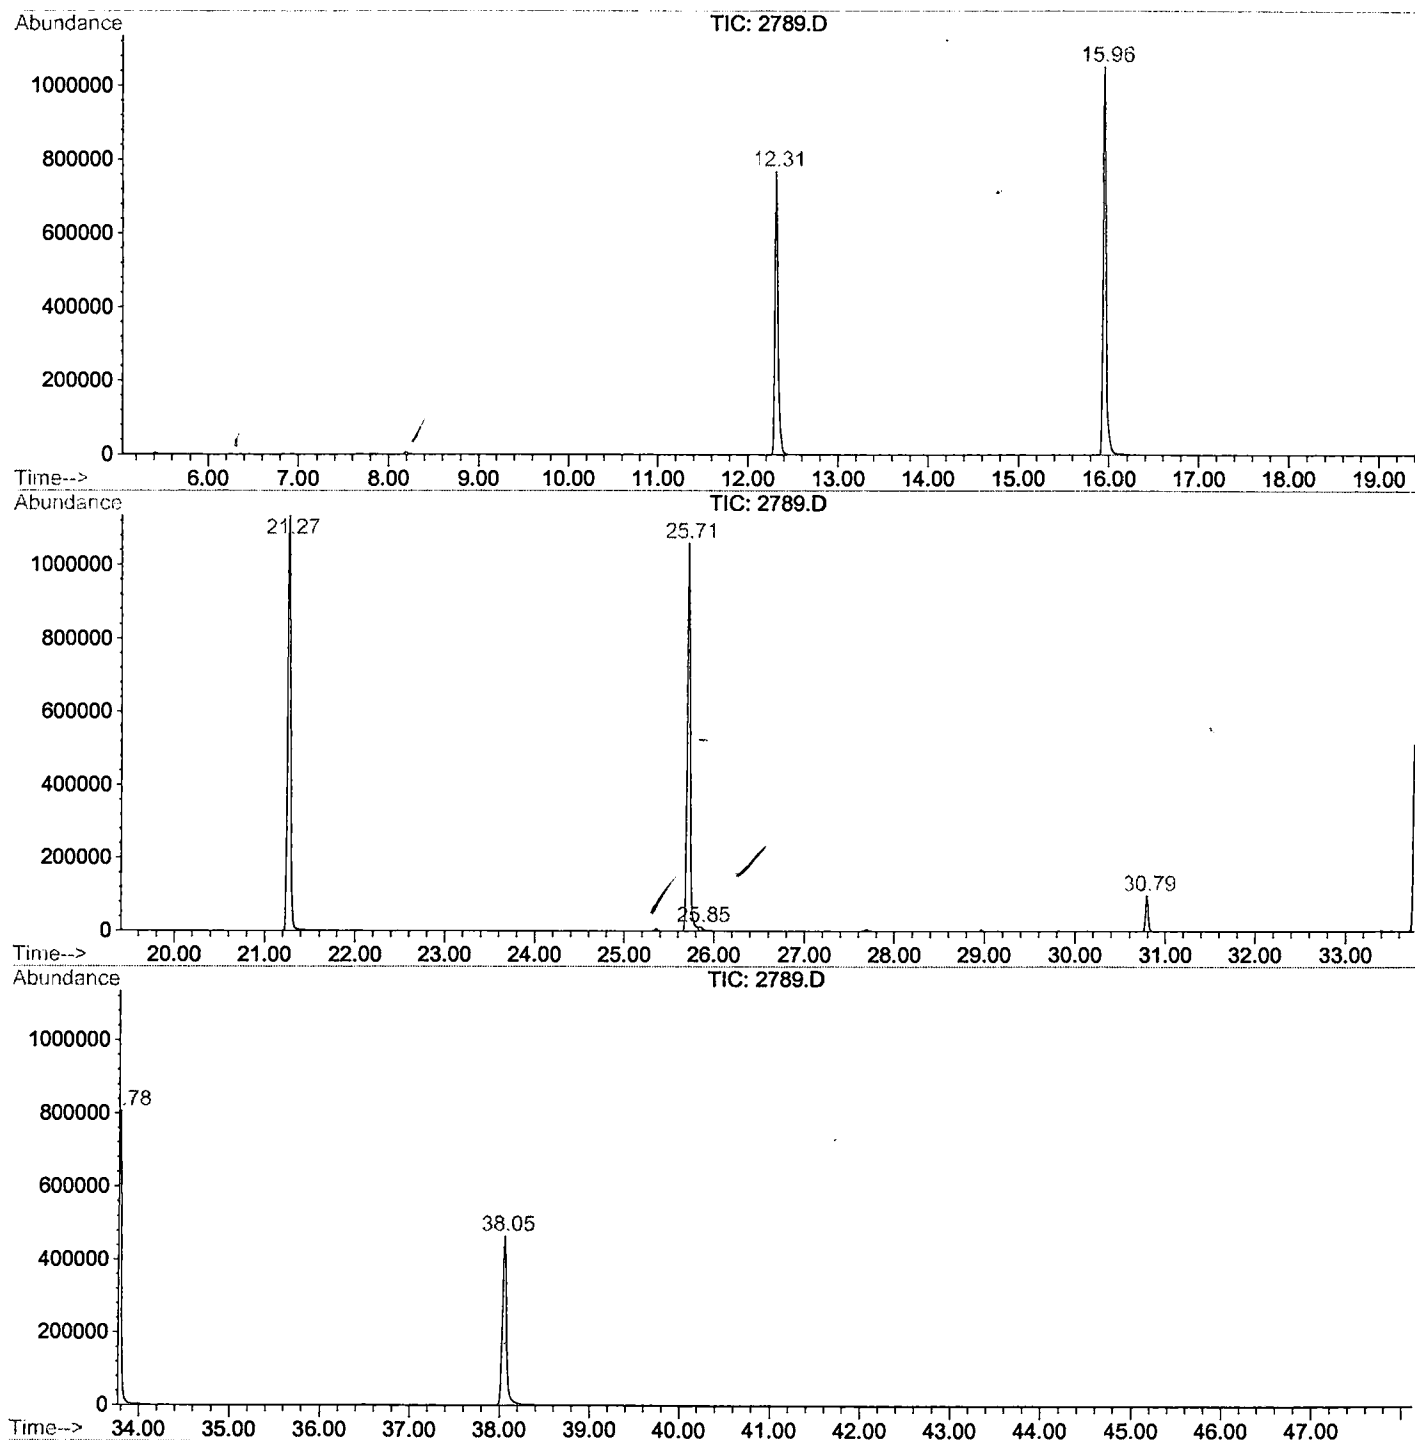

2789.D GCMS0208.M

Tue Mar 05 10:54:12 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR0102\2789.D
 Acq On : 2 Mar 2002 5:58 am
 Sample : gc/ms scan 2/6 fb
 Misc :
 MS Integration Params: LSCINT.P











Vial: 23
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 Anthracene-d10- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.85	0.25 ug/l	30300	Phenanthrene-d10	25.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Anthracene-d10- <i>IS</i>	188	C14D10	001719-06-8	80
2		Phenanthrene-d10	188	C14D10	001517-22-2	50
3		1,4-Naphthalenedione, 2-hydroxy-3-m	188	C11H8O3	000483-55-6	50
4		3H-Pyrazol-3-one, 2,4-dihydro-4,4-d	188	C11H12N2O	017694-06-3	42

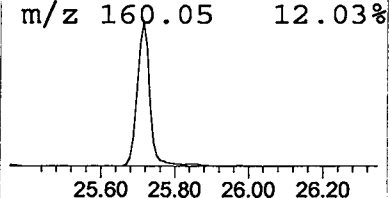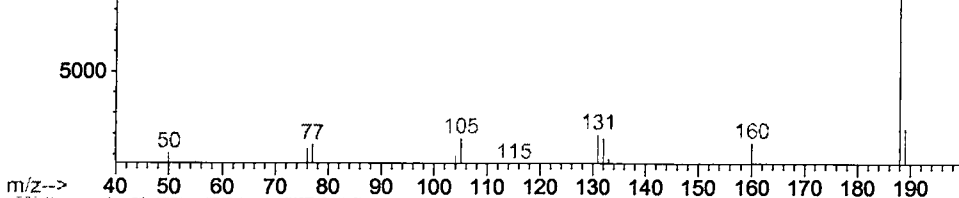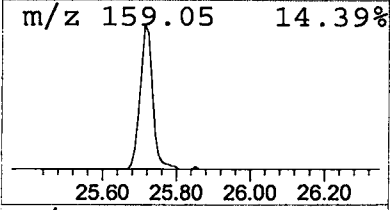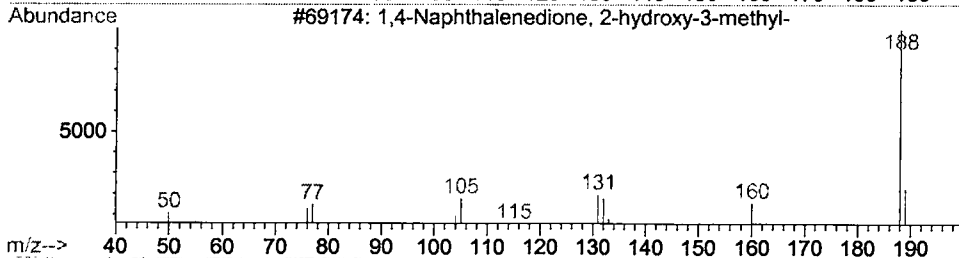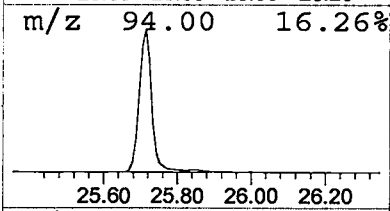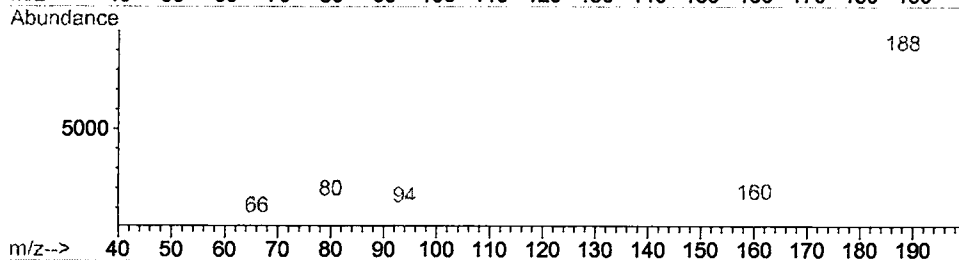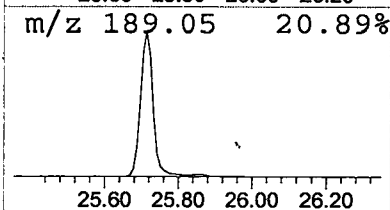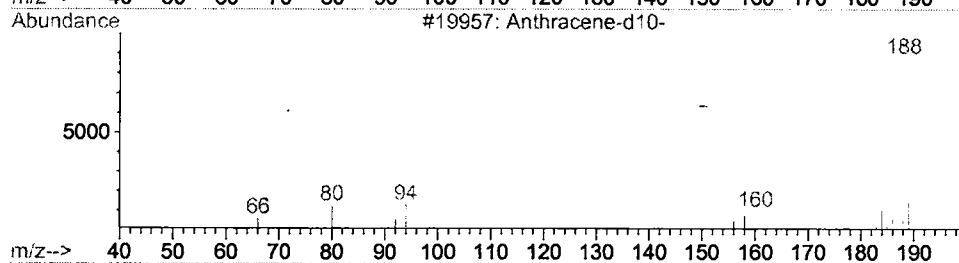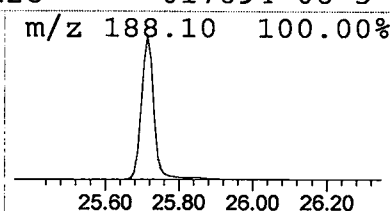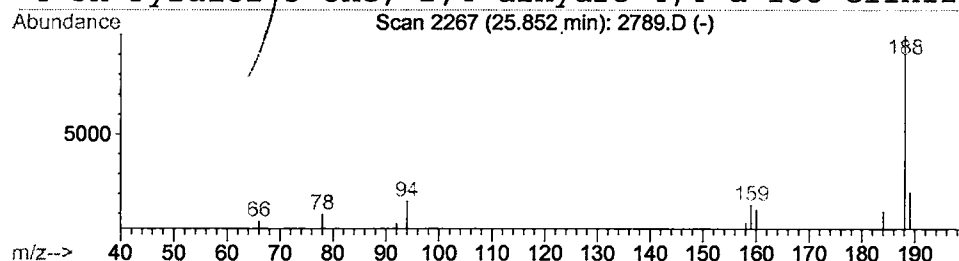

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 2 Mar 2002 5:58 am
 Data File: C:\HPCHEM\1\DATA\MAR0102\2789.D
 Name: gc/ms scan 2/6 fb
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Anthracene d10	25.85	0.2	ug/l	30300	ISTD04	25.71	2430550	20.0

2789.D GCMS0208.M Tue Mar 05 10:54:21 2002