

Method 508 MOD.

Date Extracted 2-7-02

Page 74

Ref

#GCMs-16917

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
L.B.		500 ml		1 ml			1 ml	9B	7	
Ref.					0.5 ml			9A		
2966								10A		
2967								10B		
2968								6A		
2969								6B		
2970								7B		
2971								8A		
2972								7A		
2973	FB							9A		
3014								8B		
3015								10B		
31344	Re-EXTRACT							10A		
31136	Re-EXTRACT Q-Bottle FB.							9B		
Remarks 31344 → RE-EXTRACT 31136 → RE-EXTRACT A Field blank Q Bottle NaOH was added to BRING pH to 7.										
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - Sep. Run Solv. lot# <u>V41470</u> NaCl lot# <u>V3961P</u> Na2SO4 lot# <u>V39400</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
(REF) SPIKE	91759									
MDL/MDRF										
Q. CHECK										
INT. STD.	Lot# <u>2410320</u>									
SURROGATE	02 01 02									
LPC										
ENDRIN/DDT										

Reviewed by,
JB 5/24/02

Analyst A.D.
revision 4/12/01

Verified by _____

Reviewed by DW
Date 2/15/02

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB0802\DFTPP1.D

Acq On : 9 Feb 2002 9:37 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 26

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

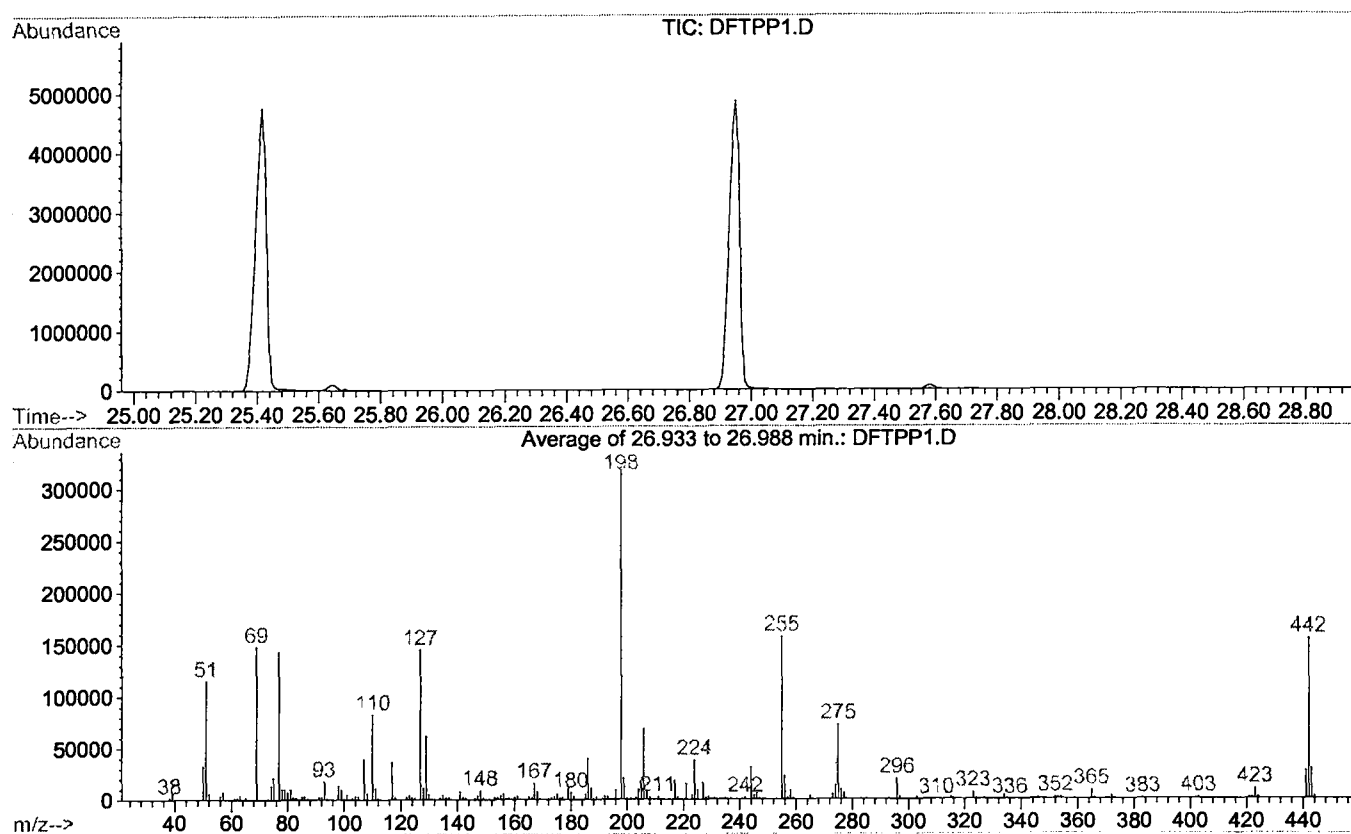

Spectrum Information: Average of 26.933 to 26.988 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.9	115305	PASS
68	69	0.00	2	0.0	23	PASS
69	198	0.00	100	46.2	148236	PASS
70	69	0.00	2	0.1	186	PASS
127	198	40	60	45.3	145297	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	320744	PASS
199	198	5	9	6.6	21087	PASS
275	198	10	30	22.6	72595	PASS
365	198	1	100	2.7	8637	PASS
441	443	0.01	100	92.9	27480	PASS
442	198	40	110	48.3	154996	PASS
443	442	17	23	19.1	29573	PASS