

User: Vinci, David L.
Westchester Dept. of Labs & Research
Date: 02/15/2002 Time: 09:26:13

Sample: AE02969

Analysis: \$GCMS GCMS Scan For Unknowns

Units: ug

Started: 2/15/02 09:26 Ended: 2/15/02 09:26 Analyst: DLV

Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		85		5.0

Comments for Sample AE02969 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 02-15-2002 Time: 09:26:48

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

The recoveries for 7 of the 43 compounds in the LCS Standard were below their acceptance ranges.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB0802\2969.D
 Acq On : 9 Feb 2002 4:25 pm
 Sample : GC/MS SCAN 2/7
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Feb 13 10:45 2002

Vial: 33
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Feb 08 15:29:22 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.35	152	387375	20.00	ug/l	0.00
10) Naphthalene-d8	15.99	136	1483204	20.00	ug/l	-0.01
17) Acenaphthene-d10	21.30	164	811142	20.00	ug/l	-0.01
29) Phenanthrene-d10	25.75	188	1191458	20.00	ug/l	-0.01
38) Chrysene-d12	33.82	240	837570	20.00	ug/l	-0.02
44) Perylene-d12	38.11	264	559058	20.00	ug/l	-0.01

System Monitoring Compounds

37) 2,4-DDD	30.83	235	63205	4.27	ug/mL	0.33
Spiked Amount	5.000		Recovery	=	85.40%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	16.04	128	657	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.78	149	545	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#) = qualifier out of range (m) = manual integration

2969.D GCMS0208.M Wed Feb 13 10:46:12 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB0802\2969.D

Vial: 33

Acq On : 9 Feb 2002 4:25 pm

Operator: 209 GALOS

Sample : GC/MS SCAN 2/7

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 13 10:45 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Feb 08 15:29:22 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.76	178	516	N.D.		
34) Anthracene	25.76	178	420	N.D.		
35) Di-n-butylphthalate	27.72	149	3768	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.82	228	2280	N.D.		
42) Bis(2-ethylhexyl)phthalate	34.03	149	1232	N.D.		
43) Chrysene	33.82	228	2281	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.11	252	2125	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

2969.D GCMS0208.M

Wed Feb 13 10:46:16 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\FEB0802\2969.D
Acq On : 9 Feb 2002 4:25 pm
Sample : GC/MS SCAN 2/7
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 13 10:45 2002

Vial: 33
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Feb 08 15:29:22 2002
Response via : Initial Calibration

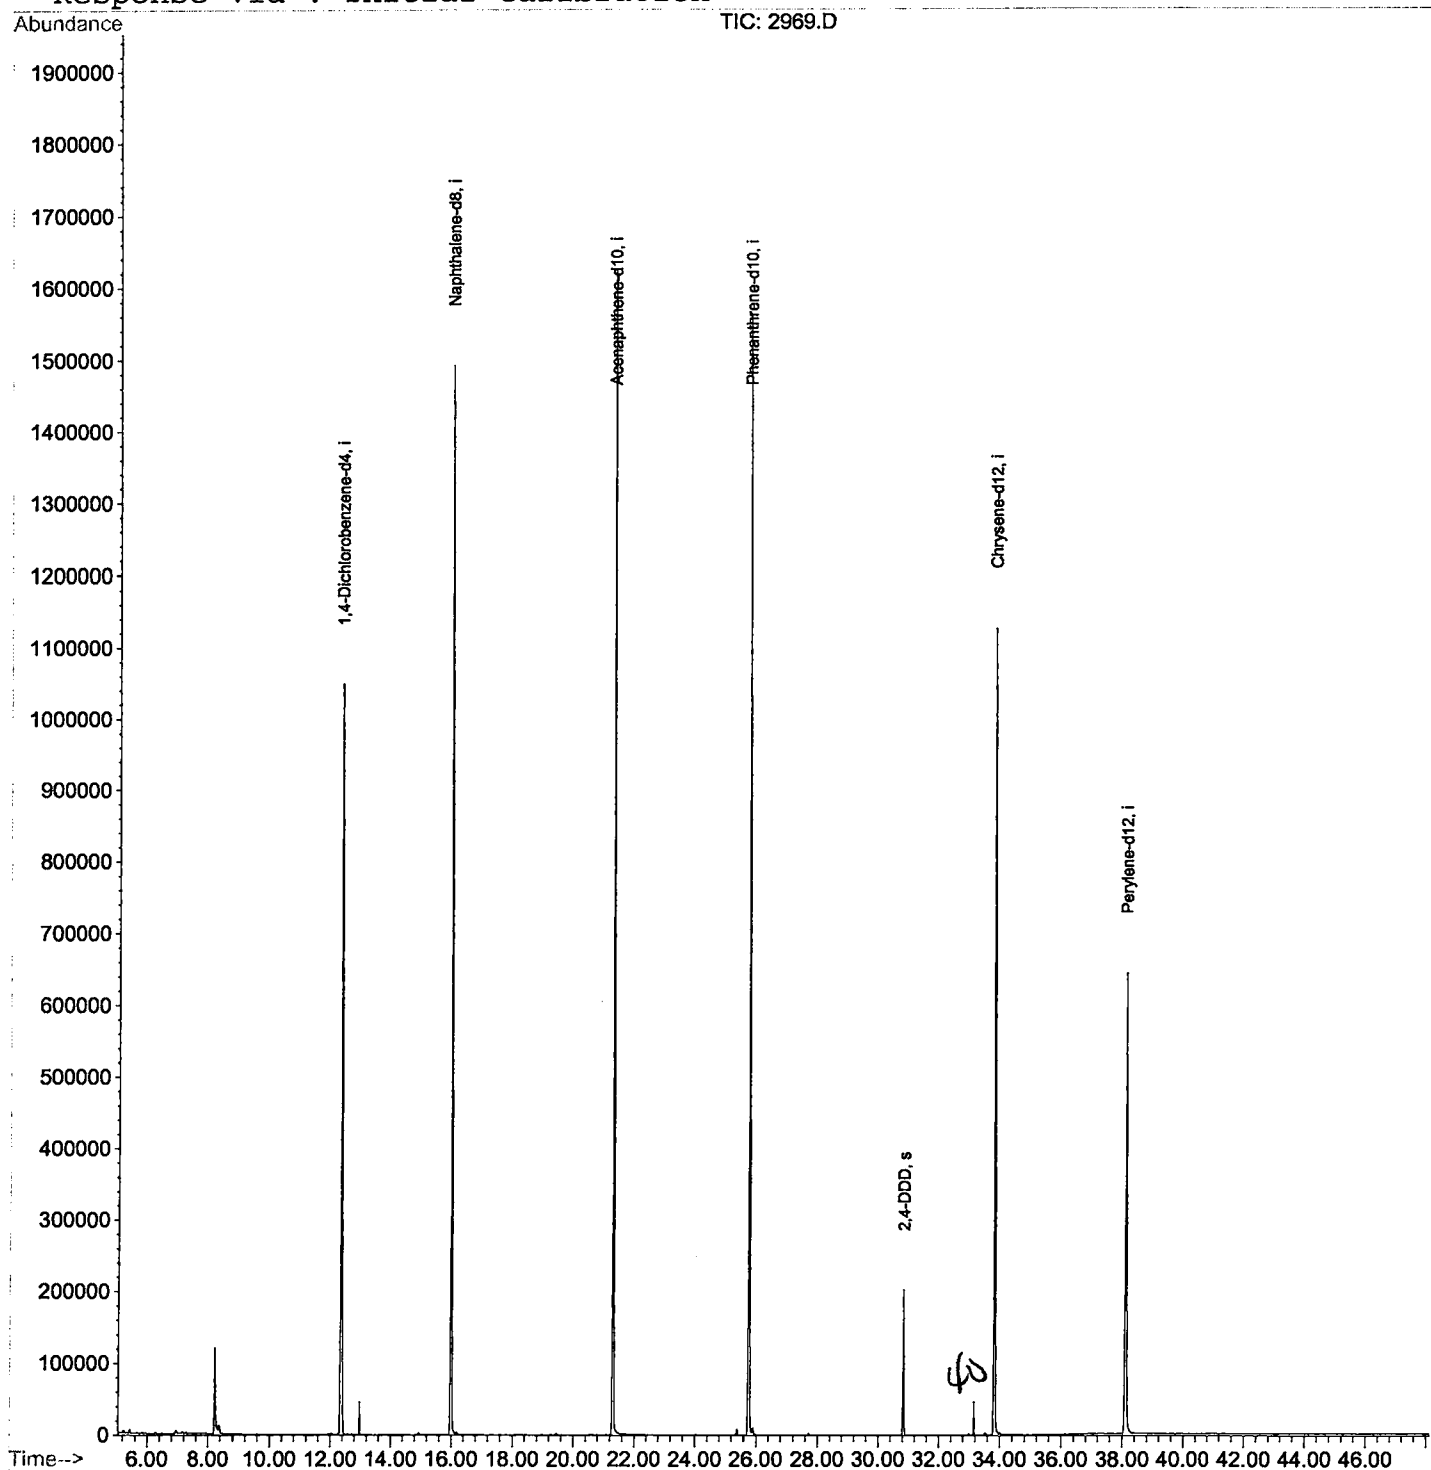

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB0802\2969.D
 Acq On : 9 Feb 2002 4:25 pm
 Sample : GC/MS SCAN 2/7
 Misc :
 MS Integration Params: LSCINT.P

Vial: 33
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.219	341	346	359	rBV	119581	295924	8.73%	1.704%
2	12.341	790	795	811	rVB	1048497	2466593	72.76%	14.202%
3	15.986	1186	1192	1208	rBV	1492192	3064327	90.40%	17.643%
4	21.301	1765	1771	1789	rBV	1626329	3389916	100.00%	19.518%
5	25.754	2249	2256	2267	rBV2	1561476	3291402	97.09%	18.951%
6	30.830	2804	2809	2815	rVB	202147	389031	11.48%	2.240%
7	33.823	3128	3135	3149	rBV2	1125950	2548889	75.19%	14.676%
8	38.110	3594	3602	3620	rBV2	642068	1922230	56.70%	11.067%

Sum of corrected areas: 17368312

2969.D GCMS0208.M Wed Feb 13 11:09:37 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB0802\2969.D
 Operator : 209 GALOS
 Acquired : 9 Feb 2002 4:25 pm using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: GC/MS SCAN 2/7
 Misc Info :
 Vial Number: 33
 Quant File :GCMS0208.RES (RTE Integrator)

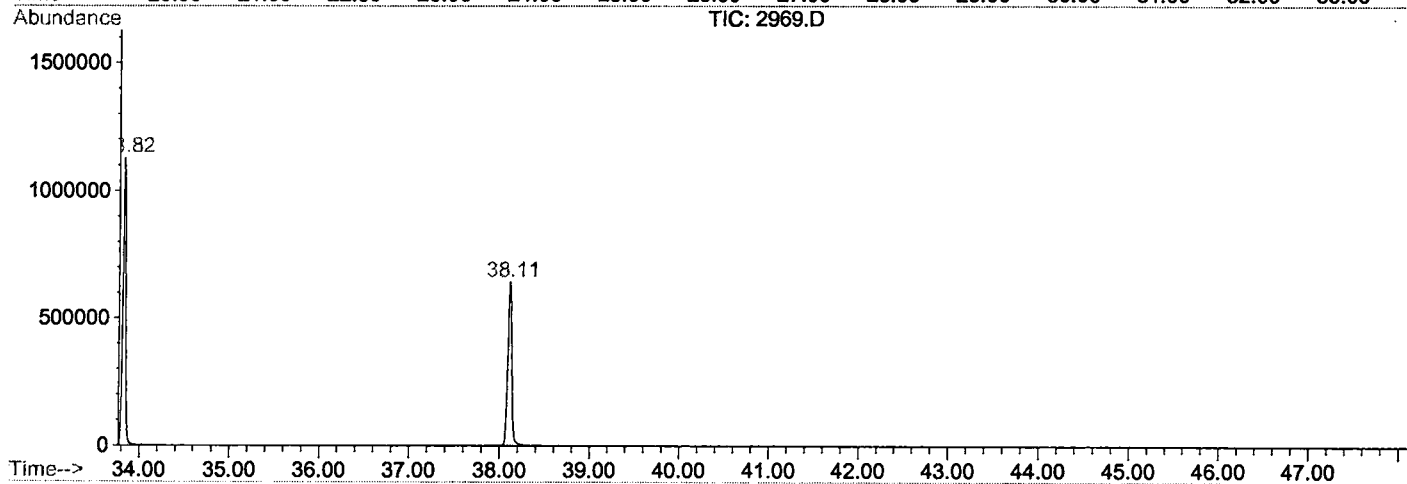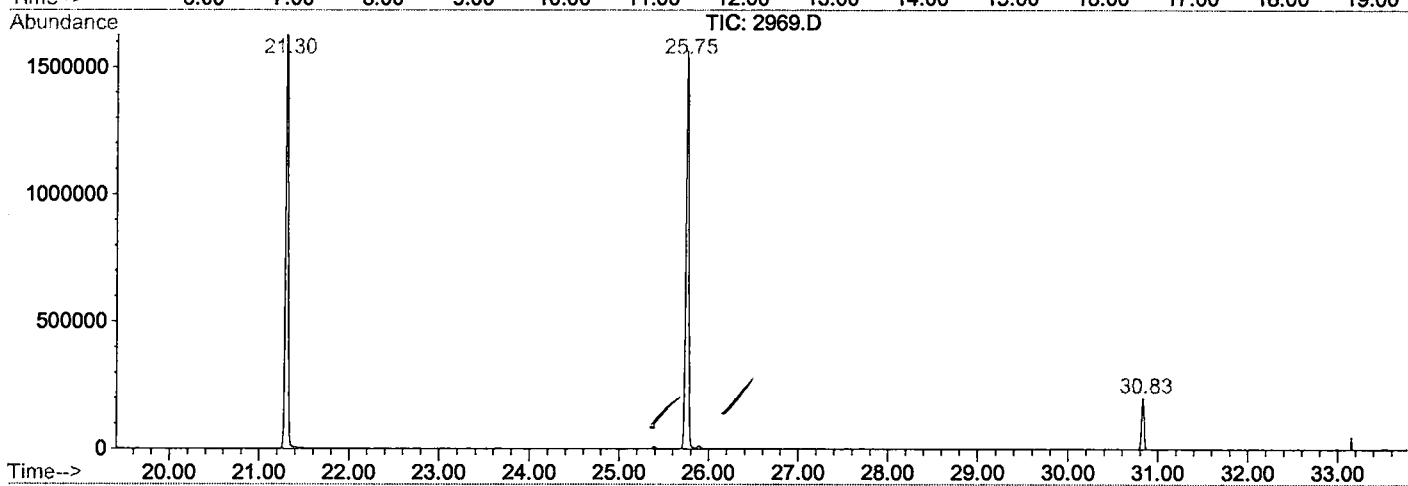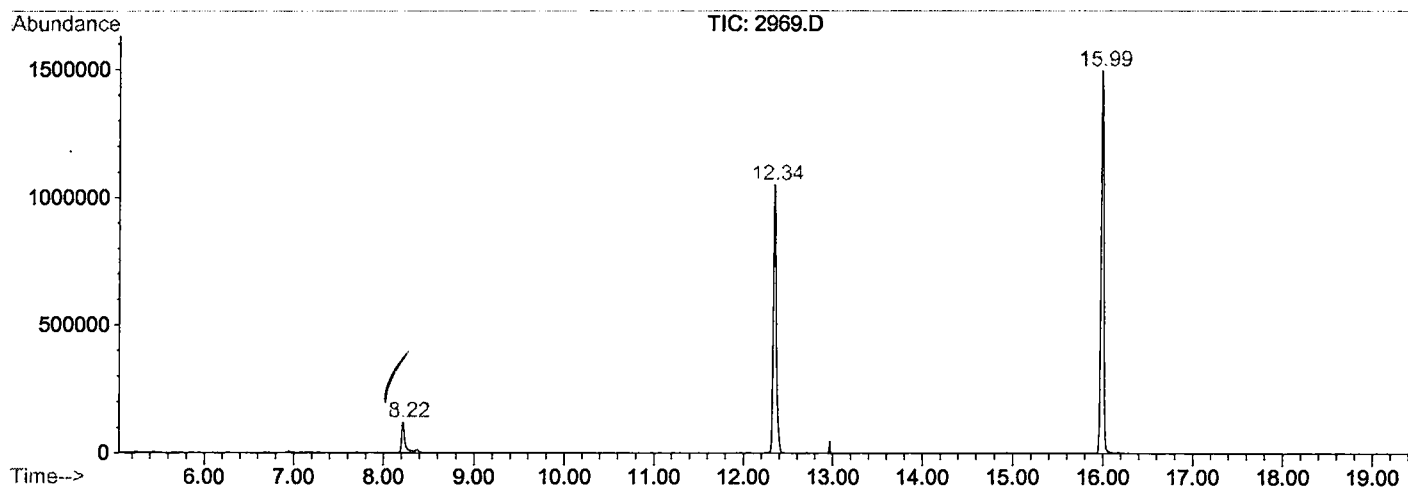

2969.D GCMS0208.M

Wed Feb 13 11:09:43 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB0802\2969.D
Acq On : 9 Feb 2002 4:25 pm
Sample : GC/MS SCAN 2/7
Misc :
MS Integration Params: LSCINT.P









Vial: 33
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 Silane, tetramethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.22	2.40 ug/l	295924	1,4-Dichlorobenzene-d4	12.35

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Silane, tetramethyl-	88	C4H12Si	000075-76-3	38
2			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	28
3			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

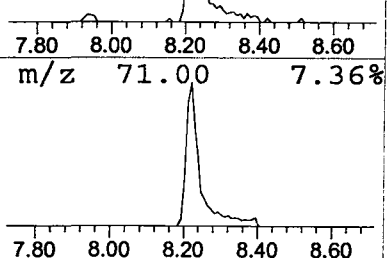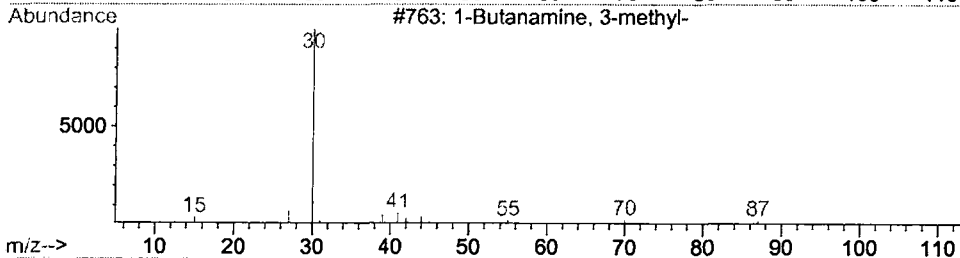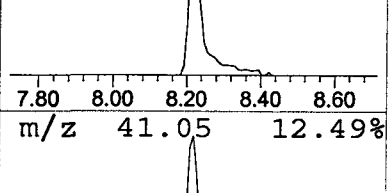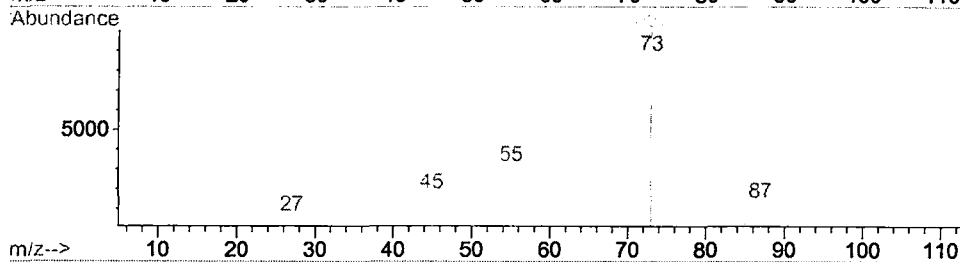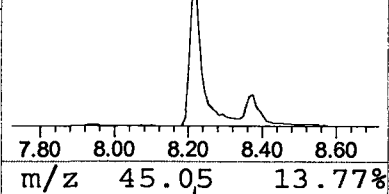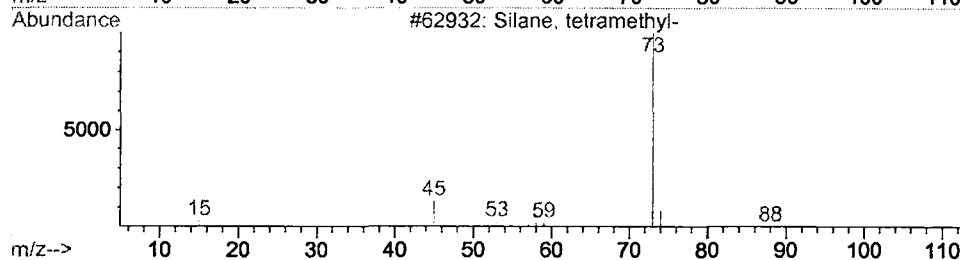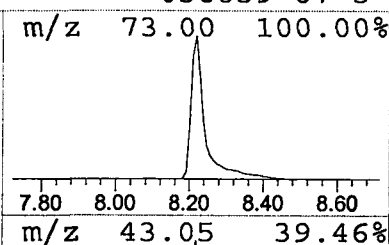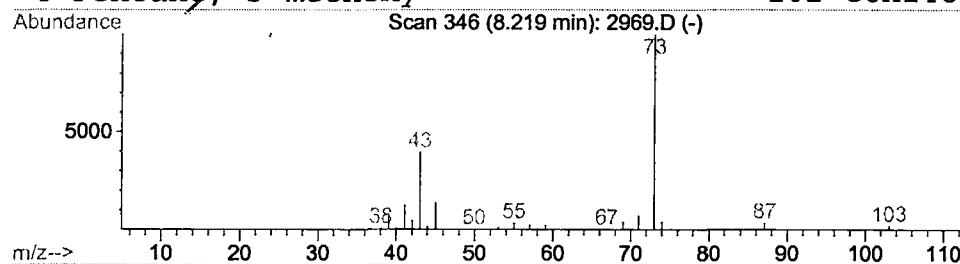

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 9 Feb 2002 4:25 pm
 Data File: C:\HPCHEM\1\DATA\FEB0802\2969.D
 Name: GC/MS SCAN 2/7
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Silane, tetramethyl-	8.22	2.4	ug/l	295924	ISTD01	12.35	2466590	20.0
2969.D GCMS0208.M	Wed Feb 13	11:09:52	2002					