

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 02/15/2002 Time: 09:28:52

Sample: AE02972
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 2/15/02 09:28 Ended: 2/15/02 09:28 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		82		5.0

• **Comments for Sample AE02972 - Analysis \$GCMS**

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 02-15-2002 Time: 09:29:02

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

The recoveries for 7 of the 43 compounds in the LCS Standard were below their acceptance ranges.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB0802\2972.D

Vial: 36

Acq On : 9 Feb 2002 7:19 pm

Operator: 209 GALOS

Sample : GC/MS SCAN 2/7

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 13 10:50 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Feb 08 15:29:22 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.35	152	408721	20.00	ug/l	0.00
10) Naphthalene-d8	15.99	136	1587795	20.00	ug/l	0.00
17) Acenaphthene-d10	21.31	164	862267	20.00	ug/l	0.00
29) Phenanthrene-d10	25.75	188	1250844	20.00	ug/l	-0.01
38) Chrysene-d12	33.82	240	865843	20.00	ug/l	-0.02
44) Perylene-d12	38.11	264	592257	20.00	ug/l	-0.01

System Monitoring Compounds

37) 2,4-DDD	30.83	235	63371	4.08	ug/mL	0.33
Spiked Amount	5.000		Recovery	=	81.60%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	16.04	128	444	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	22.78	149	420	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)=qualifier out of range (m)=manual integration

2972.D GCMS0208.M Wed Feb 13 10:50:57 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB0802\2972.D

Vial: 36

Acq On : 9 Feb 2002 7:19 pm

Operator: 209 GALOS

Sample : GC/MS SCAN 2/7

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 13 10:50 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Feb 08 15:29:22 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.75	178	353	N.D.		
34) Anthracene	25.75	178	353	N.D.		
35) Di-n-butylphthalate	27.71	149	5117	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.90	228	5796	N.D.		
42) Bis(2-ethylhexyl)phthalate	34.02	149	4300	N.D.		
43) Chrysene	33.90	228	5951	N.D.		
45) Di-n-Octylphthalate	35.77	149	2707	N.D.		
46) Benzo(b)fluoranthene	36.89	252	3765	N.D.		
47) Benzo(k)fluoranthene	36.95	252	10397	N.D.		
48) Benzo(a)pyrene	38.12	252	2660	N.D.		
49) Indeno(1,2,3-cd)pyrene	42.31	276	2847	N.D.		
50) Dibenz(a,h)anthracene	42.40	278	3831	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

2972.D GCMS0208.M Wed Feb 13 10:51:01 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\FEB0802\2972.D
Acq On : 9 Feb 2002 7:19 pm
Sample : GC/MS SCAN 2/7
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 13 10:50 2002

Vial: 36
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Feb 08 15:29:22 2002
Response via : Initial Calibration

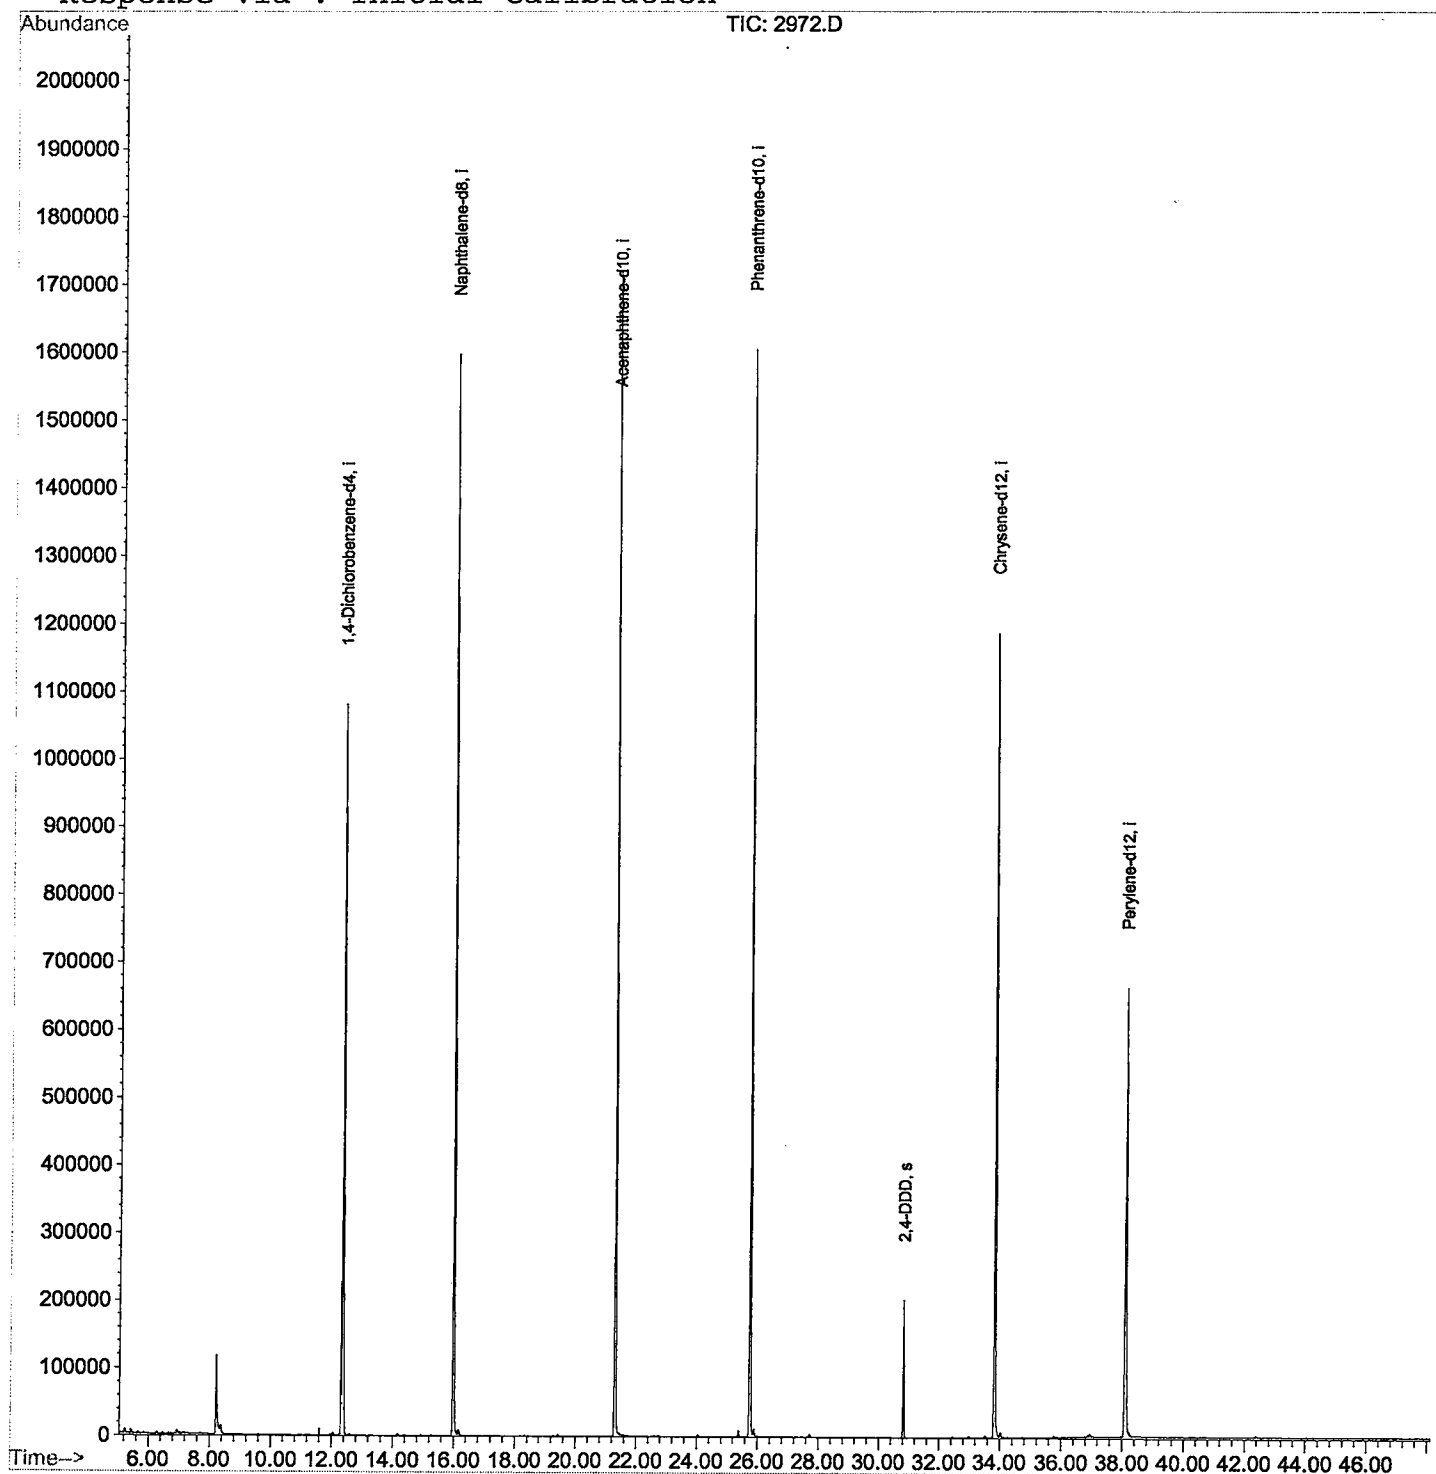

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB0802\2972.D
 Acq On : 9 Feb 2002 7:19 pm
 Sample : GC/MS SCAN 2/7
 Misc :
 MS Integration Params: LSCINT.P

Vial: 36
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.218	341	346	359	rBV	116933	318721	9.03%	1.738%
2	8.374	359	363	375	rVB	13423	41422	1.17%	0.226%
3	12.349	790	796	811	rVB	1079989	2603880	73.76%	14.196%
4	15.994	1186	1193	1207	rBV	1596958	3274541	92.76%	17.853%
5	21.309	1765	1772	1783	rBV	1721174	3530189	100.00%	19.247%
6	25.752	2249	2256	2268	rBV2	1604675	3468877	98.26%	18.912%
7	30.829	2804	2809	2815	rVB	202801	384208	10.88%	2.095%
8	33.822	3126	3135	3152	rBV2	1188011	2668918	75.60%	14.551%
9	38.109	3594	3602	3623	rBV2	662617	2051171	58.10%	11.183%

Sum of corrected areas: 18341927

2972.D GCMS0208.M Wed Feb 13 11:11:57 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB0802\2972.D
 Operator : 209 GALOS
 Acquired : 9 Feb 2002 7:19 pm using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: GC/MS SCAN 2/7
 Misc Info :
 Vial Number: 36
 Quant File :GCMS0208.RES (RTE Integrator)

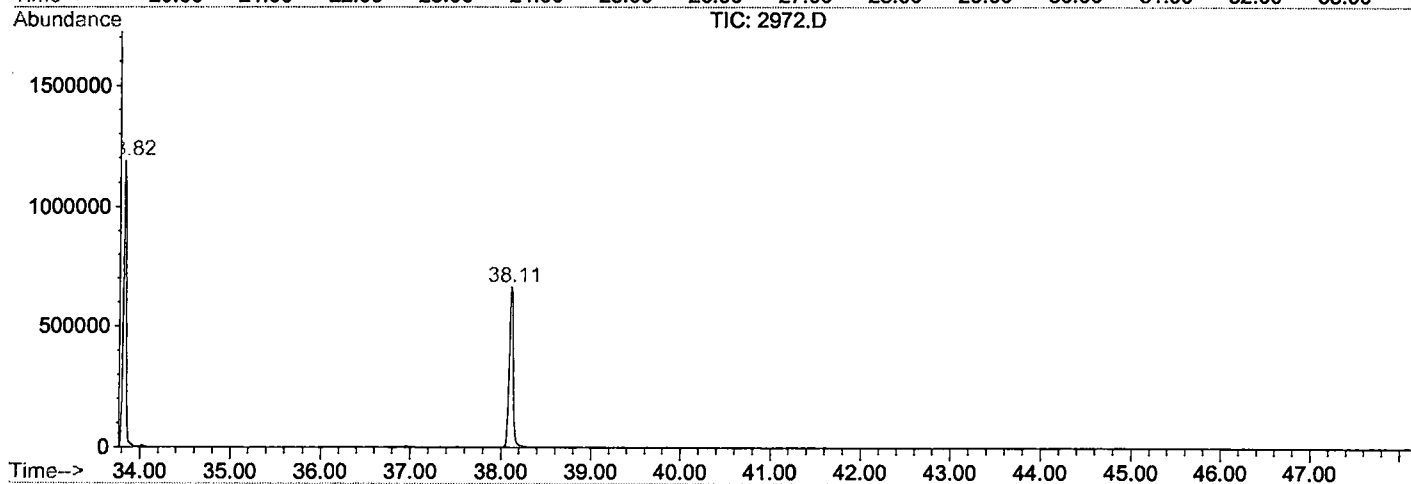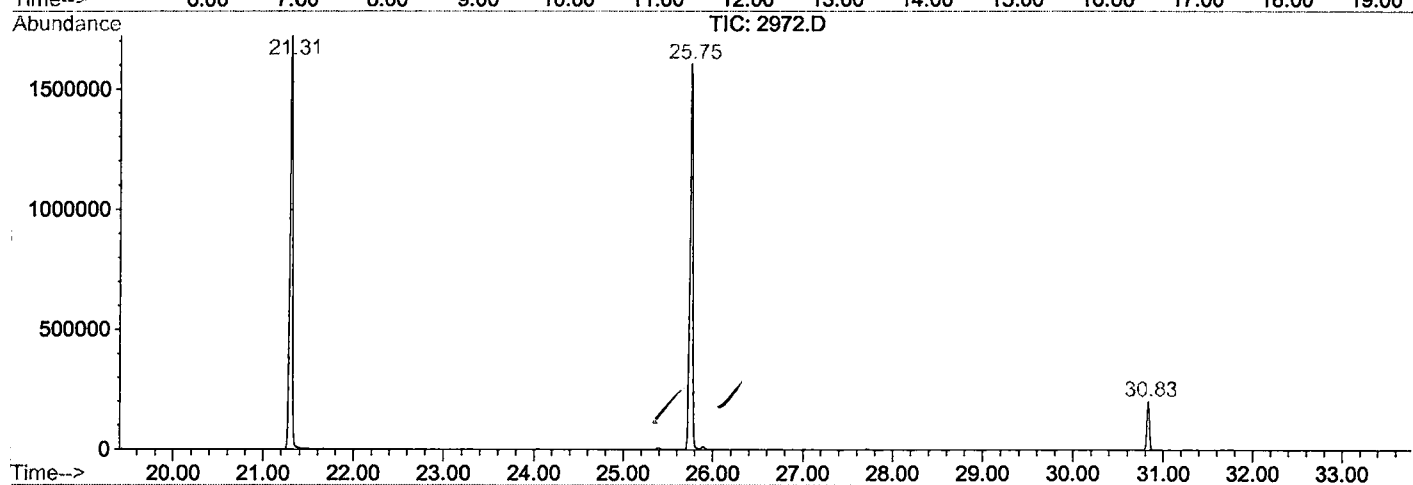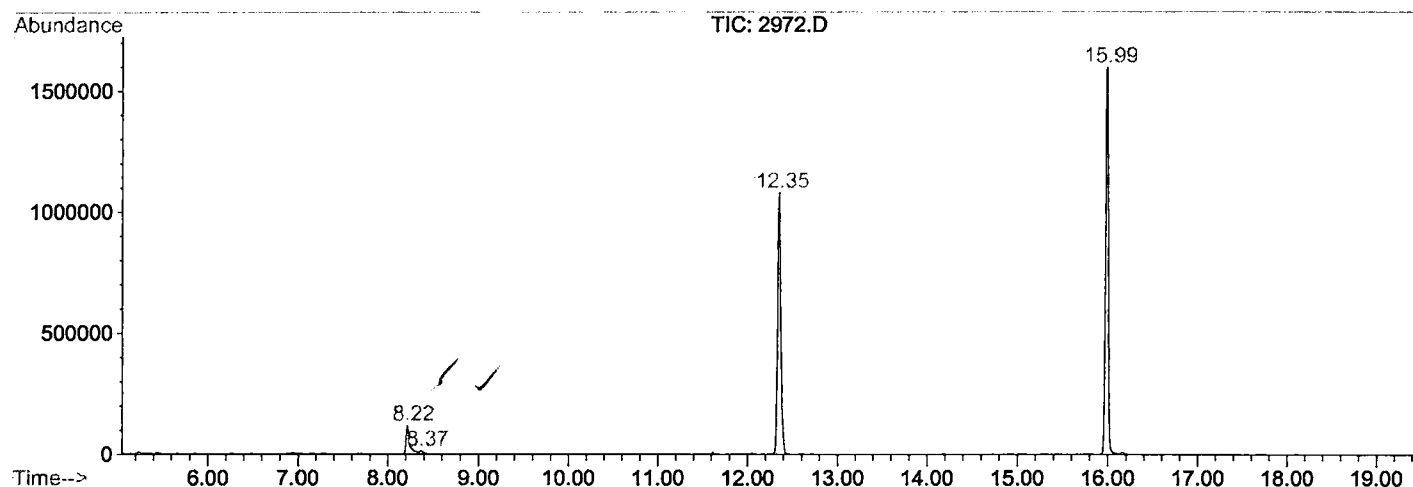

2972.D GCMS0208.M

Wed Feb 13 11:12:03 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB0802\2972.D
Acq On : 9 Feb 2002 7:19 pm
Sample : GC/MS SCAN 2/7
Misc :
MS Integration Params: LSCINT.P










Vial: 36
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 Silane, tetramethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.22	2.45 ug/l	318721	1,4-Dichlorobenzene-d4	12.35

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Silane, tetramethyl-	88	C4H12Si	000075-76-3	50
2			3-Pentanol 3-methyl-	102	C6H14O	000077-74-7	36
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9
4			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9

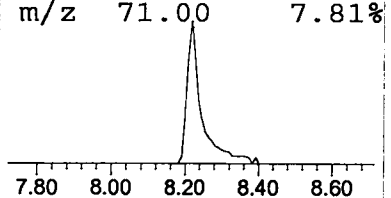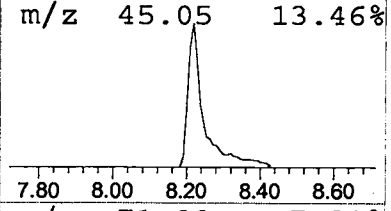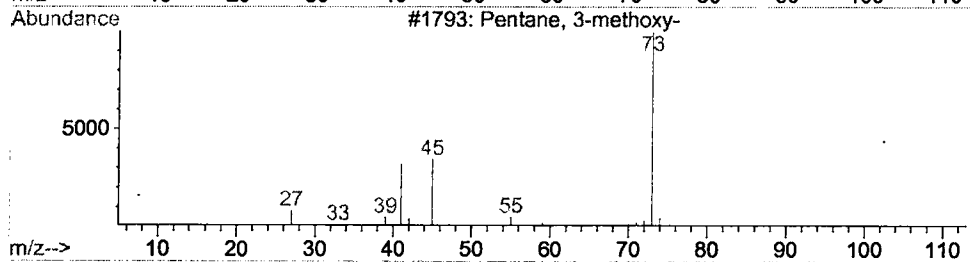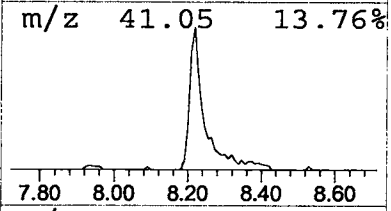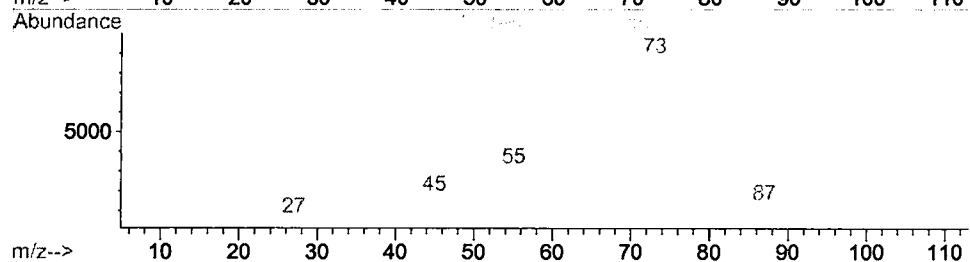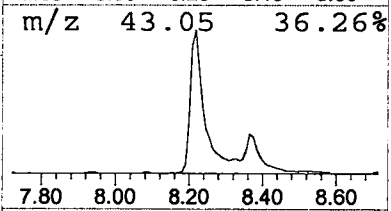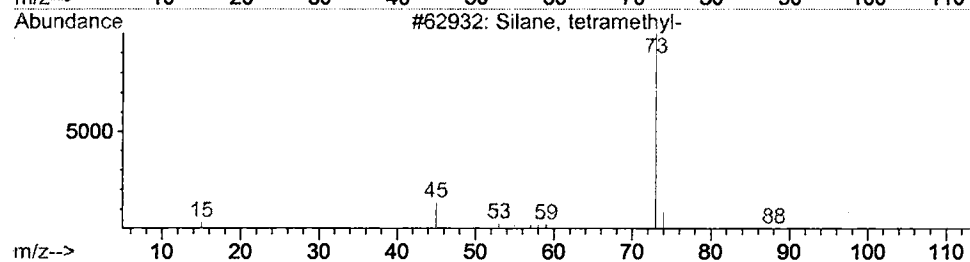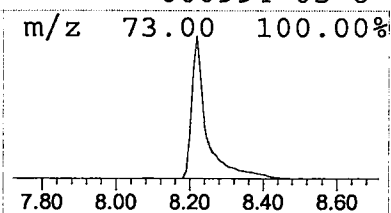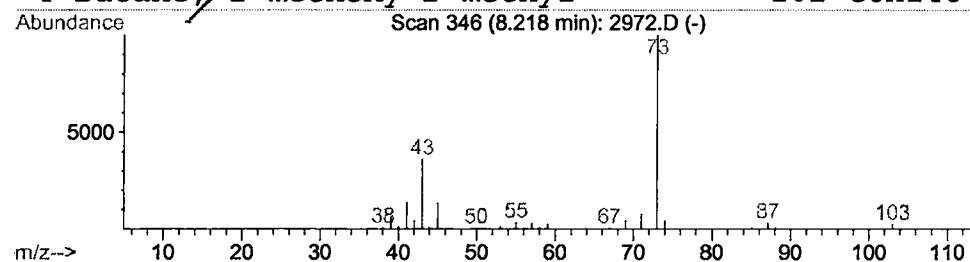

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB0802\2972.D
 Acq On : 9 Feb 2002 7:19 pm
 Sample : GC/MS SCAN 2/7
 Misc :
 MS Integration Params: LSCINT.P











Vial: 36
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 1-Octadecanol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.37	0.32 ug/l	41422	1,4-Dichlorobenzene-d4	12.35

Hit#	5	Tentative ID	MW	MolForm	CAS#	Qual
1		1-Octadecanol	270	C18H38O	000112-92-5	17
2		1-Fluorononane	146	C9H19F	000463-18-3	9
3		Decane, 1-fluoro-	160	C10H21F	000334-56-5	9
4		2-Butanone, 4-butoxy-3-methyl-	158	C9H18O2	054340-94-2	9

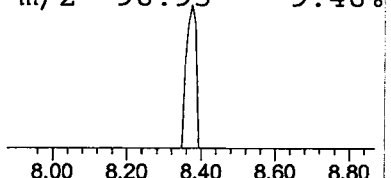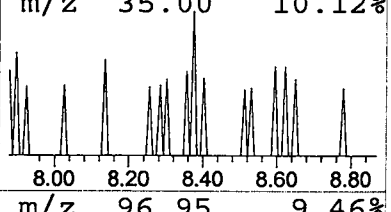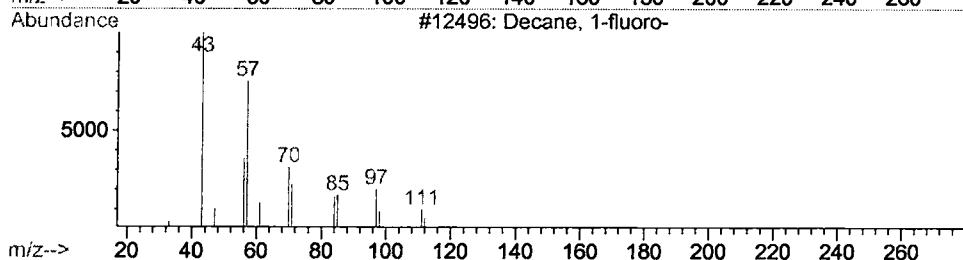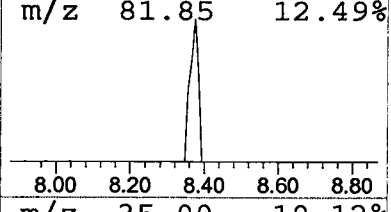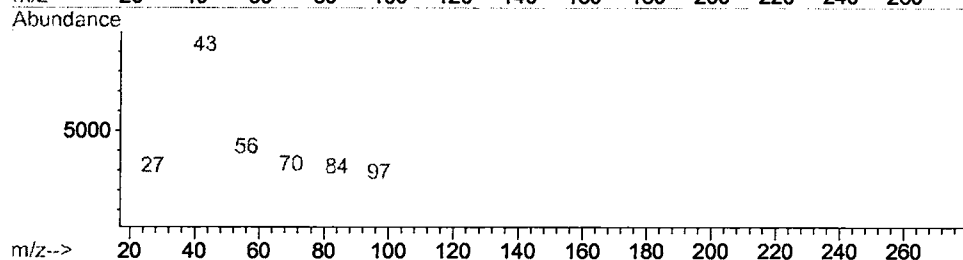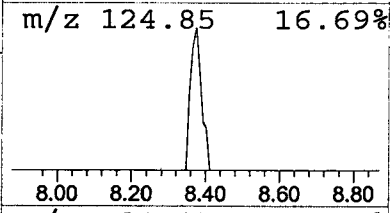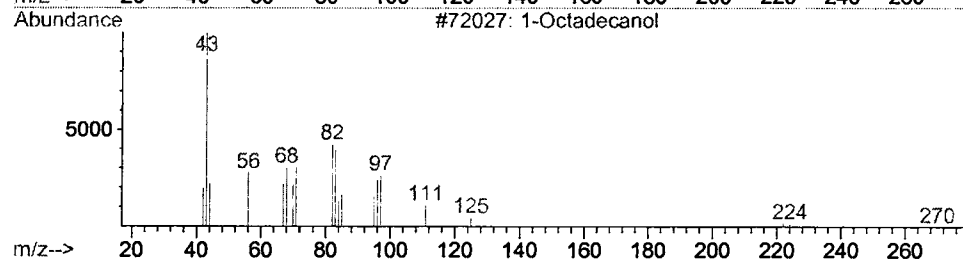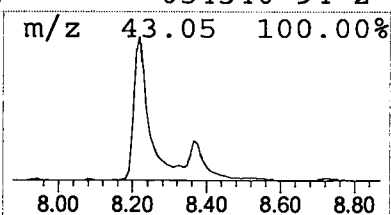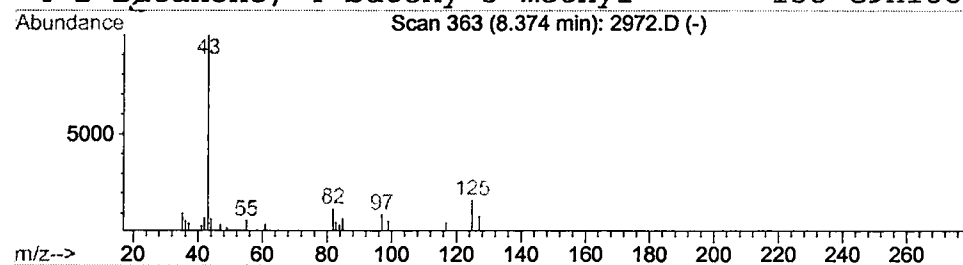

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 9 Feb 2002 7:19 pm
 Data File: C:\HPCHEM\1\DATA\FEB0802\2972.D
 Name: GC/MS SCAN 2/7
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Silane, tetramethyl-	8.22	2.4	ug/l	318721	ISTD01	12.35	2603880	20.0
1-Octadecanol	8.37	0.3	ug/l	41422	ISTD01	12.35	2603880	20.0

2972.D GCMS0208.M Wed Feb 13 11:12:16 2002