

Jser: Fakhouri, Morgan
 Westchester Dept. of Labs & Research
 Date: 03/04/2002 Time: 10:32:00

Sample: AE03017
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 3/4/02 10:29 Ended: 3/4/02 10:29 Analyst: MF
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	n-Nitrosodimethylamine		< MDL		2.0
2	bis(2-Chloroethyl)ether		< MDL		2.0
3	1,3-Dichlorobenzene		< MDL		2.0
4	1,4-Dichlorobenzene		< MDL		2.0
5	1,2-Dichlorobenzene		< MDL		2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL		2.0
7	n-Nitrosodi-n-propylamine		< MDL		2.0
8	Hexachloroethane		< MDL		2.0
9	Nitrobenzene		< MDL		2.0
10	Isophorone		< MDL		2.0
11	bis(2-Chloroethoxy)methane		< MDL		2.0
12	1,2,4-Trichlorobenzene		< MDL		2.0
13	Naphthalene		< MDL		2.0
14	Hexachlorobutadiene		< MDL		2.0
15	2-Chloronaphthalene		< MDL		2.0
16	Dimethylphthalate		< MDL		2.0
17	2,6-Dinitrotoluene		< MDL		2.0
18	Acenaphthylene		< MDL		2.0
19	Acenaphthene		< MDL		2.0
20	2,4-Dinitrotoluene		< MDL		2.0
21	Diethylphthalate		< MDL		2.0
22	4-Chlorophenylphenylether		< MDL		2.0
23	Fluorene		< MDL		2.0
24	Azobenzene/1,2-Diphenylhydraz		< MDL		2.0
25	n-Nitrosodiphenylamine		< MDL		2.0
26	4-Bromophenylphenylether		< MDL		2.0
27	Hexachlorobenzene		< MDL		2.0
28	Phenanthrene		< MDL		2.0
29	Anthracene		< MDL		2.0
30	Di-n-butylphthalate		< MDL		2.0
31	Fluoranthene		< MDL		2.0
32	Pyrene		< MDL		2.0
33	Butylbenzylphthalate		< MDL		2.0
34	Benzo(a)anthracene		< MDL		2.0
35	bis(2-Ethylhexyl)phthalate		< MDL		2.0
36	Chrysene		< MDL		2.0
37	Di-n-octylphthalate		< MDL		2.0
38	Benzo(b)fluoranthene		< MDL		2.0
39	Benzo(k)fluoranthene		< MDL		2.0
40	Benzo(a)pyrene		< MDL		2.0
41	Indeno(1,2,3-cd)pyrene		< MDL		2.0
42	Dibenz(a,h)anthracene		< MDL		2.0
43	Benzo(g,h,i)perylene		< MDL		2.0

Data File : C:\MSDCHEM\1\DATA\022802\212LBK.D

Vial: 5

Acq On : 1 Mar 2002 3:40 pm

Operator: McLean

Sample : 2/12/02 GC SCAN

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 04 05:53:56 2002

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.58	150	1380487	20.00	ug/L	0.00
10) Naphthalene-d8	13.05	136	3668906	20.00	ug/L	0.00
17) Acenaphthene-d10	18.17	164	2039133	20.00	ug/L	0.00
29) Phenanthrene-d10	22.52	188	3110142	20.00	ug/L	0.00
38) Chrysene-d12	30.34	240	2870671	20.00	ug/L	-0.02
44) Perylene-d12	34.21	264	1762064	20.00	ug/L	0.00

System Monitoring Compounds

37) 2,4-ddd surr	27.46	235	200154	4.05	ug/L	0.00
Spiked Amount	5.000		Recovery	=	81.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2 ' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	0.00	178	0	N.D.	
34) Anthracene	0.00	178	0	N.D.	
35) Di-n-butylphthalate	24.67	149	3050	0.01	ug/L 79
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo (a) anthracene	0.00	228	0	N.D.	d
42) Bis (2-ethylhexyl) phthala	30.94	149	16924	0.13	ug/L 90
43) Chrysene	0.00	228	0	N.D.	d
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo (b) fluoranthene	0.00	252	0	N.D.	

(#)= qualifier out of range (m) = manual integration

212LBK.D 5080202.M Mon Mar 04 05:54:23 2002

Page 1

Data File : C:\MSDCHEM\1\DATA\022802\212LBK.D Vial: 5
Acq On : 1 Mar 2002 3:40 pm Operator: McLean
Sample : 2/12/02 GC SCAN Inst : Instrumen
Misc : Multiplr: 1.00
MS Integration Params: BENZO.P
Quant Time: Mar 04 05:53:56 2002 Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Last Update : Mon Feb 25 19:17:14 2002
Response via : Initial Calibration
DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

212LBK.D 5080202.M Mon Mar 04 05:54:23 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\022802\212LBK.D

Acq On : 1 Mar 2002 3:40 pm

Sample : 2/12/02 GC SCAN

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 4 5:54 2002

Vial: 5

Operator: McLean

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080202.RES

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

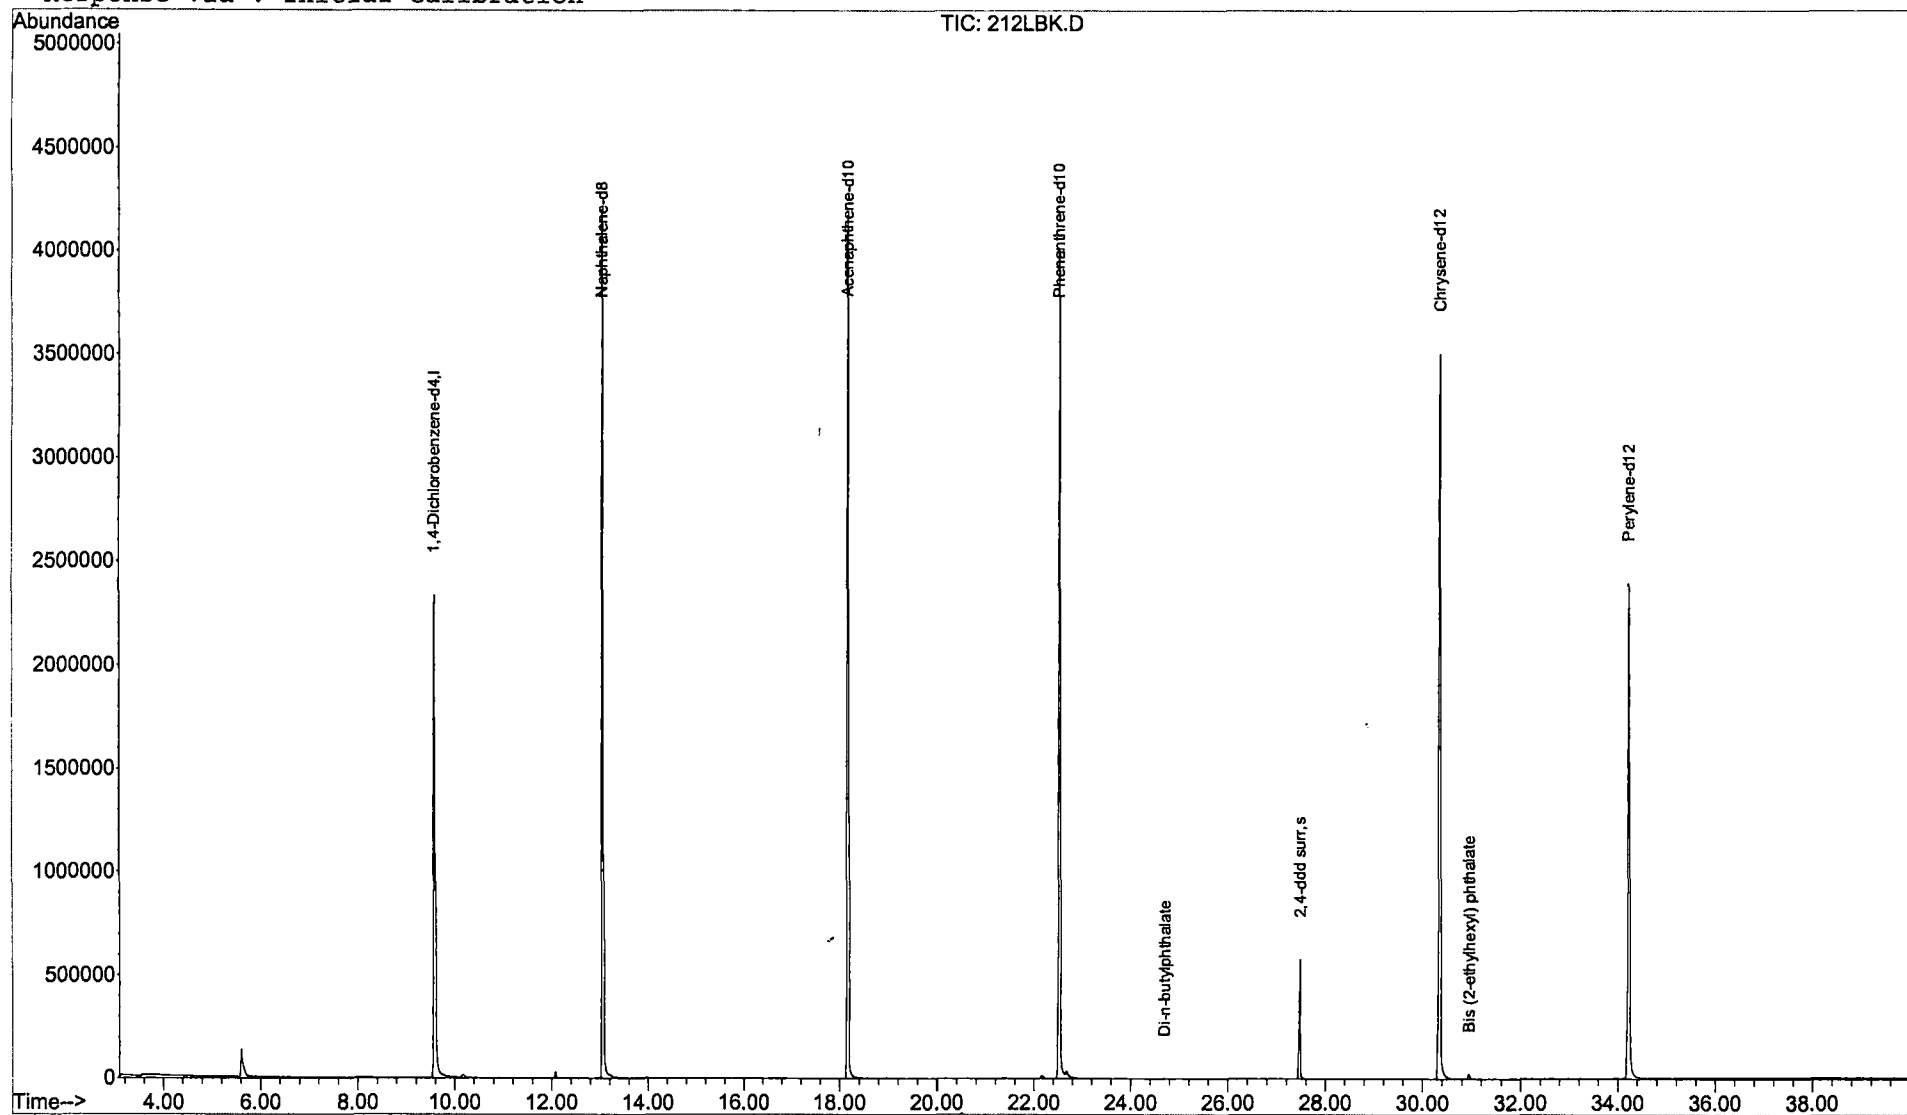

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\022802\212LBK.D

Acq On : 1 Mar 2002 3:40 pm

Sample : 2/12/02 GC SCAN

Misc :

MS Integration Params: LSCINT.P

Vial: 5

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF Filtering: 5

Sampling : 1 Min Area: 1 % of largest Peak

Start Thrs: 0.2 Max Peaks: 100

Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.597	275	278	293	rBV	132139	421752	4.93%	0.905%
2	9.579	712	717	738	rBV	2333303	5874580	68.63%	12.607%
3	13.053	1095	1100	1114	rBV	4201927	7910438	92.41%	16.975%
4	18.169	1657	1664	1676	rBV	4176872	8480978	99.08%	18.200%
5	22.522	2138	2144	2156	rBV2	4010966	8559780	100.00%	18.369%
6	22.677	2158	2161	2173	rVB3	30352	93457	1.09%	0.201%
7	27.457	2684	2688	2696	rBV	578289	1054746	12.32%	2.263%
8	30.341	2998	3006	3028	rBV	3506065	8402497	98.16%	18.031%
9	34.214	3425	3433	3451	rBV	2394723	5800975	67.77%	12.449%

Sum of corrected areas: 46599203

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\022802\212LBK.D
 Operator : McLean
 Acquired : 1 Mar 2002 3:40 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: 2/12/02 GC SCAN
 Misc Info :
 Vial Number: 5
 Quant File :5080202.RES (RTE Integrator)

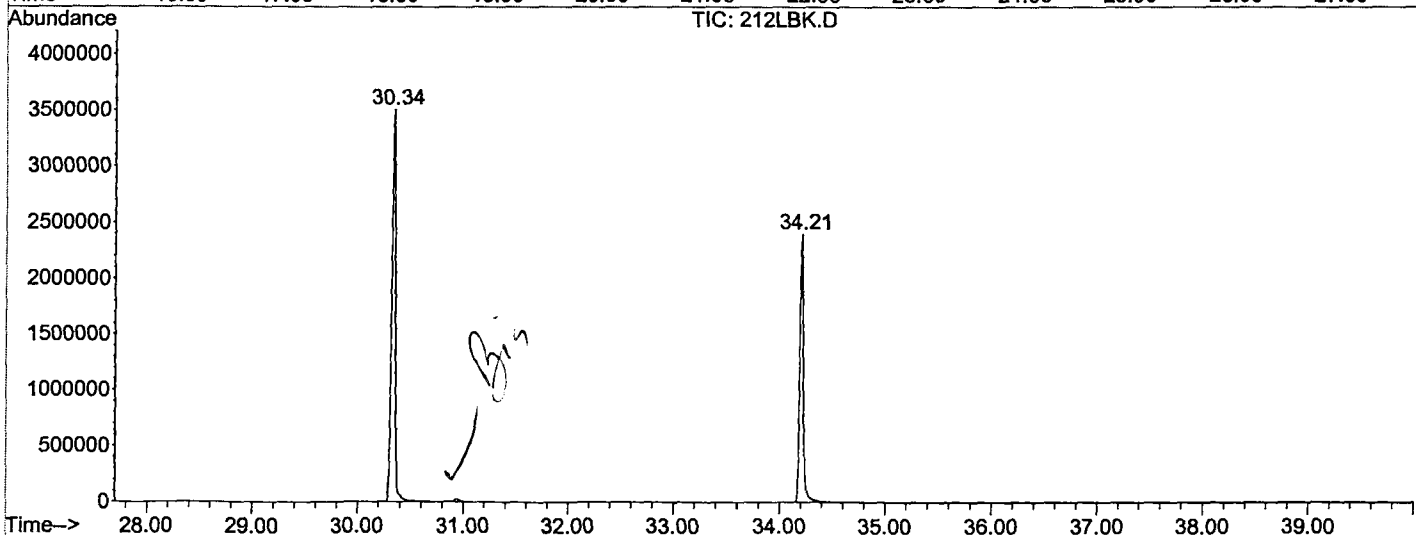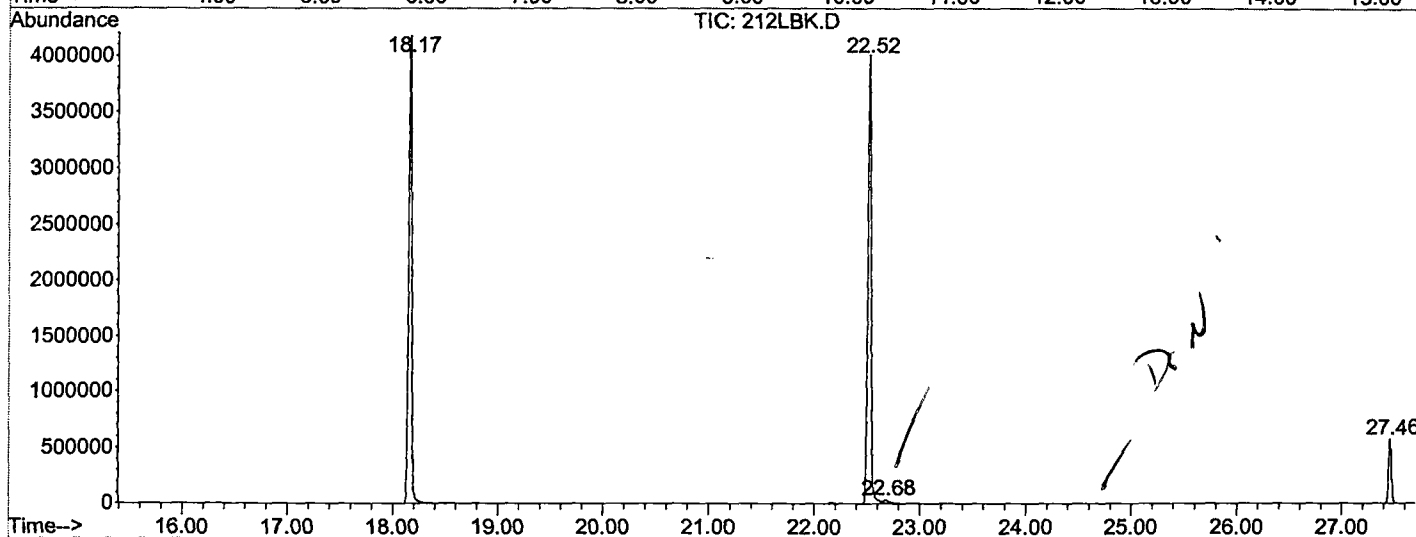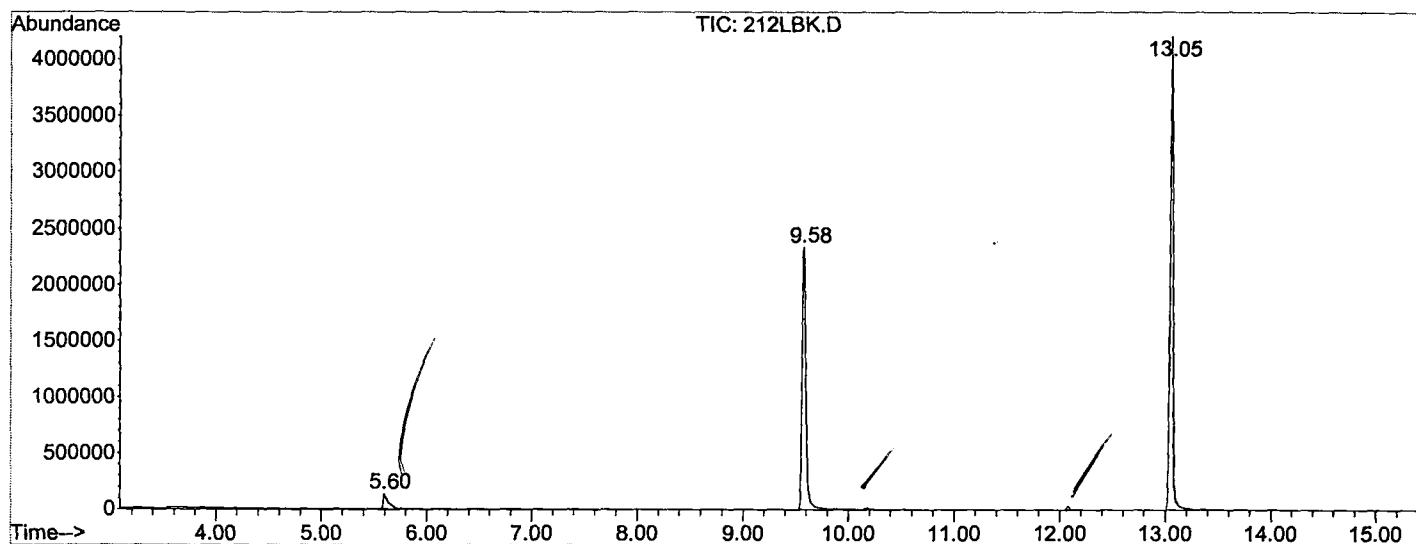

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\022802\212LBK.D

Acq On : 1 Mar 2002 3:40 pm

Sample : 2/12/02 GC SCAN

Misc :

MS Integration Params: LSCINT.P

Vial: 5

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)









Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Methane, isothiocyanato- (C... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.60	1.44 ug/L	421752	1,4-Dichlorobenzene-d4	9.58

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Methane, isothiocyanato- (CAS) \$...	73	C2H3NS	000556-61-6	9
2		Acetic acid, 3-[1,3]dioxolan-2-y...	174	C8H14O4	000000-00-0	9
3		Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
4		3-(CYCLOHEX-3'-EN-YL)PROPANOL \$\$...	174	C8H14O4	015745-87-6	9

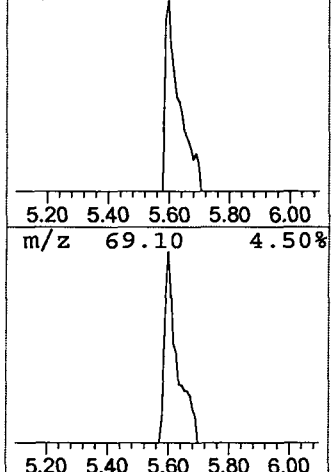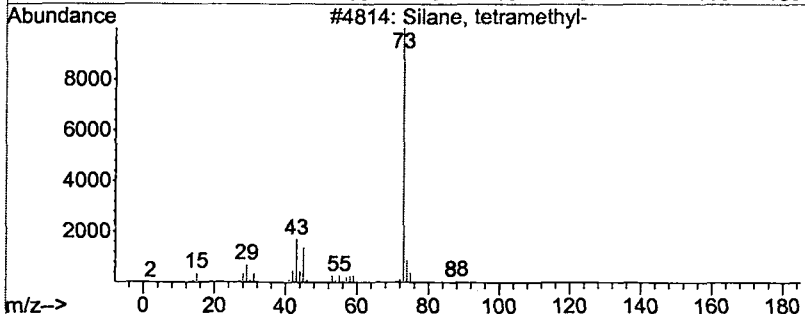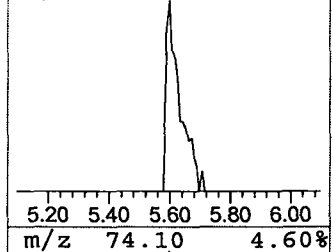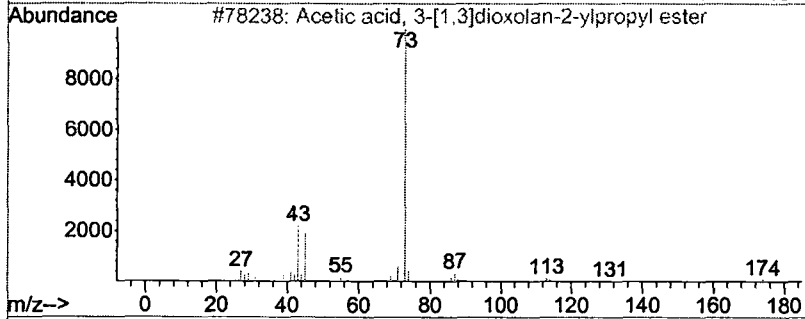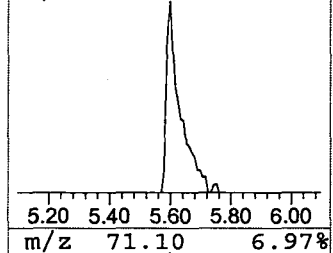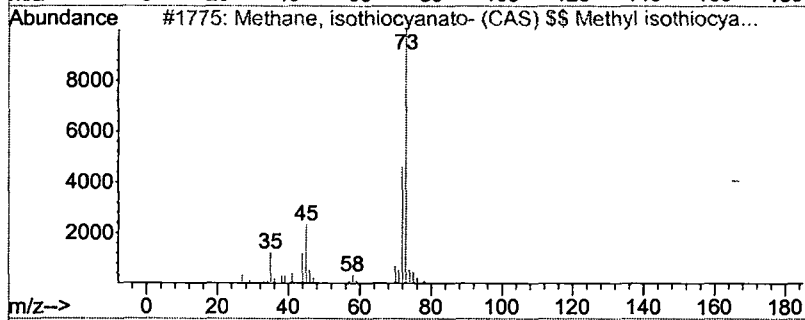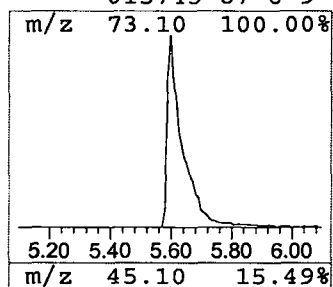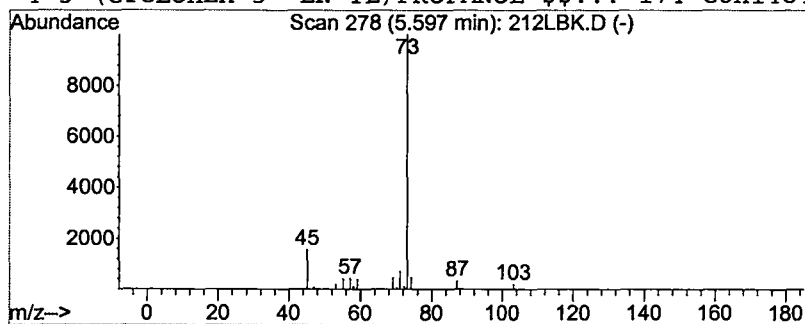

Operator ID: McLean Date Acquired: 1 Mar 2002 3:40 pm
 Data File: C:\MSDCHEM\1\DATA\022802\212LBK.D
 Name: 2/12/02 GC SCAN
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	#	--Internal Standard--		
						RT	Resp	Conc
Methane, isothioc...	5.60	1.4	ug/L	421752	1	9.58	5874580	20.0