

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 03/12/2002 Time: 15:07:12

Sample: AE03074
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 3/12/02 15:06 Ended: 3/12/02 15:06 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		-		
2	Surr_2,4-DDD		84		5.0

Comments for Sample AE03074 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-12-2002 Time: 15:07:17

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Data File : C:\MSDCHEM\1\DATA\022802\03074.D

Vial: 8

Acq On : 1 Mar 2002 6:07 pm

Operator: McLean

Sample : 2/12/02 GC SCAN

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 04 05:51:47 2002

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.58	150	1595255	20.00	ug/L	0.00
10) Naphthalene-d8	13.05	136	4153927	20.00	ug/L	0.00
17) Acenaphthene-d10	18.17	164	2320277	20.00	ug/L	0.00
29) Phenanthrene-d10	22.52	188	3515025	20.00	ug/L	0.00
38) Chrysene-d12	30.34	240	3234196	20.00	ug/L	-0.02
44) Perylene-d12	34.21	264	2149445	20.00	ug/L	0.00

System Monitoring Compounds

37) 2,4-ddd surr	27.46	235	233339	4.18	ug/L	0.00
Spiked Amount	5.000		Recovery	=	83.60%	

Target Compounds

						Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.		
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	0.00	128	0	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	0.00	149	0	N.D.		
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	24.67	149	5020	0.02	ug/L	79
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo (a) anthracene	30.34	228	8536	0.04	ug/L	46
42) Bis (2-ethylhexyl) phthala	30.94	149	19427	0.13	ug/L	97
43) Chrysene	0.00	228	0	N.D.	d	
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo (b) fluoranthene	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

03074.D 5080202.M Mon Mar 04 05:52:35 2002

Data File : C:\MSDCHEM\1\DATA\022802\03074.D

Vial: 8

Acq On : 1 Mar 2002 6:07 pm

Operator: McLean

Sample : 2/12/02 GC SCAN

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 04 05:51:47 2002

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.	.	
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

03074.D 5080202.M Mon Mar 04 05:52:35 2002

Data File : C:\MSDCHEM\1\DATA\022802\03074.D

Vial: 8

Acq On : 1 Mar 2002 6:07 pm

Operator: McLean

Sample : 2/12/02 GC SCAN

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 4 5:52 2002


Quant Results File: 5080202.RES

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

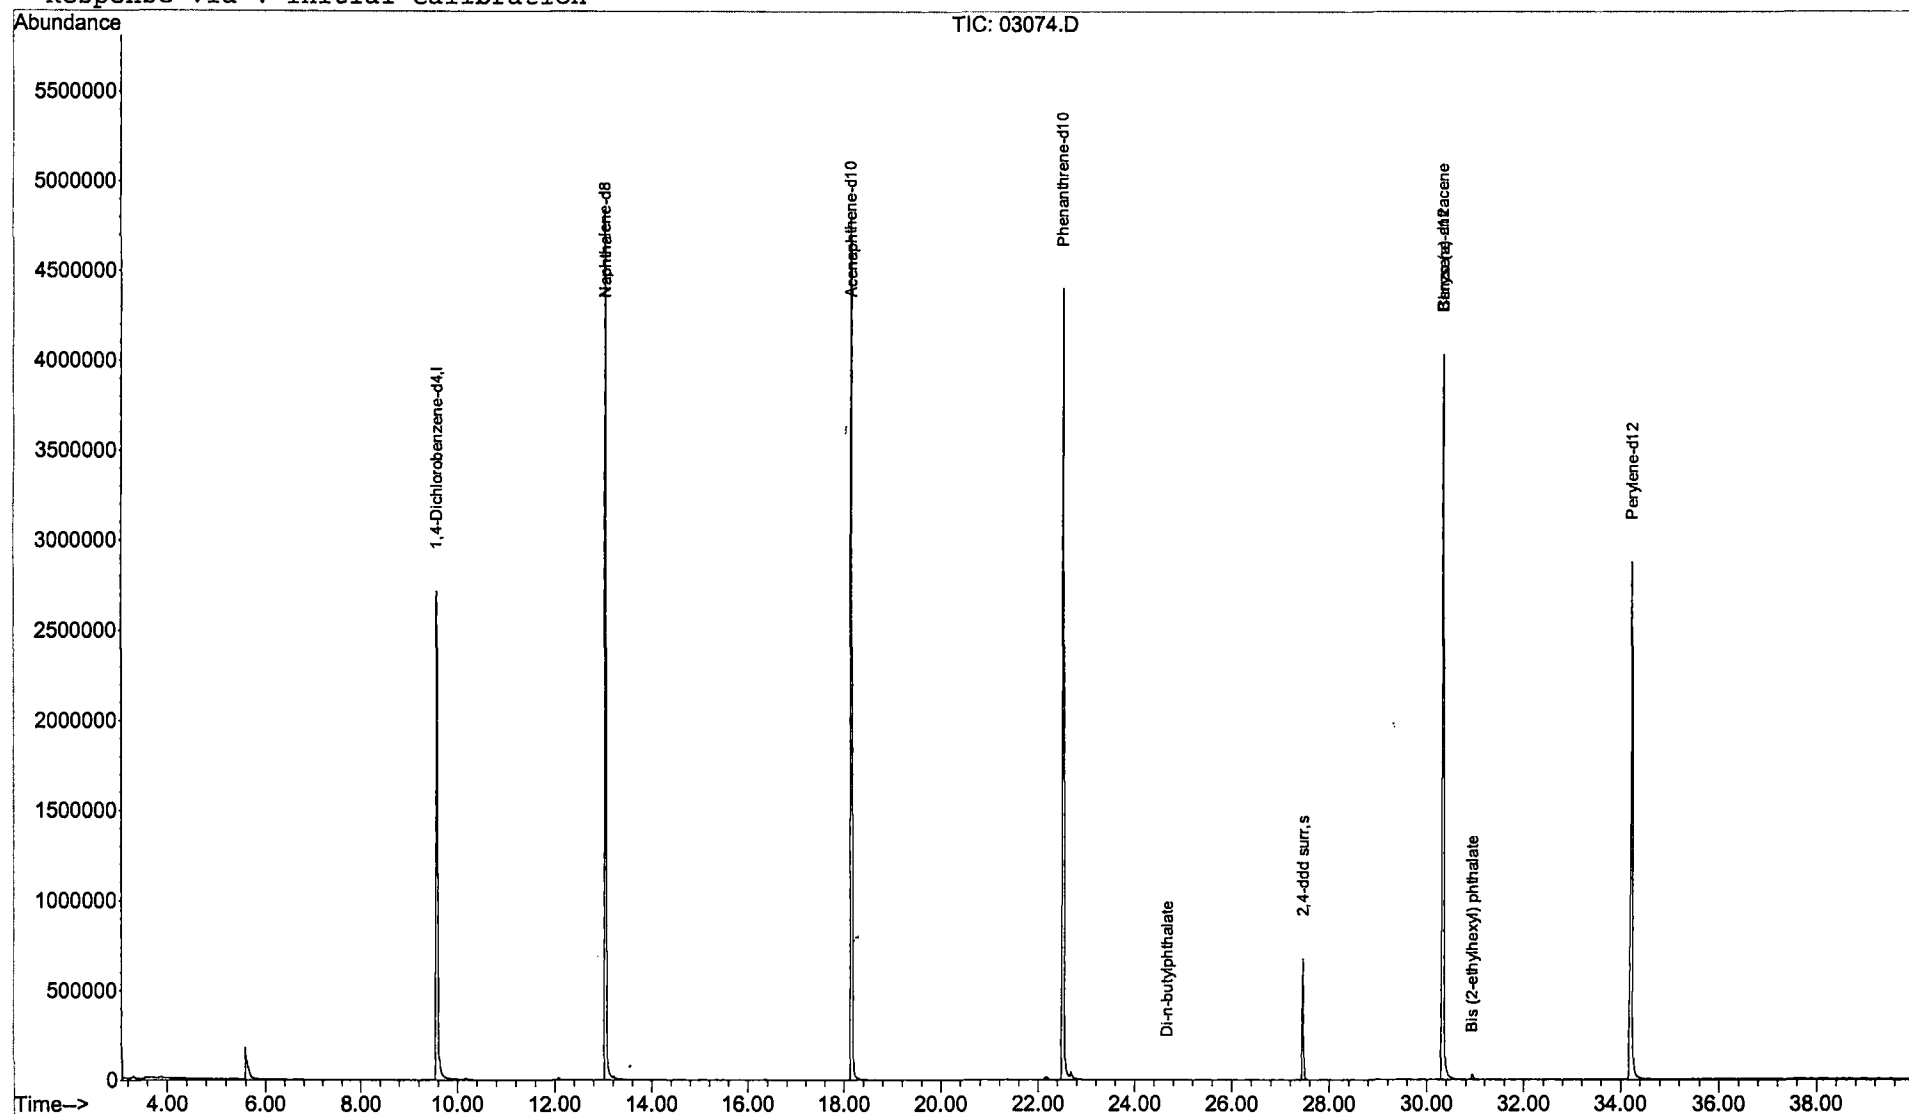

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\022802\03074.D

Vial: 8

Acq On : 1 Mar 2002 6:07 pm

Operator: McLean

Sample : 2/12/02 GC SCAN

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.597	275	278	294	rBV	174324	549397	5.68%	1.027%
2	9.579	711	717	740	rBV	2716221	6709691	69.37%	12.548%
3	13.053	1094	1100	1114	rBV	4841241	9014338	93.20%	16.857%
4	18.169	1657	1664	1678	rBV	4789345	9633566	99.60%	18.015%
5	22.523	2137	2144	2157	rBV2	4404207	9672012	100.00%	18.087%
6	22.677	2157	2161	2172	rVB	39137	121769	1.26%	0.228%
7	27.457	2683	2688	2699	rVB	675816	1231730	12.73%	2.303%
8	30.341	2998	3006	3028	rBV2	4039932	9525328	98.48%	17.813%
9	34.214	3425	3433	3448	rBV2	2879405	7016466	72.54%	13.121%

Sum of corrected areas: 53474297

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\022802\03074.D
 Operator : McLean
 Acquired : 1 Mar 2002 6:07 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: 2/12/02 GC SCAN
 Misc Info :
 Vial Number: 8
 Quant File : 5080202.RES (RTE Integrator)

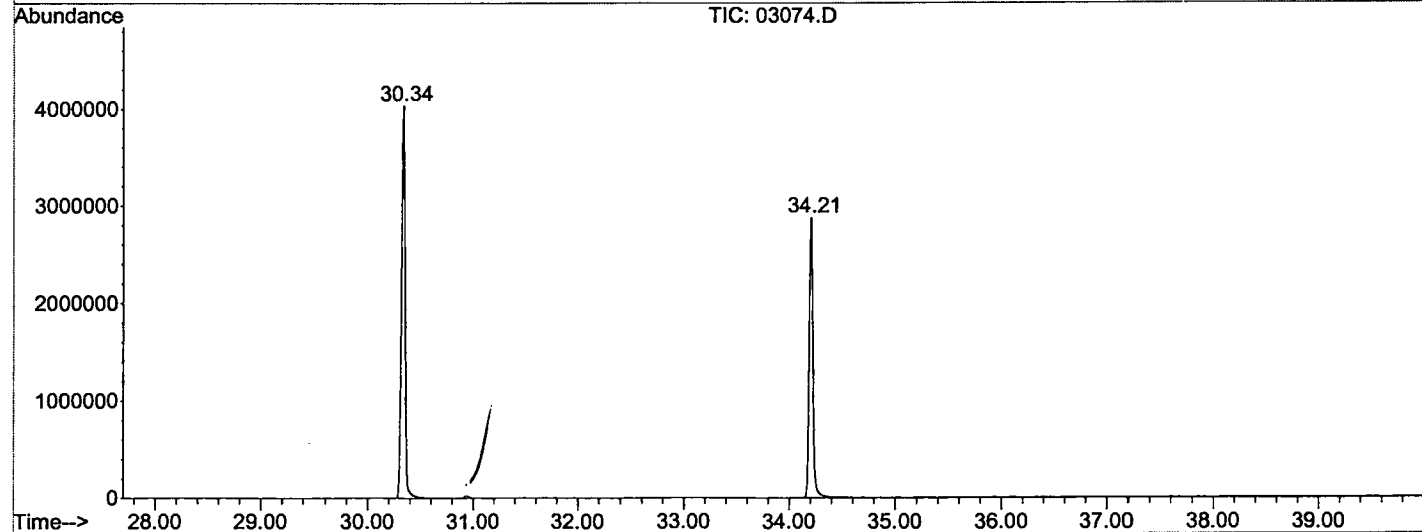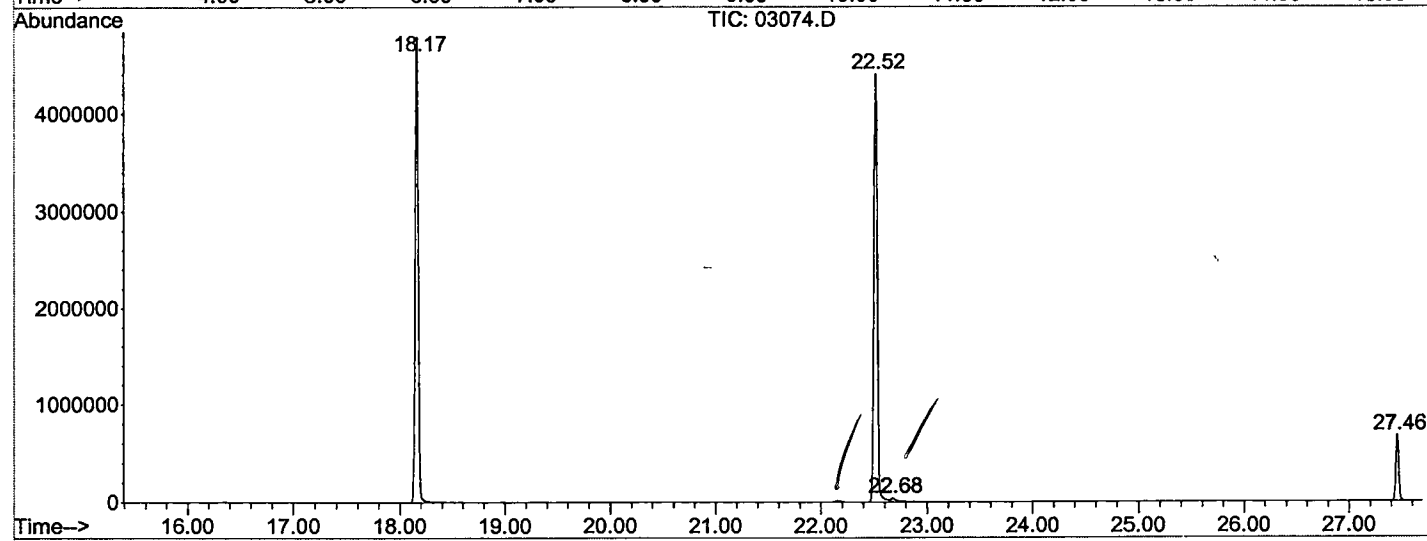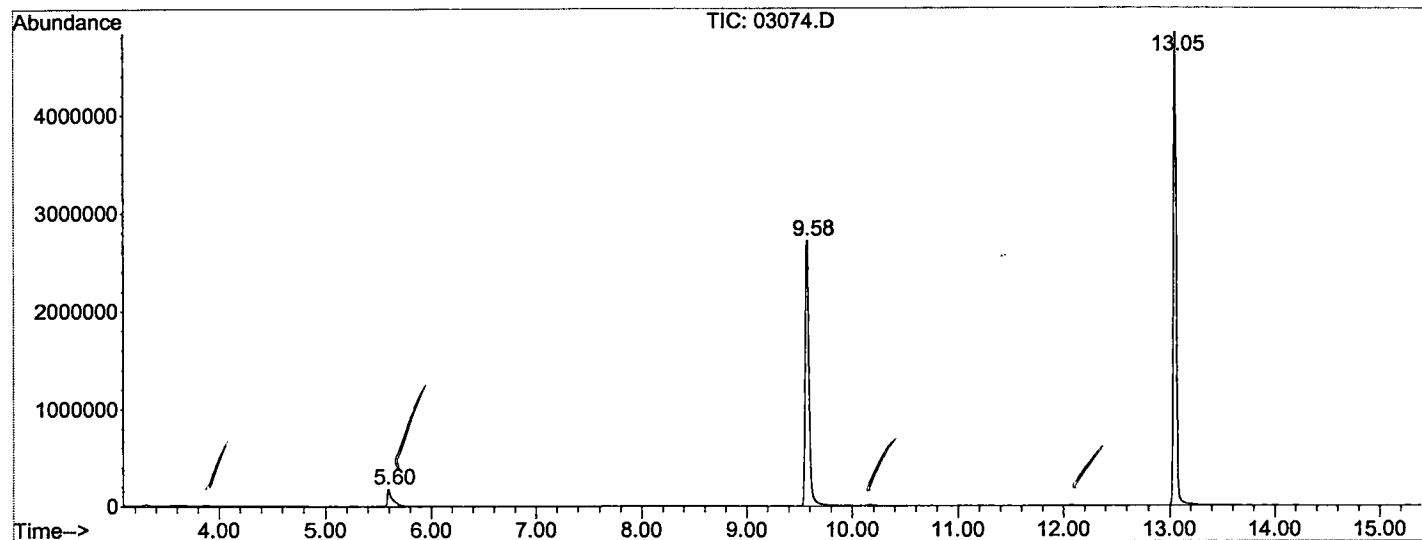

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\022802\03074.D

Acq On : 1 Mar 2002 6:07 pm

Sample : 2/12/02 GC SCAN

Misc :

MS Integration Params: LSCINT.P

Vial: 8

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Octanal, 7-methoxy-3,7-dime... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.60	1.64 ug/L	549397	1,4-Dichlorobenzene-d4	9.58

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Octanal, 7-methoxy-3,7-dimethyl-...	186	C11H22O2	003613-30-7	9
2		3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	9
3		Butane, 2-methoxy-2-methyl- \$\$ E...	102	C6H14O	000994-05-8	9
4		3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	9

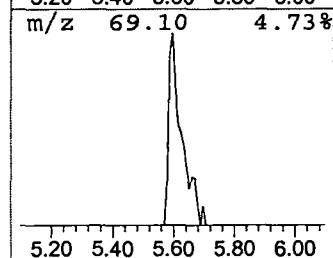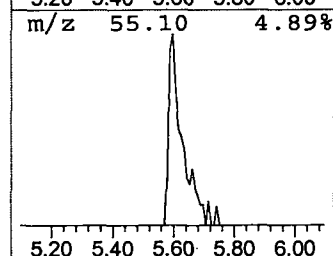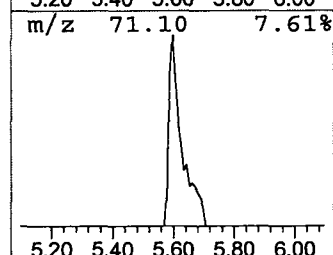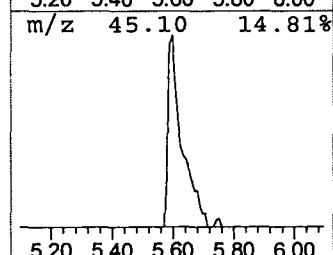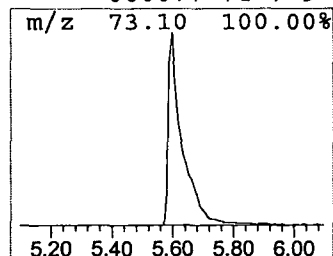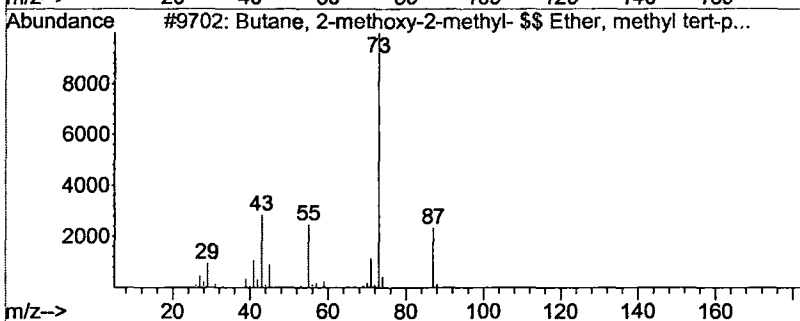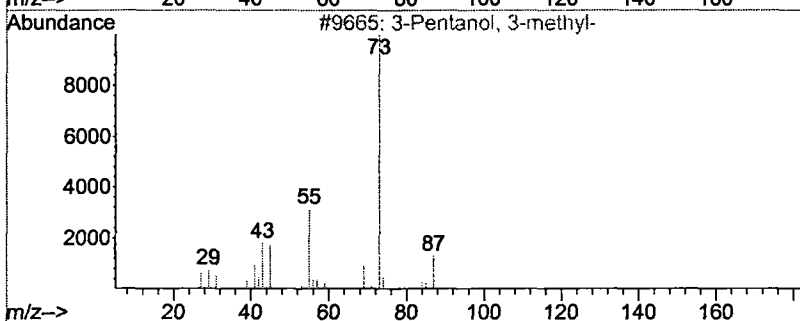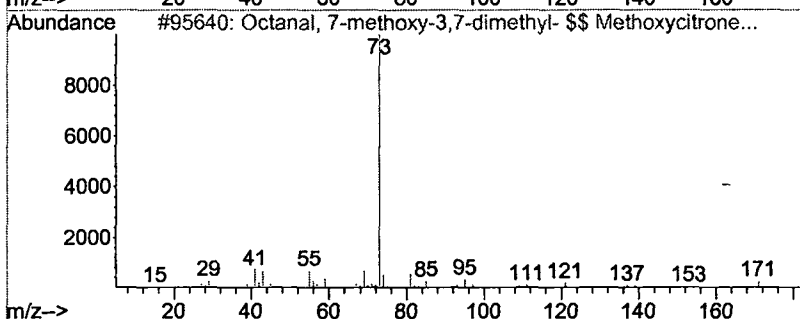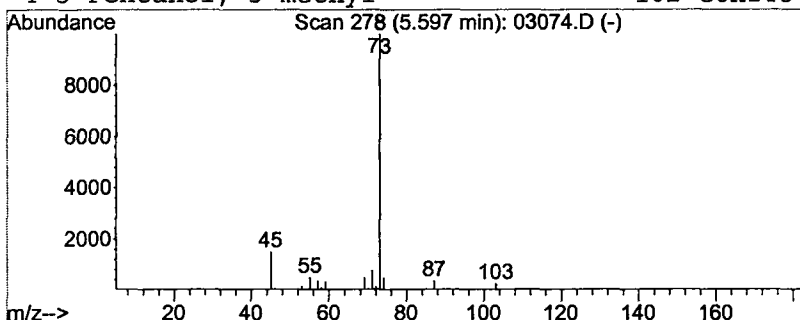

Tentatively Identified Compound (LSC) summary

Operator ID: McLean Date Acquired: 1 Mar 2002 6:07 pm
Data File: C:\MSDCHEM\1\DATA\022802\03074.D
Name: 2/12/02 GC SCAN
Misc:
Method: C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
Title: Quantitation For Method 508gcscan
Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Octanal, 7-methox...	5.60	1.6	ug/L	549397	1	9.58	6709690	20.0