

Method 508 MOD

Date Extracted 2-12-02

Page 81

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB.		500.00		1.00			1.00	6A	17			
Ref 1					1.00			2B				
Ref 2					1.00			9B				
3184								7A				
3185								6A				
3245								7A				
3246								9B				
3247								9A				
3248	F.B.							8B				
3249								10B				
3250								8A				
3251								8A				
3252								10A				
Remarks ① BATCH # 56005 - 17250 ② REF#2 ASSOCIATED W/ SAMPLE 03185 Reviewed by, <u>7/3/4/02</u> drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - <u>Sep. Fun</u> Solv. lot# <u>V41470</u> NaCl lot# <u>V39618</u> Na2SO4 lot# <u>V39400</u> STANDARD INT STD LOG# CALIBRATION REF SPIKE <u>91759</u> MDL/MDRF Q. CHECK INT. STD. SURROGATE <u>021202</u> LPC ENDRIN/DDT												

Analyst A.D.
revision 4/12/01

Verified by _____

Reviewed by DN
Date 3/15/02

DFTPP

Data File : C:\MSDCHEM\1\5973N\02MAR01\0301DF.D

Vial: 1

Acq On : 1 Mar 2002 8:25 am

Operator:

Sample : dftpp

Inst : Instrume


Misc : March 1, 2002

Multiplr: 1.00

MS Integration Params: SPLIT.P

Method : C:\MSDCHEM\1\METHODS\METHODS\HP022102.M (RTE Integrator)

Title : 508 scan method

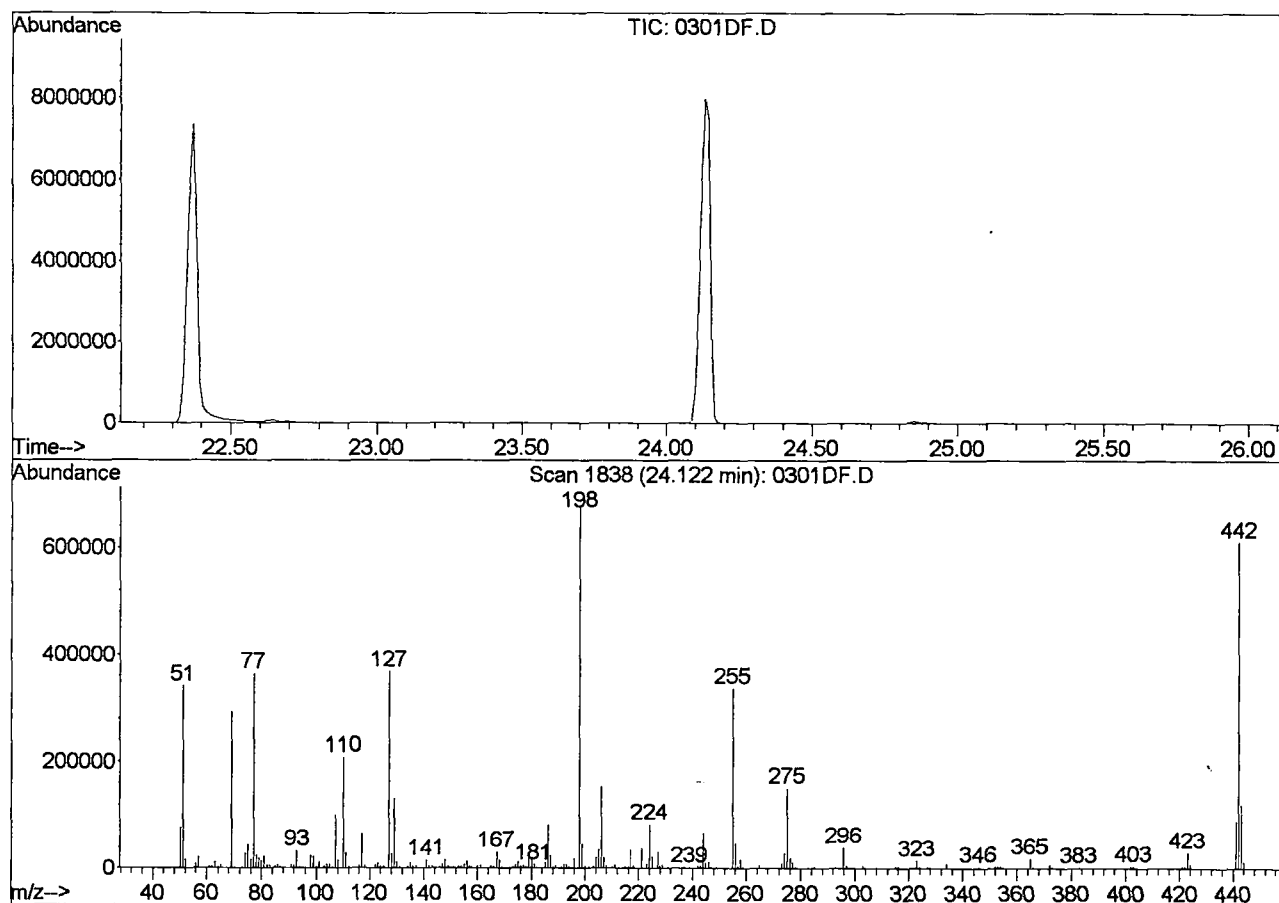

Spectrum Information: Scan 1838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	50.3	341632	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.3	294080	PASS
70	69	0.00	2	0.6	1715	PASS
127	198	40	60	54.4	369280	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	678656	PASS
199	198	5	9	6.9	46960	PASS
275	198	10	30	22.2	150912	PASS
365	198	1	99	2.6	17936	PASS
441	443	1	99	73.9	90128	PASS
442	198	40	110	90.1	611584	PASS
443	442	17	23	19.9	121968	PASS

0301DF.D HP022102.M

Fri Mar 01 09:56:49 2002