

Date Extracted 2-14-02

Page 86

\$GCMs-17307

Reviewed by,
C/B 6/4/02


Analyst A.D.
revision 4/12/01

Verified by my

Reviewed by [Signature]
Date 3/12/12

Data File : C:\HPCHEM\1\DATA\FEB2102\DFTPP3.D
 Acq On : 23 Feb 2002 9:29 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

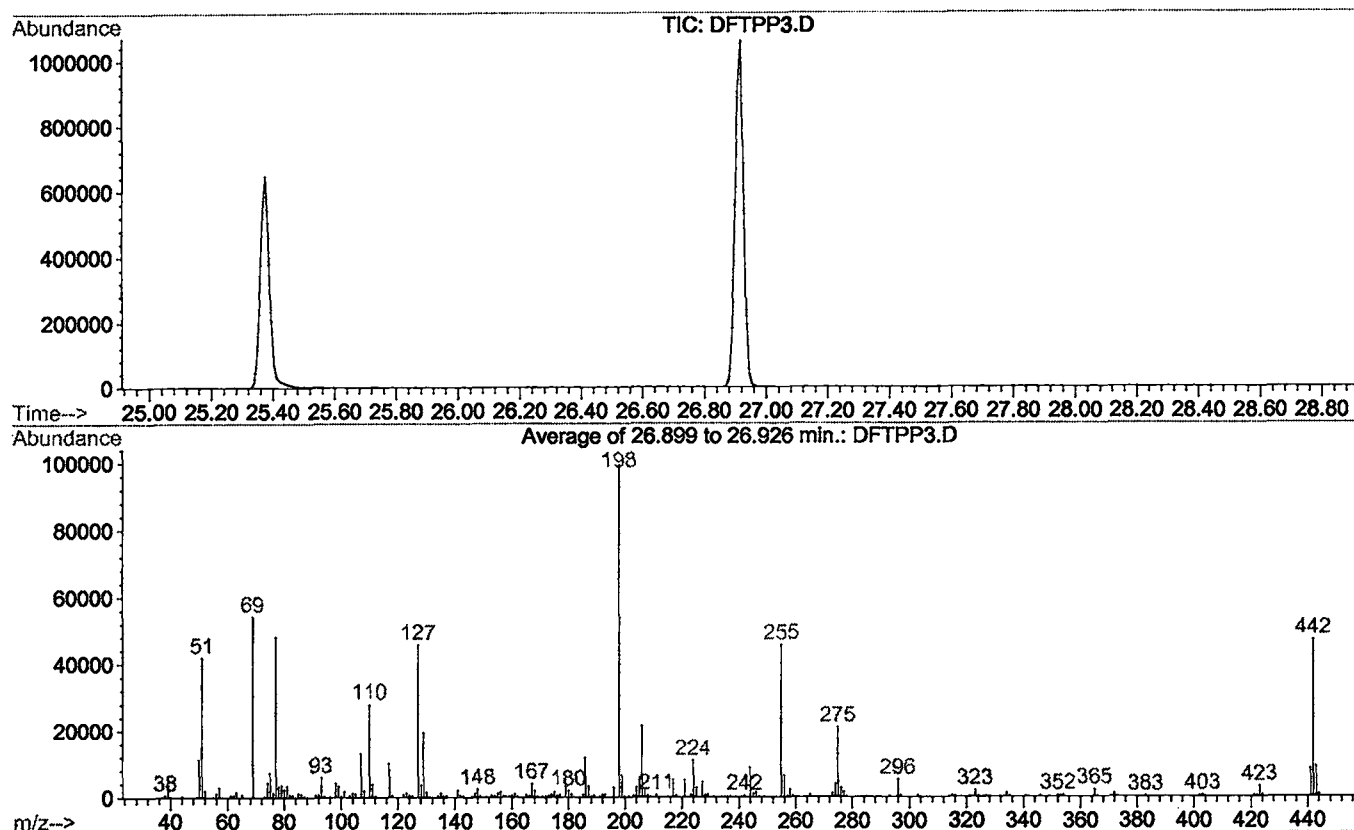

Spectrum Information: Average of 26.899 to 26.926 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	42.2	41914	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	54.6	54274	PASS
70	69	0.00	2	0.1	60	PASS
127	198	40	60	46.1	45798	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	99370	PASS
199	198	5	9	6.8	6718	PASS
275	198	10	30	21.2	21061	PASS
365	198	1	100	2.3	2237	PASS
441	443	0.01	100	91.3	8311	PASS
442	198	40	110	47.2	46952	PASS
443	442	17	23	19.4	9101	PASS

DFTPP3.D GCMS0208.M Fri Mar 08 09:02:41 2002