

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 02/20/2002 Time: 11:44:58

Sample: AE00892
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 2/20/02 11:44 Ended: 2/20/02 11:44 Analyst: MG
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	n-Nitrosodimethylamine		< MDL		2.0
2	bis(2-Chloroethyl)ether		< MDL		2.0
3	1,3-Dichlorobenzene		< MDL		2.0
4	1,4-Dichlorobenzene		< MDL		2.0
5	1,2-Dichlorobenzene		< MDL		2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL		2.0
7	n-Nitrosodi-n-propylamine		< MDL		2.0
8	Hexachloroethane		< MDL		2.0
9	Nitrobenzene		< MDL		2.0
10	Isophorone		< MDL		2.0
11	bis(2-Chloroethoxy)methane		< MDL		2.0
12	1,2,4-Trichlorobenzene		< MDL		2.0
13	Naphthalene		< MDL		2.0
14	Hexachlorobutadiene		< MDL		2.0
15	2-Chloronaphthalene		< MDL		2.0
16	Dimethylphthalate		< MDL		2.0
17	2,6-Dinitrotoluene		< MDL		2.0
18	Acenaphthylene		< MDL		2.0
19	Acenaphthene		< MDL		2.0
20	2,4-Dinitrotoluene		< MDL		2.0
21	Diethylphthalate		< MDL		2.0
22	4-Chlorophenylphenylether		< MDL		2.0
23	Fluorene		< MDL		2.0
24	Azobenzene/1,2-Diphenylhydraz		< MDL		2.0
25	n-Nitrosodiphenylamine		< MDL		2.0
26	4-Bromophenylphenylether		< MDL		2.0
27	Hexachlorobenzene		< MDL		2.0
28	Phenanthrene		< MDL		2.0
29	Anthracene		< MDL		2.0
30	Di-n-butylphthalate		< MDL		2.0
31	Fluoranthene		< MDL		2.0
32	Pyrene		< MDL		2.0
33	Butylbenzylphthalate		< MDL		2.0
34	Benzo(a)anthracene		< MDL		2.0
35	bis(2-Ethylhexyl)phthalate		< MDL		2.0
36	Chrysene		< MDL		2.0
37	Di-n-octylphthalate		< MDL		2.0
38	Benzo(b)fluoranthene		< MDL		2.0
39	Benzo(k)fluoranthene		< MDL		2.0
40	Benzo(a)pyrene		< MDL		2.0
41	Indeno(1,2,3-cd)pyrene		< MDL		2.0
42	Dibenz(a,h)anthracene		< MDL		2.0
43	Benzo(g,h,i)perylene		< MDL		2.0

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB1102\LBB.D
 Acq On : 12 Feb 2002 4:21 pm
 Sample : GC/MS SCAN 1/14
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Feb 12 17:10 2002

Vial: 30
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Feb 08 15:29:22 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.35	152	235125	20.00	ug/l	0.00
10) Naphthalene-d8	15.99	136	896074	20.00	ug/l	0.00
17) Acenaphthene-d10	21.31	164	474188	20.00	ug/l	0.00
29) Phenanthrene-d10	25.75	188	703271	20.00	ug/l	-0.02
38) Chrysene-d12	33.82	240	498946	20.00	ug/l	-0.02
44) Perylene-d12	38.11	264	319668	20.00	ug/l	-0.02

System Monitoring Compounds

37) 2,4-DDD	30.84	235	50905	5.82	ug/mL	0.34
Spiked Amount	5.000		Recovery	=	116.40%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.79	149	298	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#) = qualifier out of range (m) = manual integration

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB1102\LBB.D

Vial: 30

Acq On : 12 Feb 2002 4:21 pm

Operator: 209 GALOS

Sample : GC/MS SCAN 1/14

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 12 17:10 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Feb 08 15:29:22 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	25.76	178	181	N.D.	
34) Anthracene	25.76	178	181	N.D.	
35) Di-n-butylphthalate	27.72	149	2312	N.D.	
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	30.13	202	229	N.D.	
40) Butylbenzylphthalate	32.25	149	600	N.D.	
41) Benzo(a)anthracene	33.89	228	4615	N.D.	
42) Bis(2-ethylhexyl)phthalate	34.02	149	2460	N.D.	
43) Chrysene	33.89	228	4448	N.D.	
45) Di-n-Octylphthalate	35.77	149	1332	N.D.	
46) Benzo(b)fluoranthene	36.90	252	2026	N.D.	
47) Benzo(k)fluoranthene	36.97	252	2928	N.D.	
48) Benzo(a)pyrene	37.90	252	1183	N.D.	
49) Indeno(1,2,3-cd)pyrene	42.35	276	218	N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
51) Benzo(g,h,i)perylene	43.63	276	837	N.D.	

(#) = qualifier out of range (m) = manual integration

LBB.D GCMS0208.M

Tue Feb 19 15:28:53 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\FEB1102\LBB.D
Acq On : 12 Feb 2002 4:21 pm
Sample : GC/MS SCAN 1/14
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 12 17:10 2002

Vial: 30
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 13 11:43:23 2002
Response via : Initial Calibration

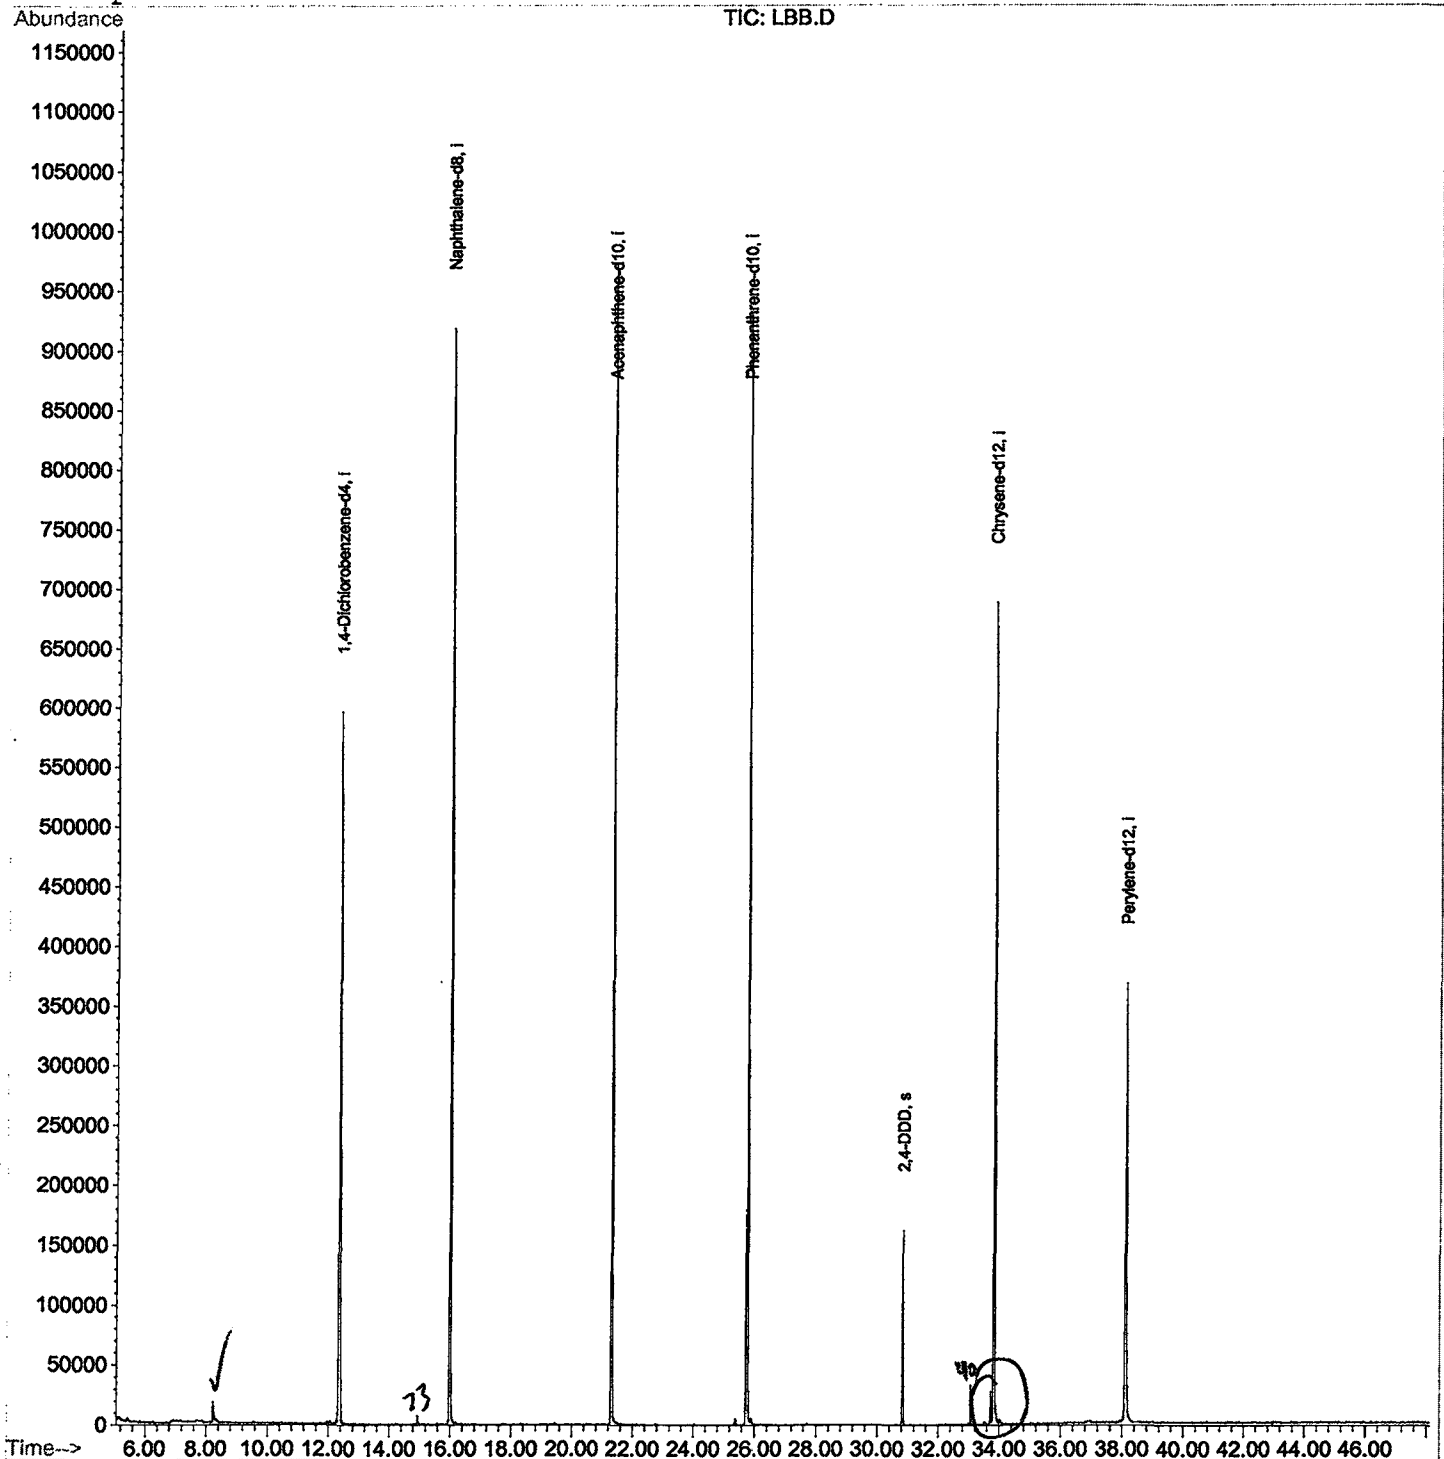

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB1102\LBB.D
 Acq On : 12 Feb 2002 4:21 pm
 Sample : GC/MS SCAN 1/14
 Misc :
 MS Integration Params: LSCINT.P

Vial: 30
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.226	X 343	347	354	rBV	17403	44503	2.26%	0.431%
2	12.348	✓ 790	796	811	rVB	595764	1517427	77.11%	14.689%
3	15.992	✓ 1187	1193	1206	rBV	917982	1863897	94.71%	18.043%
4	21.308	✓ 1766	1772	1785	rBV	972861	1967928	100.00%	19.050%
5	25.751	✓ 2250	2256	2267	rBV2	929857	1951082	99.14%	18.887%
6	30.837	✓ 2805	2810	2815	rVB	162214	313861	15.95%	3.038%
7	33.720	X 3120	3124	3127	rBV	27452	45747	2.32%	0.443%
8	33.821	✓ 3129	3135	3152	rVB	687895	1529754	77.73%	14.809%
9	38.108	✓ 3594	3602	3621	rVB2	366135	1095968	55.69%	10.609%

methoxychlor




Sum of corrected areas: 10330167

LBB.D GCMS0208.M

Wed Feb 20 09:55:56 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB1102\LBB.D
 Operator : 209 GALOS
 Acquired : 12 Feb 2002 4:21 pm using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: GC/MS SCAN 1/14
 Misc Info :
 Vial Number: 30
 Quant File :GCMS0208.RES (RTE Integrator)

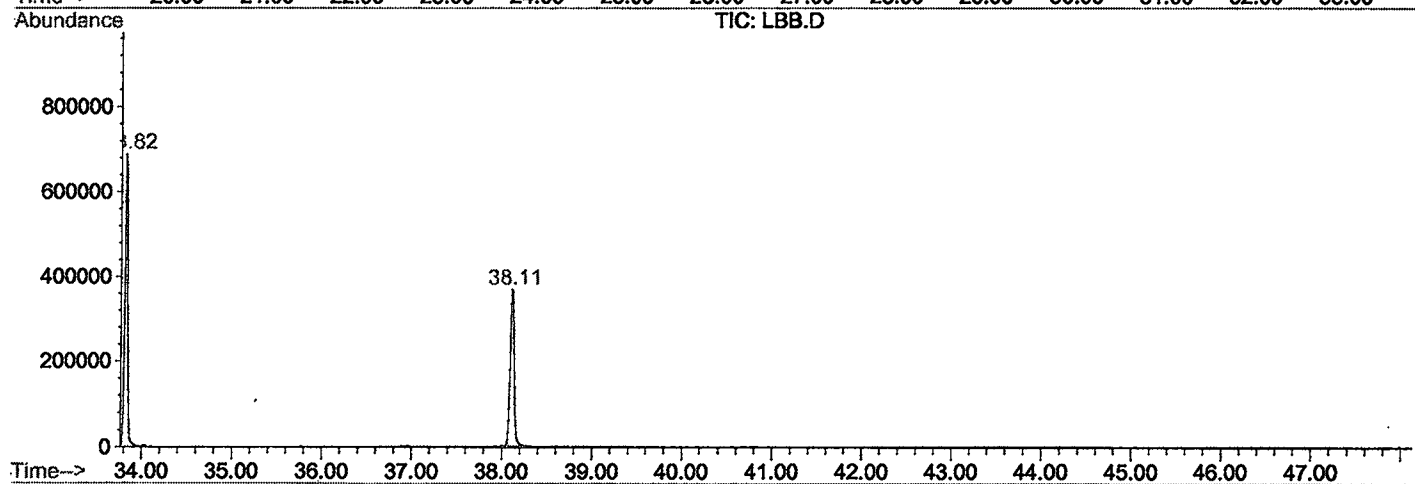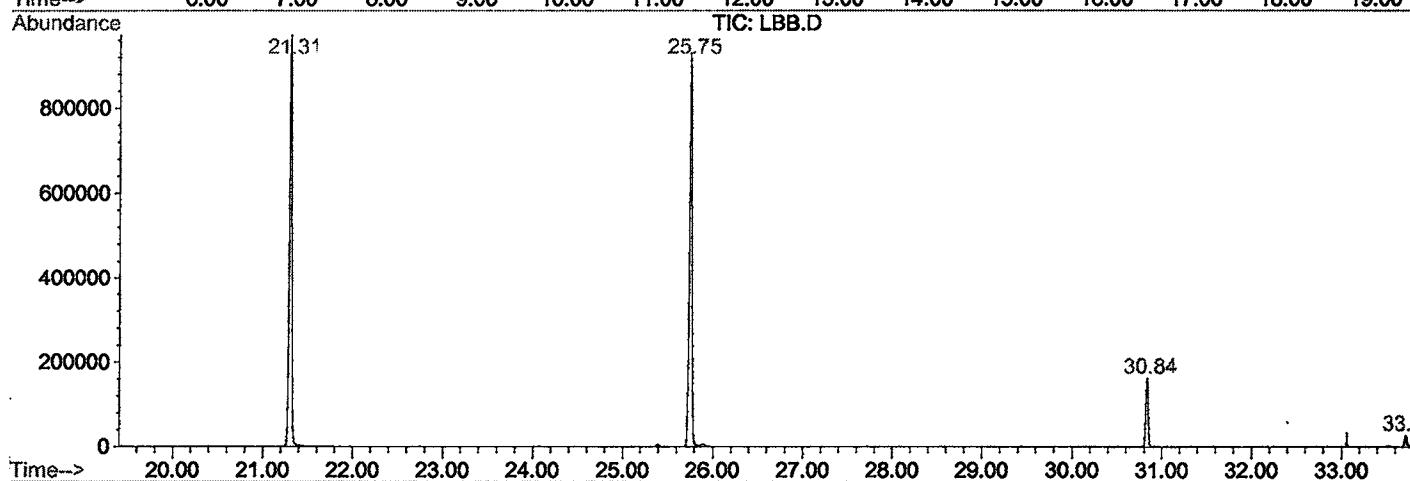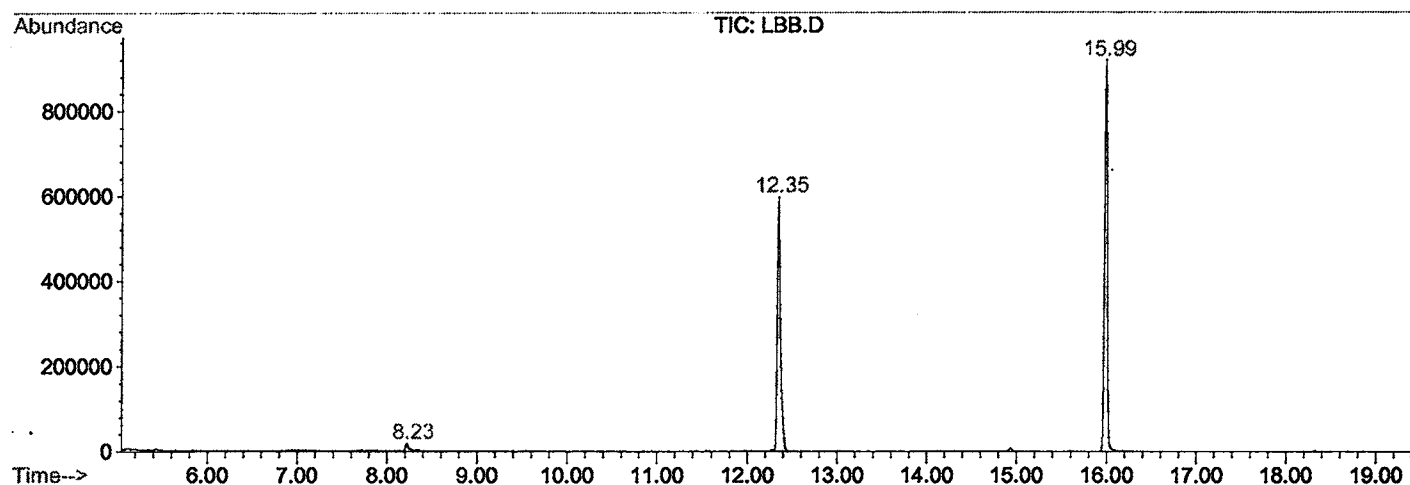

LBB.D GCMS0208.M

Wed Feb 20 09:56:01 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB1102\LBB.D
Acq On : 12 Feb 2002 4:21 pm
Sample : GC/MS SCAN 1/14
Misc :
MS Integration Params: LSCINT.P


Vial: 30
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 3-Pentanol, 3-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.23	0.59 ug/l	44503	1,4-Dichlorobenzene-d4	12.35

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	33
2			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

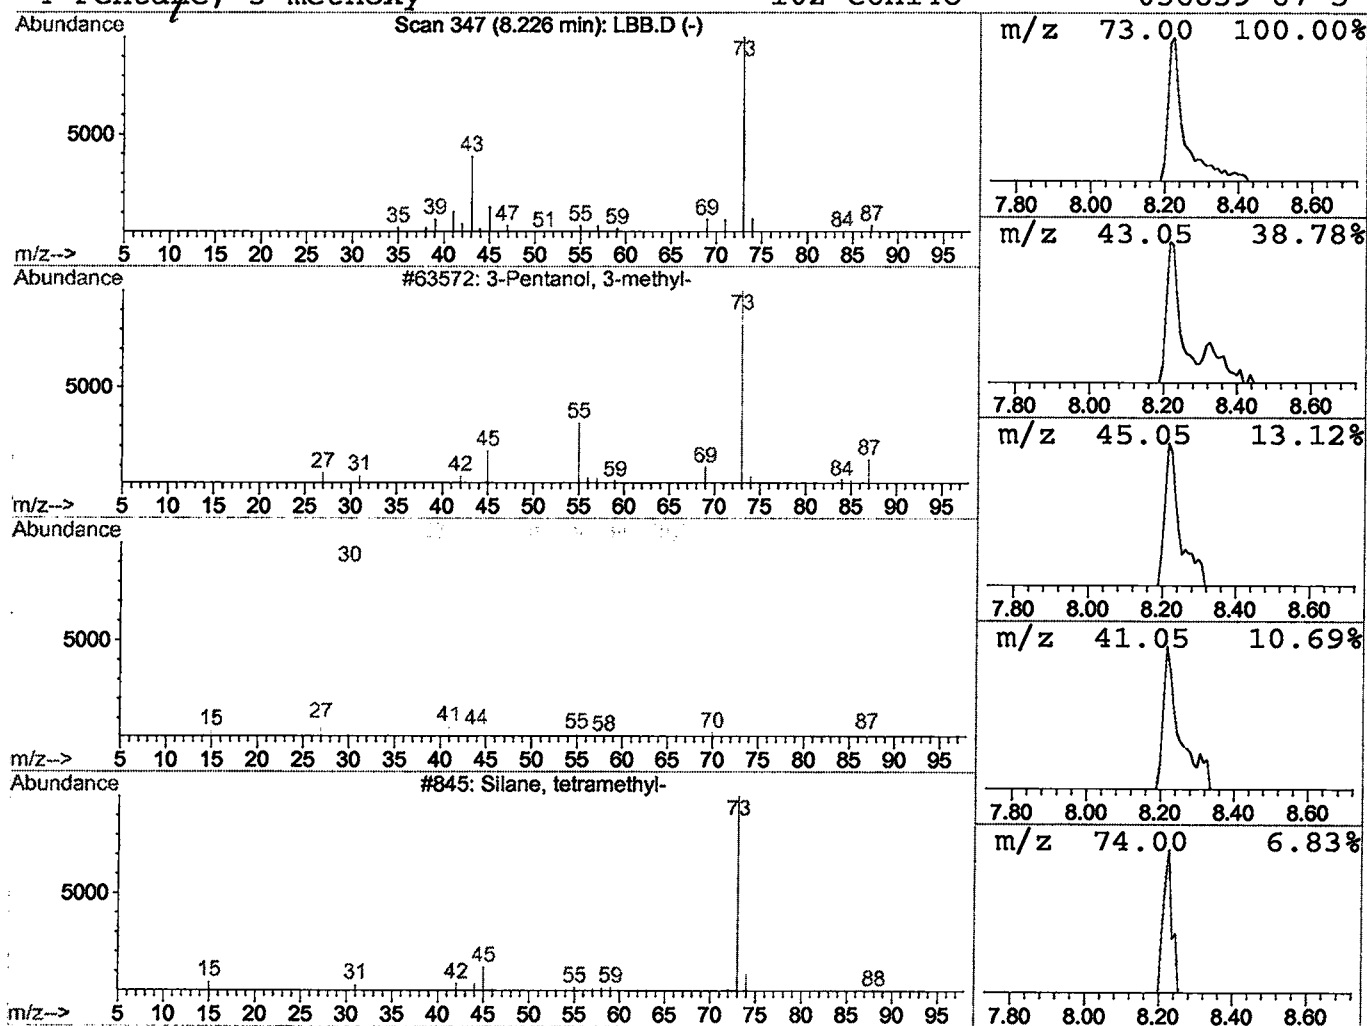

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB1102\LBB.D
 Acq On : 12 Feb 2002 4:21 pm
 Sample : GC/MS SCAN 1/14
 Misc :
 MS Integration Params: LSCINT.P










Vial: 30
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Methoxychlor Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
33.72	0.60 ug/l	45747	Chrysene-d12	33.82

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Methoxychlor	344	C16H15Cl3O2	000072-43-5	90	
2	Phenol, 4-[[(4-methoxyphenyl)methyl	227	C14H13NO2	003230-39-5	64	
3	Benzoic acid, 3-(phenylamino)-, met	227	C14H13NO2	055622-43-0	42	
4	S-Indacene, 1,2,3,5,6,7-hexahydro-1	242	C18H26	017465-58-6	38	

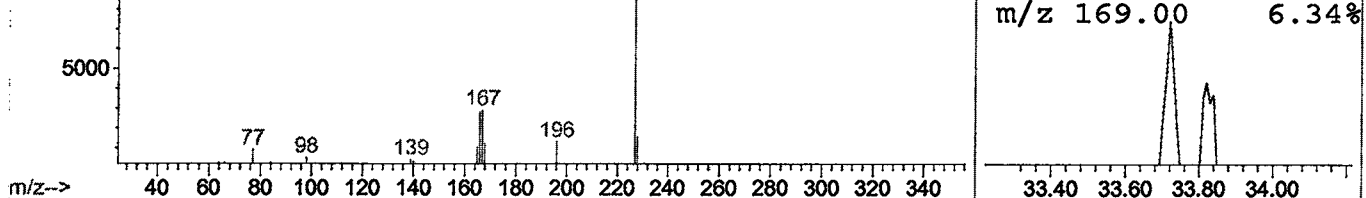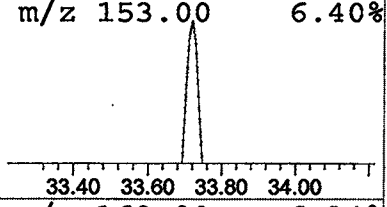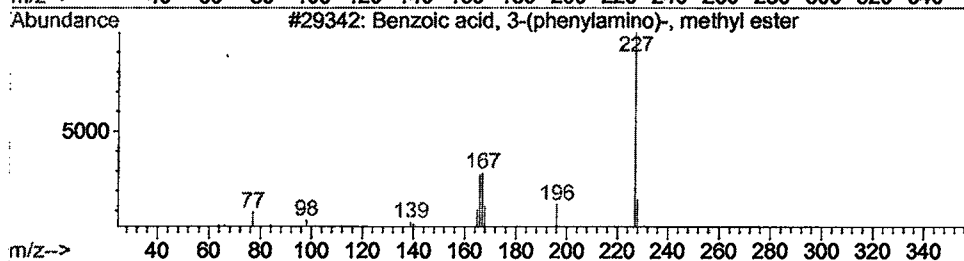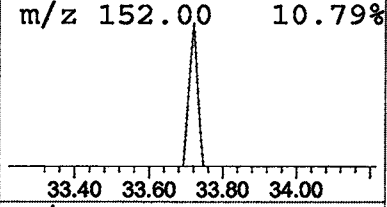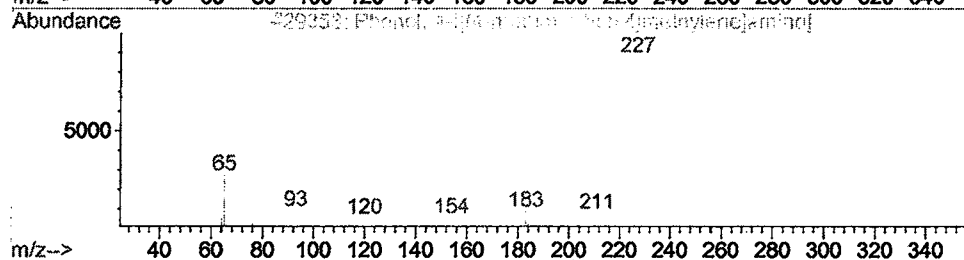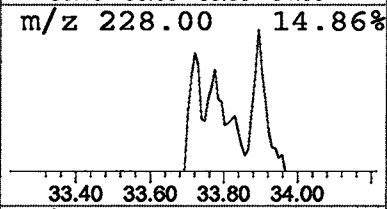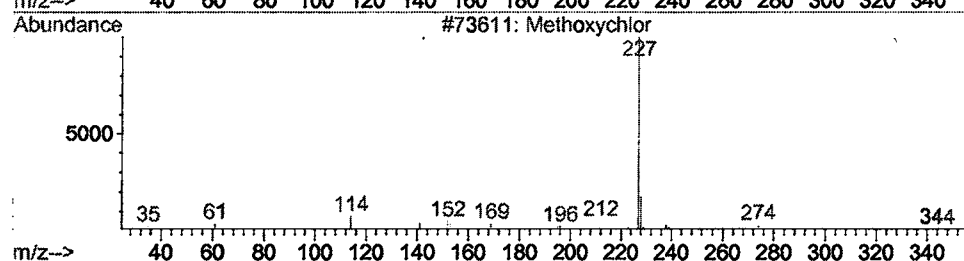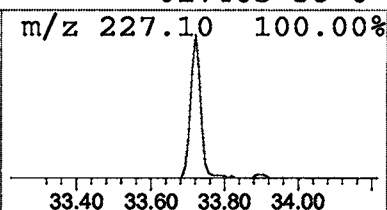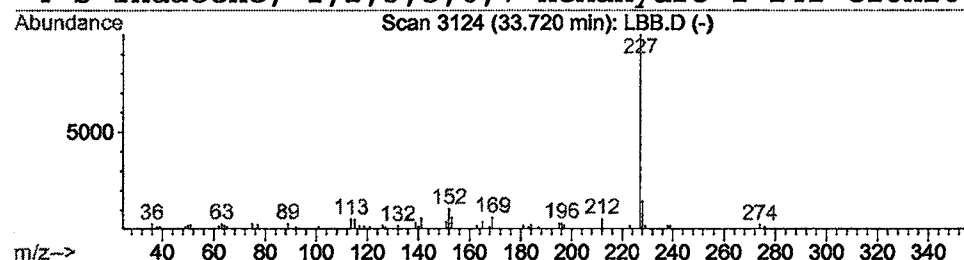

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 12 Feb 2002 4:21 pm
 Data File: C:\HPCHEM\1\DATA\FEB1102\LBB.D
 Name: GC/MS SCAN 1/14
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
3-Pentanol, 3-methyl	8.23	0.6	ug/l	44503	ISTD01	12.35	1517430	20.0
Methoxychlor	33.72	0.6	ug/l	45747	ISTD05	33.82	1529750	20.0

LBB.D GCMS0208.M Wed Feb 20 09:56:30 2002