

Method 508 mod

Date Extracted 1/17/02

Page 38

REF

#GMS-17043

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500mL		1mL			1mL	6B	7			
REF					5mL			9A				
1224								7B				
1223								8A				
1221								8B				
1220								6B				
1230								10A				
1231								7A				
1232								10B				
1227								6A				
1233								9B				
Remarks												
Reviewed by, <u>JB 8/12/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type - <u>Sep fun</u> Solv. lot# <u>V39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39400</u>												
STANDARD	INT STD LOG#											
CALIBRATION	<u>HP01302</u>											
REF SPIKE	<u>91759</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>3110320 2/15</u>											
SURROGATE	<u>GMS</u>											
LPC												
ENDRIN/DDT												

Analyst EH/LF
revision 4/12/01

Verified by my

Reviewed by DW
Date 2/25/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\FEB1502.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\feb1502\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch

(X) Full Method (X) Inject Anyway

() Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0208	
2	Sample	2	CAL10	GCMS0208	
3	Sample	3	LB	GCMS0208	gc/ms scan 1/16
4	Sample	4	REF	GCMS0208	gc/ms scan 1/16
5	Sample	5	1143	GCMS0208	gc/ms scan 1/16
6	Sample	6	1156	GCMS0208	gc/ms scan 1/16
7	Sample	7	1153	GCMS0208	gc/ms scan 1/16
8	Sample	8	1155	GCMS0208	gc/ms scan 1/16
9	Sample	9	1154	GCMS0208	gc/ms scan 1/16
10	Sample	10	1137	GCMS0208	gc/ms scan 1/16
11	Sample	11	LBA	GCMS0208	gc/ms scan 2/15
12	Sample	12	REFA	GCMS0208	gc/ms scan 2/15
13	Sample	13	REFA2	GCMS0208	gc/ms scan 2/15
14	Sample	14	1940	GCMS0208	re-extract
15	Sample	15	1941	GCMS0208	re-extract
16	Sample	16	1943	GCMS0208	re-extract
17	Sample	17	3438	GCMS0208	gc/ms scan 2/15
18	Sample	18	3439	GCMS0208	gc/ms scan 2/15
19	Sample	19	3440	GCMS0208	gc/ms scan 2/15
20	Sample	20	3441	GCMS0208	gc/ms scan 2/15
21	Sample	21	3454	GCMS0208	gc/ms scan 2/15
22	Sample	22	3471	GCMS0208	gc/ms scan 2/15
23	Sample	23	3472	GCMS0208	gc/ms scan 2/15
24	Sample	1	DFTPP1	GCMS0208	gc/ms scan 2/15
25	Sample	2	CAL10A	GCMS0208	gc/ms scan 2/15
26	Sample	24	LBB	GCMS0208	gc/ms scan 1/17
27	Sample	25	REFB	GCMS0208	gc/ms scan 1/17
28	Sample	26	1226	GCMS0208	gc/ms scan 1/17
29	Sample	27	1225	GCMS0208	gc/ms scan 1/17
30	Sample	28	1222	GCMS0208	gc/ms scan 1/17
31	Sample	29	1043	GCMS0208	gc/ms scan 1/17
32	Sample	30	1041	GCMS0208	gc/ms scan 1/17
33	Sample	31	LBC	GCMS0208	gc/ms scan 1/17
34	Sample	32	REFC	GCMS0208	gc/ms scan 1/17
35	Sample	33	1224	GCMS0208	gc/ms scan 1/17
36	Sample	34	1223	GCMS0208	gc/ms scan 1/17
37	Sample	35	1221	GCMS0208	gc/ms scan 1/17
38	Sample	36	1220	GCMS0208	gc/ms scan 1/17
39	Sample	37	1230	GCMS0208	gc/ms scan 1/17
40	Sample	38	1231	GCMS0208	gc/ms scan 1/17
41	Sample	39	1232	GCMS0208	gc/ms scan 1/17
42	Sample	40	1227	GCMS0208	gc/ms scan 1/17


Last Modified: Mon Feb 18 10:57:17 2002

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB1802\DFTPP.D
 Acq On : 18 Feb 2002 12:14 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

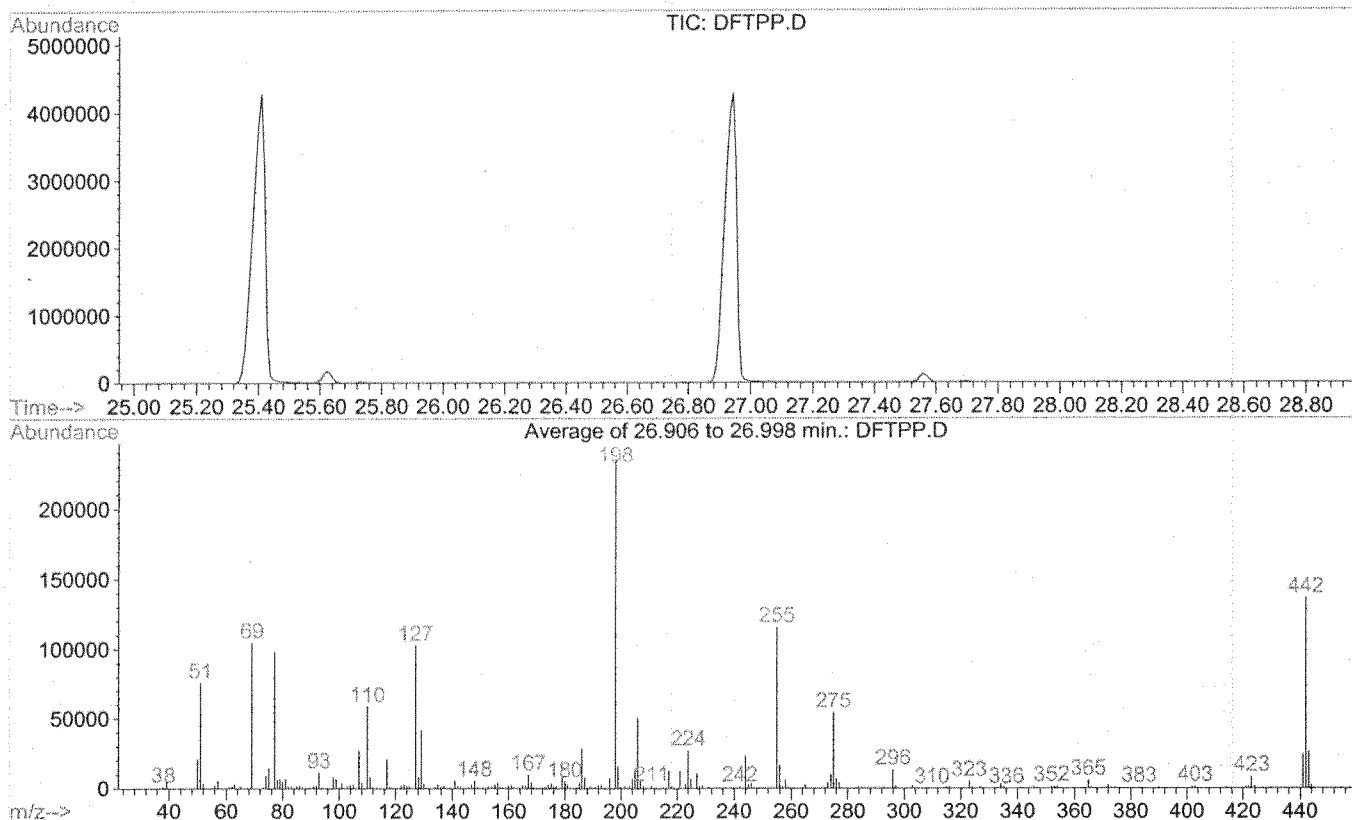

Spectrum Information: Average of 26.906 to 26.998 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.4	76174	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.5	104726	PASS
70	69	0.00	2	0.1	118	PASS
127	198	40	60	43.7	102836	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	235127	PASS
199	198	5	9	6.7	15748	PASS
275	198	10	30	23.1	54322	PASS
365	198	1	100	2.5	5869	PASS
441	443	0.01	100	92.4	24189	PASS
442	198	40	110	58.2	136740	PASS
443	442	17	23	19.1	26182	PASS