

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 02/25/2002 Time: 10:00:45

Sample: AE01220
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 2/25/02 10:00 Ended: 2/25/02 10:00 Analyst: DLV
 Page: 1

	Component Name	Vol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		99		5.0

Comments for Sample AE01220 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 02-25-2002 Time: 10:05:53

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 1 of the 43 compounds in the LCS Standard was below its acceptance range.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB1502\1220.D

Vial: 36

Acq On : 17 Feb 2002 3:18 am

Operator: 209 GALOS

Sample : gc/ms scan 1/17

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 20 15:32 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 13 11:43:23 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.34	152	276718	20.00	ug/l	-0.02
10) Naphthalene-d8	15.97	136	1056559	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.29	164	571937	20.00	ug/l	-0.03
29) Phenanthrene-d10	25.74	188	805798	20.00	ug/l	-0.03
38) Chrysene-d12	33.80	240	529053	20.00	ug/l	-0.05
44) Perylene-d12	38.09	264	348466	20.00	ug/l	-0.04

System Monitoring Compounds

37) 2,4-DDD	30.82	235	40043	4.95	ug/mL	0.32
Spiked Amount	5.000		Recovery	=	99.00%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	16.03	128	502	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	0.00	149	0	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)=qualifier out of range (m)=manual integration

1220.D GCMS0208.M Wed Feb 20 15:32:52 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB1502\1220.D

Vial: 36

Acq On : 17 Feb 2002 3:18 am

Operator: 209 GALOS

Sample : gc/ms scan 1/17

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 20 15:32 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 13 11:43:23 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	27.69	149	2712	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.80	228	1330	N.D.		
42) Bis(2-ethylhexyl)phthalate	34.01	149	2564	N.D.		
43) Chrysene	33.80	228	1330	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.09	252	1497	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

1220.D GCMS0208.M Wed Feb 20 15:32:55 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\FEB1502\1220.D
Acq On : 17 Feb 2002 3:18 am
Sample : gc/ms scan 1/17
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 20 15:32 2002

Vial: 36
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 13 11:43:23 2002
Response via : Initial Calibration

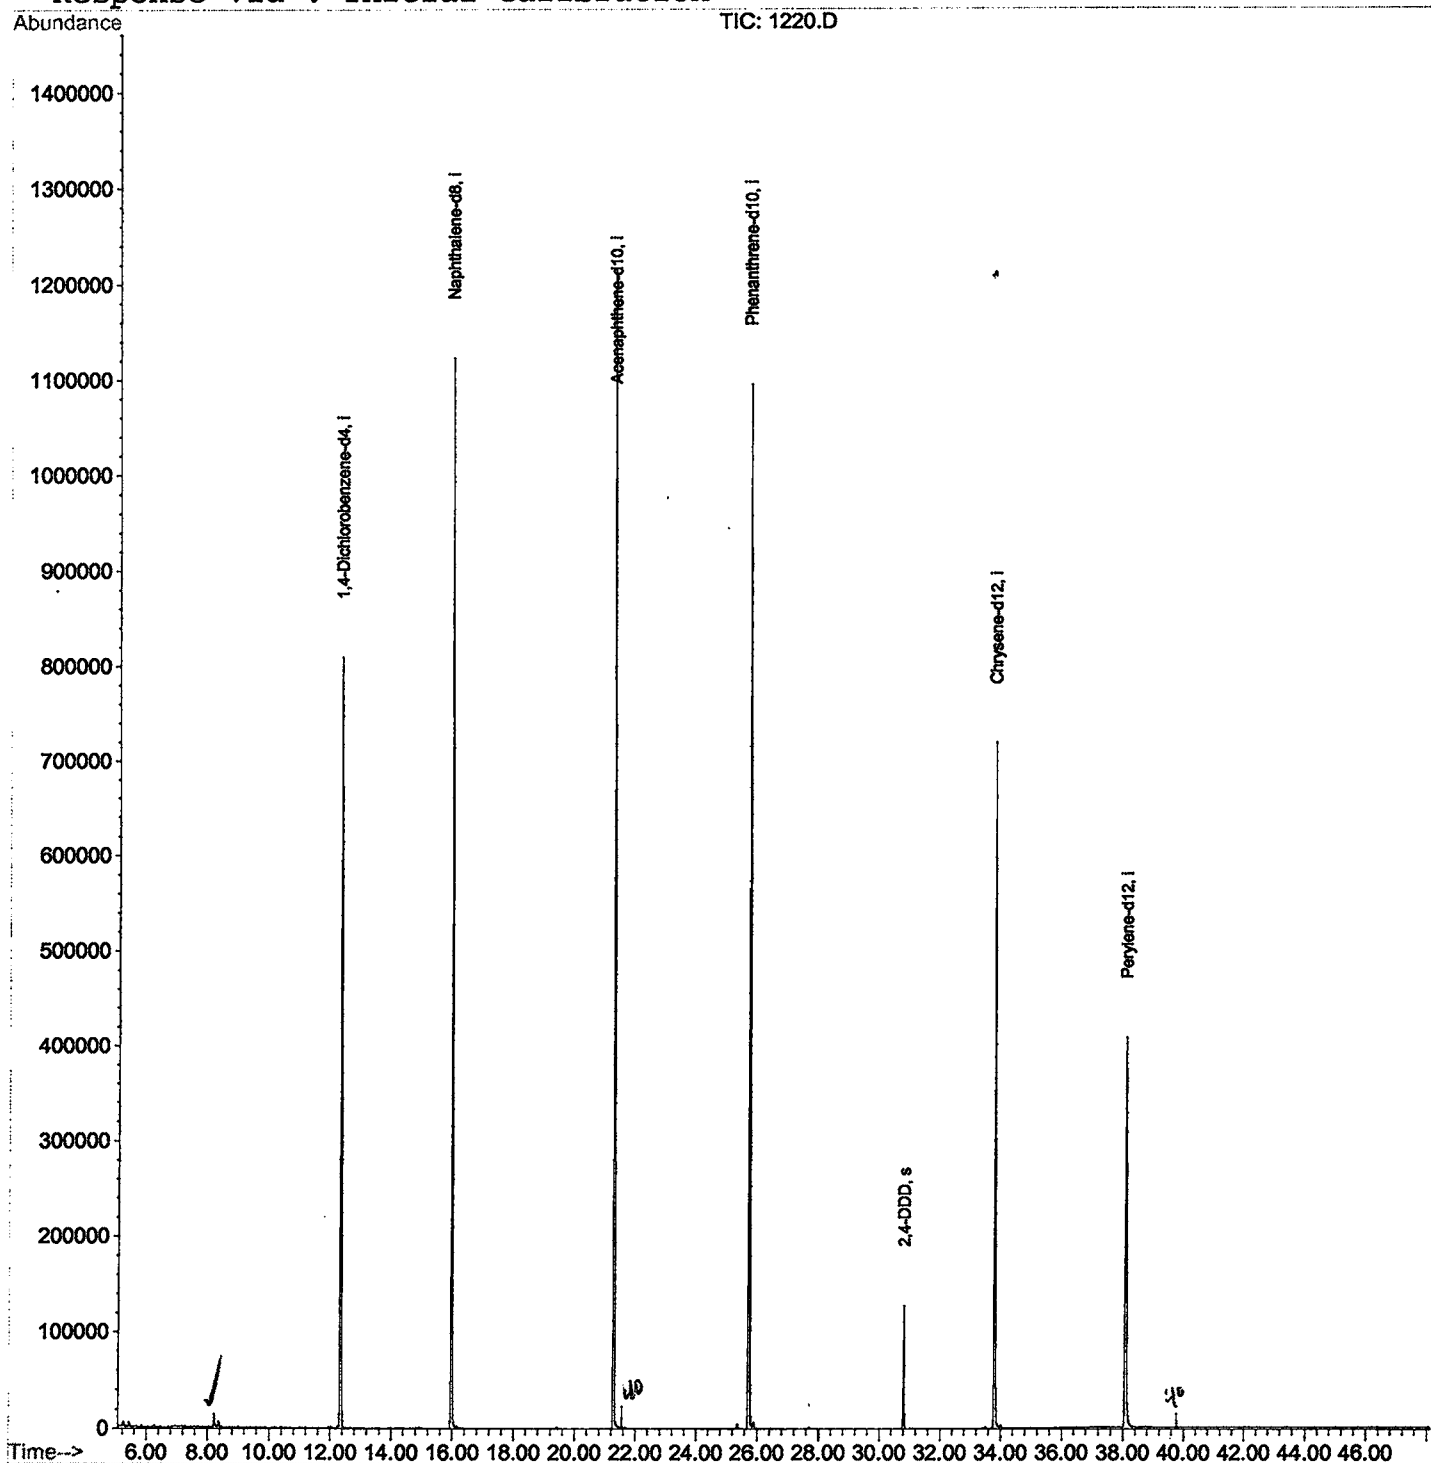

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB1502\1220.D
 Acq On : 17 Feb 2002 3:18 am
 Sample : gc/ms scan 1/17
 Misc :
 MS Integration Params: LSCINT.P

Vial: 36
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.213	341	345	352	rBV	14486	29544	1.23%	0.251%
2	12.335	788	794	805	rVB	808786	1800863	74.90%	15.286%
3	15.970	1184	1190	1204	rBV	1123178	2214385	92.10%	18.795%
4	21.286	1763	1769	1780	rBV	1216971	2404323	100.00%	20.408%
5	25.738	2247	2254	2265	rBV	1095118	2258805	93.95%	19.173%
6	30.815	2802	2807	2814	rVB	128464	246311	10.24%	2.091%
7	33.799	3126	3132	3151	rBV2	718701	1616126	67.22%	13.718%
8	38.086	3590	3599	3621	rBV2	406933	1211124	50.37%	10.280%

Sum of corrected areas: 11781481

1220.D GCMS0208.M Thu Feb 21 09:27:21 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB1502\1220.D
Operator : 209 GALOS
Acquired : 17 Feb 2002 3:18 am using AcqMethod GCMS0208
Instrument : GC/MS 209
Sample Name: gc/ms scan 1/17
Misc Info :
Vial Number: 36
Quant File :GCMS0208.RES (RTE Integrator)

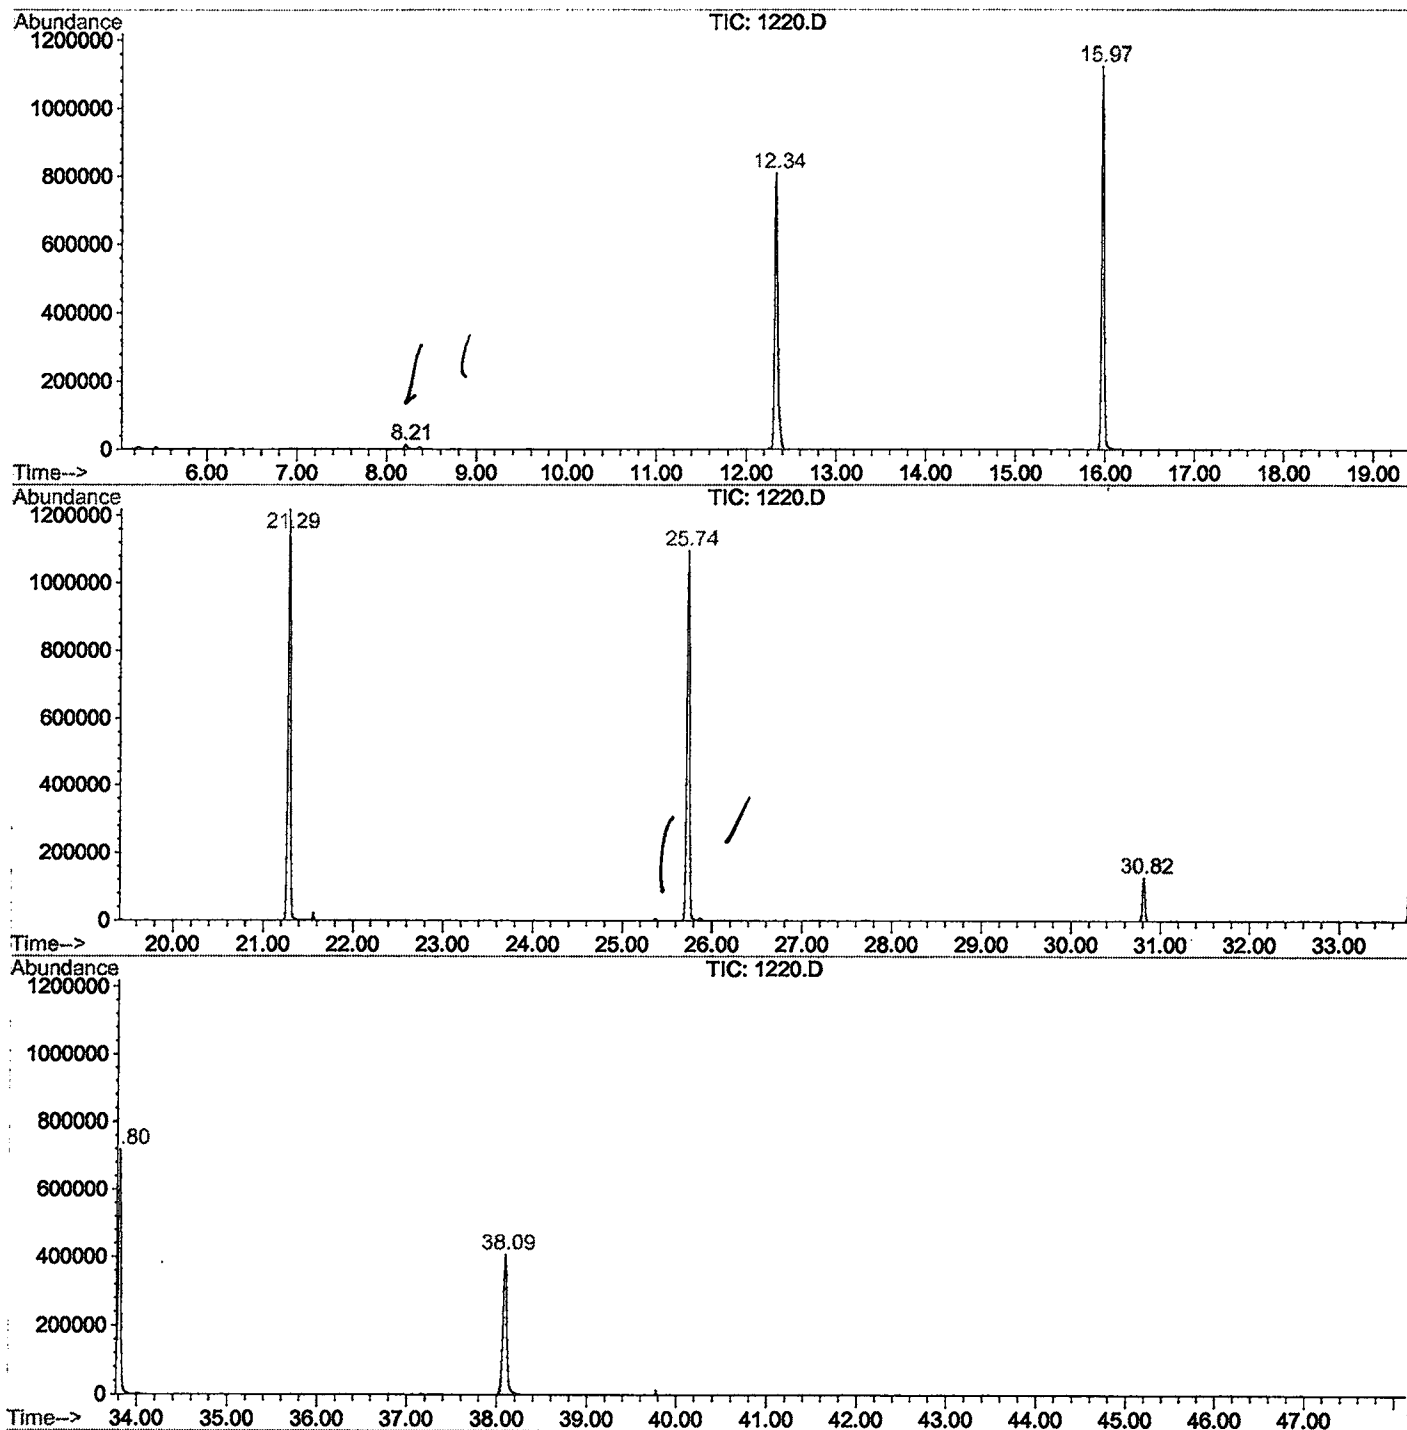

1220.D GCMS0208.M

Thu Feb 21 09:27:28 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB1502\1220.D
Acq On : 17 Feb 2002 3:18 am
Sample : gc/ms scan 1/17
Misc :
MS Integration Params: LSCINT.P











Vial: 36
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 3-Pentanol, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.21	0.33 ug/l	29544	1,4-Dichlorobenzene-d4	12.34

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	33
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	28
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25
4			2-Butanone, 3-methoxy-3-methyl-	116	C6H12O2	036687-98-6	9

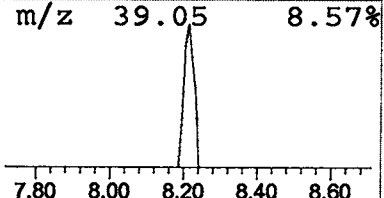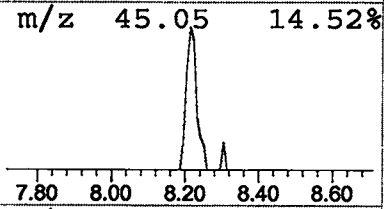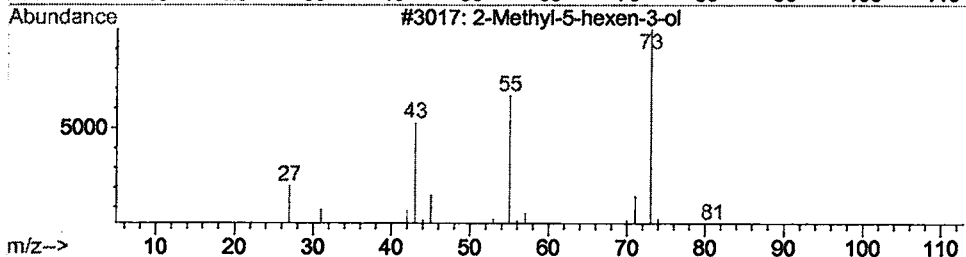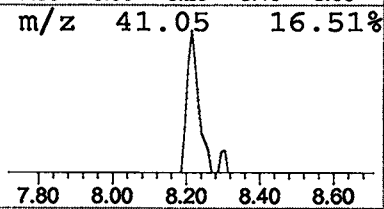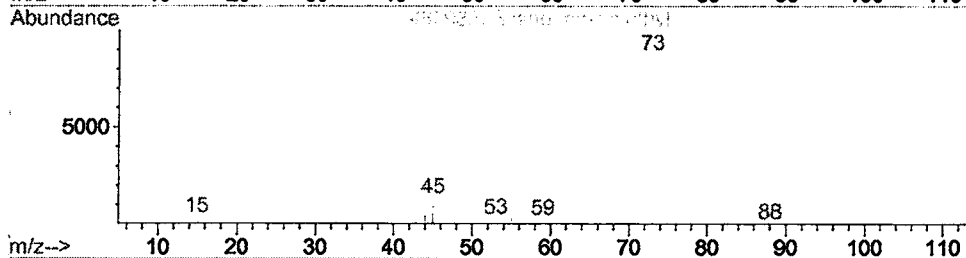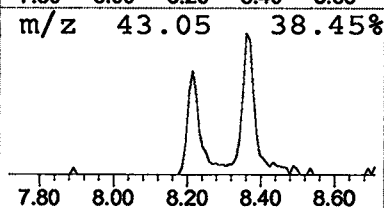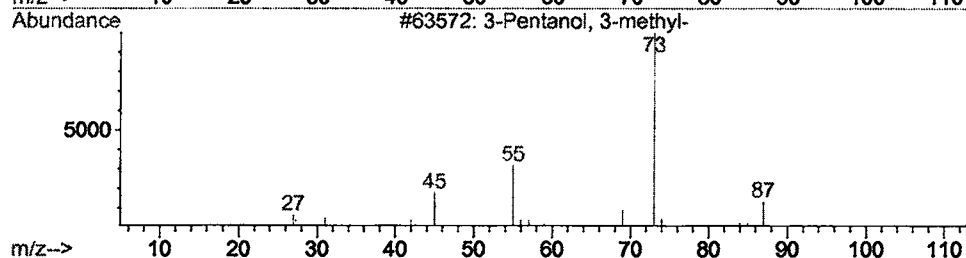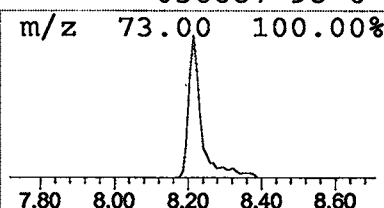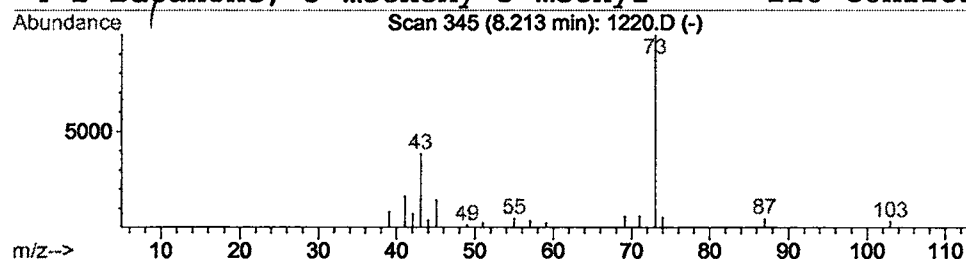

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 17 Feb 2002 3:18 am
 Data File: C:\HPCHEM\1\DATA\FEB1502\1220.D
 Name: gc/ms scan 1/17
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

3-Pentanol, 3-methyl	8.21	0.3	ug/l	29544	ISTD01	12.34	1800860	20.0

1220.D GCMS0208.M Thu Feb 21 09:27:37 2002