

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 02/25/2002 Time: 10:07:18

Sample: AE01223
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 2/25/02 10:06 Ended: 2/25/02 10:06 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		102		5.0

Comments for Sample AE01223 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 02-25-2002 Time: 10:07:35

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 1 of the 43 compounds in the LCS Standard was below its acceptance range.

Quantitation Report

(QT Reviewed)

File : C:\HPCHEM\1\DATA\FEB1502\1223.D
 Date : 17 Feb 2002 1:22 am
 Sample : gc/ms scan 1/17
 Scan : 1

Vial: 34
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 20 15:27 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 13 11:43:23 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.33	152	261242	20.00	ug/l	-0.02
10) Naphthalene-d8	15.98	136	986014	20.00	ug/l	-0.02
17) Acenaphthene-d10	21.29	164	532388	20.00	ug/l	-0.02
29) Phenanthrene-d10	25.73	188	759718	20.00	ug/l	-0.03
38) Chrysene-d12	33.80	240	500754	20.00	ug/l	-0.04
44) Perylene-d12	38.08	264	338145	20.00	ug/l	-0.04

System Monitoring Compounds

37) 2,4-DDD	30.81	235	38909	5.10	ug/mL	0.31
Spiked Amount	5.000		Recovery	=	102.00%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	16.03	128	539	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	0.00	149	0	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#) = qualifier out of range (m) = manual integration

1223.D GCMS0208.M Wed Feb 20 15:28:14 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB1502\1223.D
Acq On : 17 Feb 2002 1:22 am
Sample : gc/ms scan 1/17
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 20 15:27 2002

Vial: 34
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 13 11:43:23 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	27.70	149	1559	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.80	228	1249	N.D.		
42) Bis(2-ethylhexyl)phthalate	34.01	149	2340	N.D.		
43) Chrysene	33.80	228	1249	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.08	252	1427	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

1223.D GCMS0208.M Wed Feb 20 15:28:18 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\FEB1502\1223.D
Acq On : 17 Feb 2002 1:22 am
Sample : gc/ms scan 1/17
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 20 15:27 2002

Vial: 34
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 13 11:43:23 2002
Response via : Initial Calibration

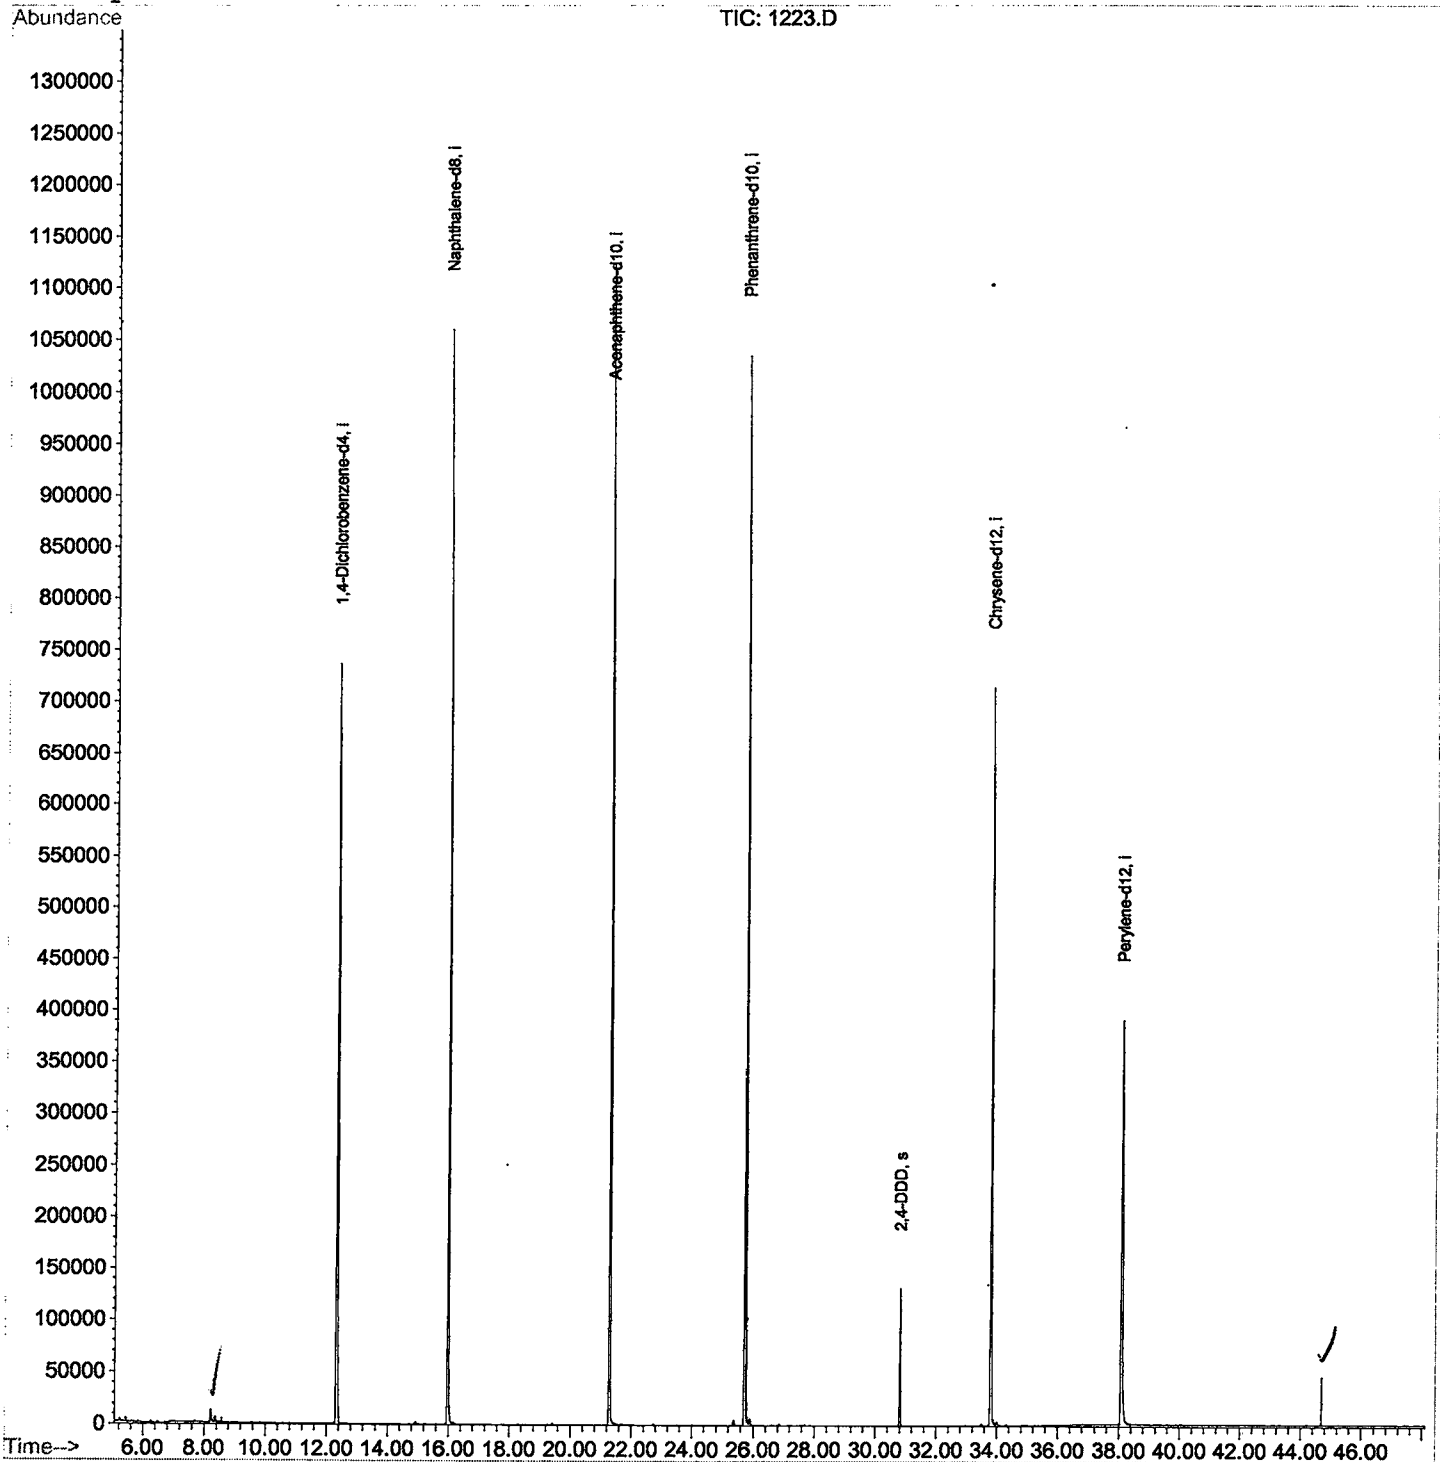

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB1502\1223.D
 Acq On : 17 Feb 2002 1:22 am
 Sample : gc/ms scan 1/17
 Misc :
 MS Integration Params: LSCINT.P

Vial: 34
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.218	342	346	357	rBV	12380	31090	1.39%	0.280%
2	12.331	789	794	806	rVB	735858	1695694	75.69%	15.256%
3	15.975	1185	1191	1208	rBV	1059218	2073269	92.54%	18.653%
4	21.291	1763	1770	1782	rBV	1123710	2240303	100.00%	20.156%
5	25.734	2248	2254	2266	rBV2	1034354	2118881	94.58%	19.064%
6	30.811	2803	2807	2813	rBV	131592	240762	10.75%	2.166%
7	33.803	3127	3133	3150	rBV2	713056	1531072	68.34%	13.775%
8	38.081	3592	3599	3614	rBV2	389241	1158509	51.71%	10.423%
9	44.691	4317	4319	4320	rBV	45642	25197	1.12%	0.227%

Sum of corrected areas: 11114777

1223.D GCMS0208.M Thu Feb 21 09:28:59 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB1502\1223.D
 Operator : 209 GALOS
 Acquired : 17 Feb 2002 1:22 am using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 1/17
 Misc Info :
 Vial Number: 34
 Quant File :GCMS0208.RES (RTE Integrator)

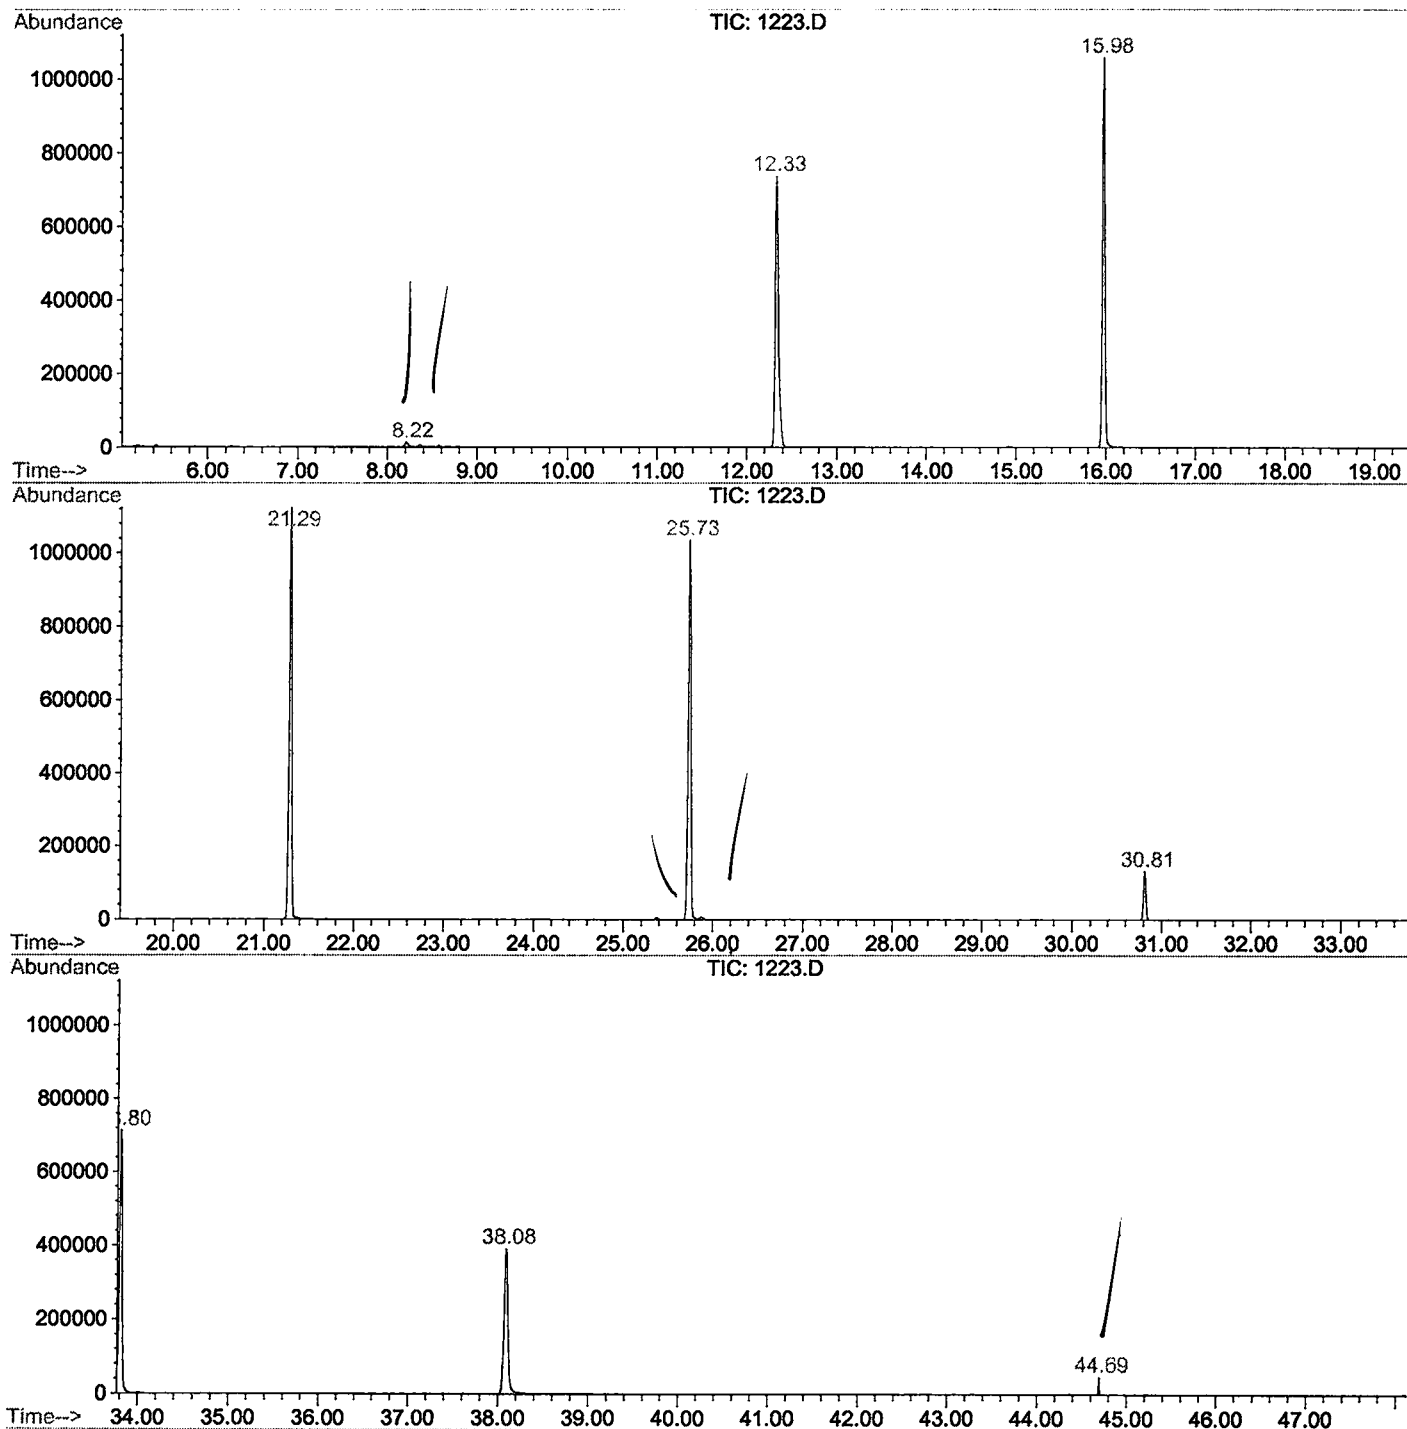

1223.D GCMS0208.M

Thu Feb 21 09:29:05 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB1502\1223.D
Acq On : 17 Feb 2002 1:22 am
Sample : gc/ms scan 1/17
Misc :
MS Integration Params: LSCINT.P










Vial: 34
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Methyl-5-hexen-3-ol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.22	0.37 ug/l	31090	1,4-Dichlorobenzene-d4	12.33

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	33
2			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	25
3			Formic acid, ethyl ester	74	C3H6O2	000109-94-4	5
4			N-Ethylformamide	73	C3H7NO	000627-45-2	4

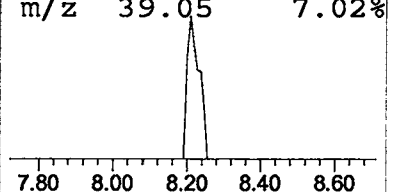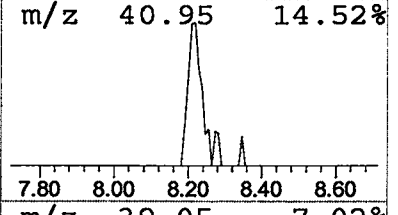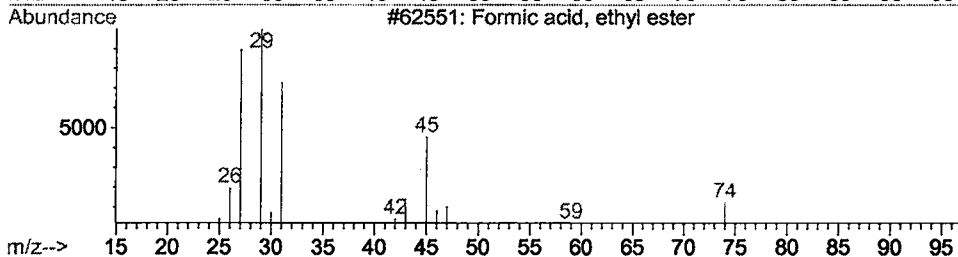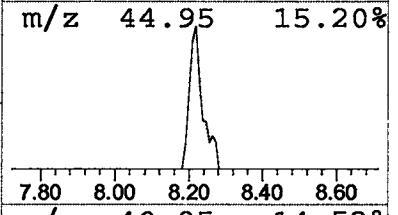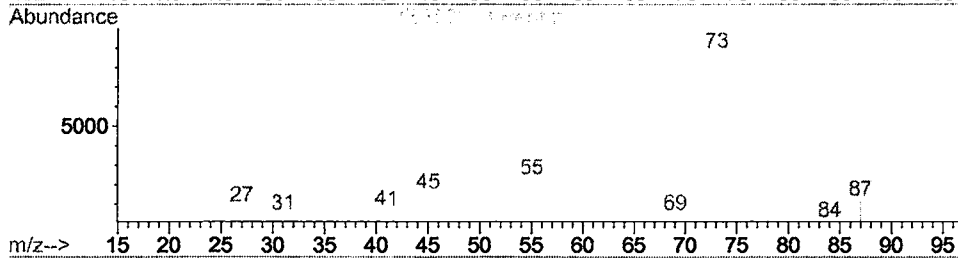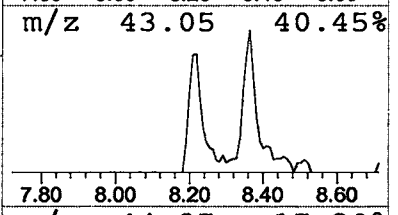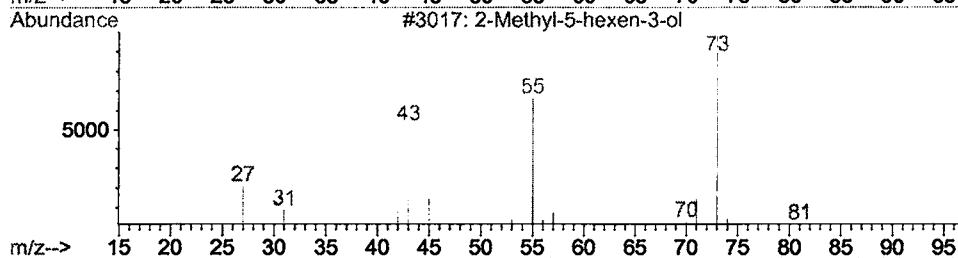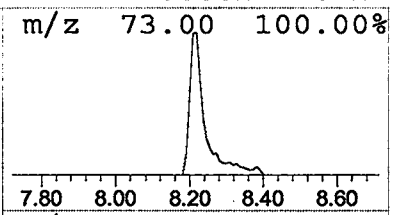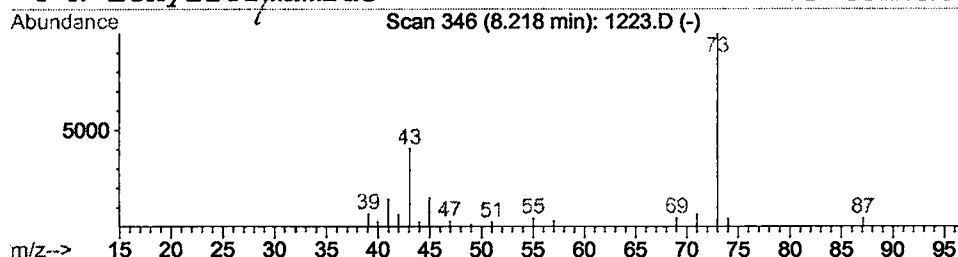

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB1502\1223.D
 Acq On : 17 Feb 2002 1:22 am
 Sample : gc/ms scan 1/17
 Misc :
 MS Integration Params: LSCINT.P









Vial: 34
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Acetaldehyde Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
44.69	0.43 ug/l	25197	Perylene-d12	38.08

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetaldehyde	44	C2H4O	000075-07-0	3
2			Ethylene oxide	44	C2H4O	000075-21-8	3
3			6-Methyl-1,2,3,4-tetrahydroquinoxal	208	C9H8N2S2	000000-00-0	2
4			Piperidine, 1-nitro-	130	C5H10N2O2	007119-94-0	2

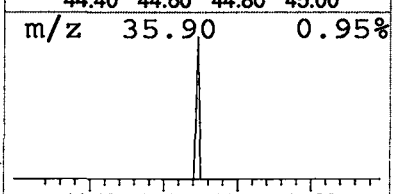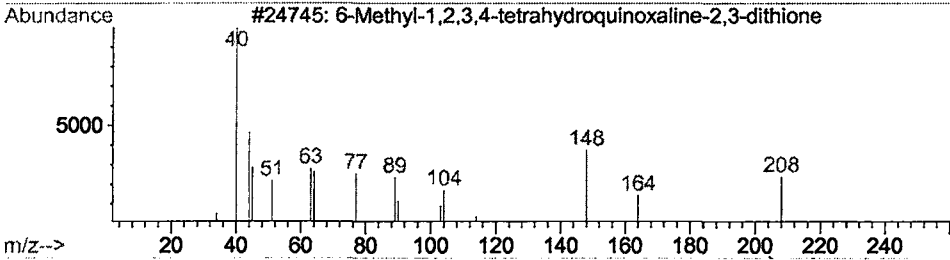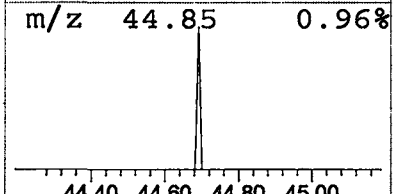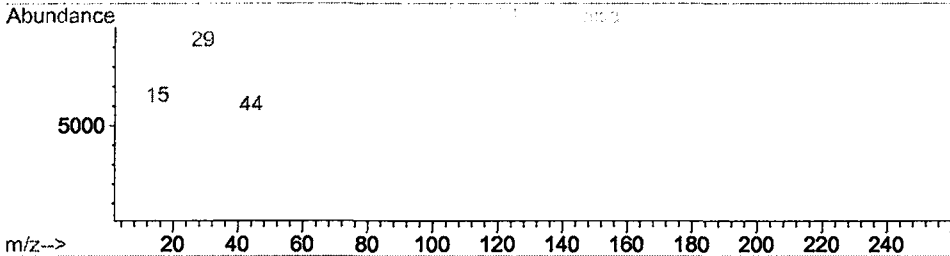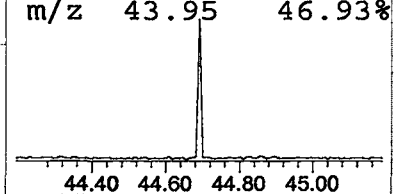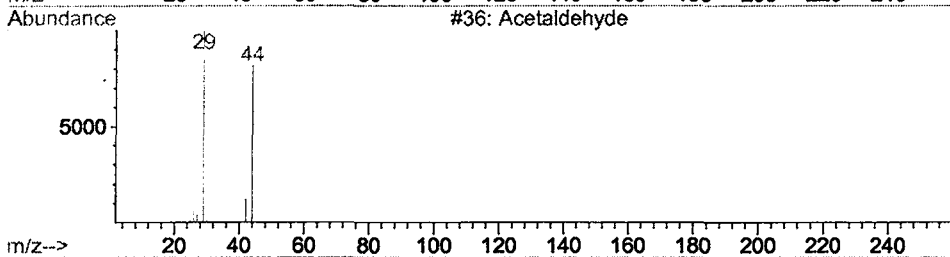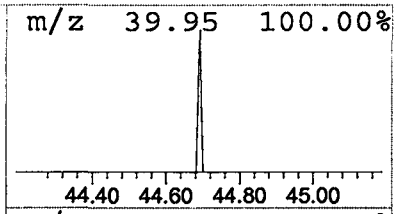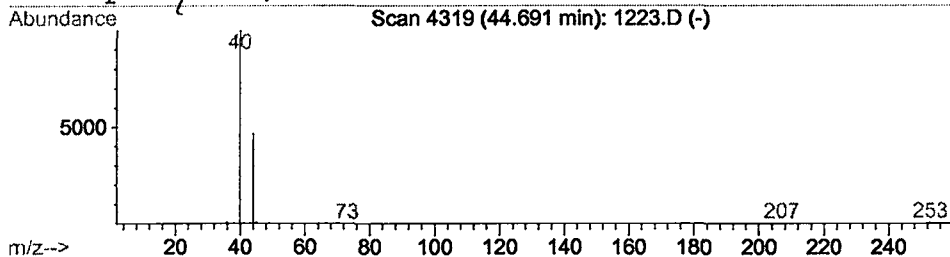

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 17 Feb 2002 1:22 am
 Data File: C:\HPCHEM\1\DATA\FEB1502\1223.D
 Name: gc/ms scan 1/17
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Methyl-5-hexen-3-ol	8.22	0.4	ug/l	31090	ISTD01	12.33	1695690	20.0
Acetaldehyde	44.69	0.4	ug/l	25197	ISTD06	38.08	1158510	20.0

1223.D GCMS0208.M Thu Feb 21 09:29:19 2002