

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 02/25/2002 Time: 10:03:16

Sample: AE01224
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 2/25/02 10:03 Ended: 2/25/02 10:03 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		93		5.0

Comments for Sample AE01224 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 02-25-2002 Time: 10:06:39

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 1 of the 43 compounds in the LCS Standard was below its acceptance range.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB1502\1224.D

Vial: 33

Acq On : 17 Feb 2002 12:24 am

Operator: 209 GALOS

Sample : gc/ms scan 1/17

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 20 15:25 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 13 11:43:23 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.34	152	280035	20.00	ug/l	-0.02
10) Naphthalene-d8	15.97	136	1050201	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.29	164	565162	20.00	ug/l	-0.03
29) Phenanthrene-d10	25.74	188	786731	20.00	ug/l	-0.03
38) Chrysene-d12	33.80	240	501563	20.00	ug/l	-0.05
44) Perylene-d12	38.09	264	329716	20.00	ug/l	-0.04

System Monitoring Compounds

37) 2,4-DDD	30.82	235	36918	4.67	ug/mL	0.32
Spiked Amount	5.000		Recovery	=	93.40%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	16.03	128	577	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

#) = qualifier out of range (m) = manual integration

224.D GCMS0208.M Wed Feb 20 15:26:46 2002

Page 1

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB1502\1224.D
Acq On : 17 Feb 2002 12:24 am
Sample : gc/ms scan 1/17
Misc :
MS Integration Params: LSCINT.P

Vial: 33
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.213	338	345	353	rBV	11265	26488	1.12%	0.231%
2	12.335	788	794	807	rBV	761882	1807812	76.78%	15.765%
3	15.971	1184	1190	1207	rBV	1092588	2200724	93.46%	19.192%
4	21.286	1763	1769	1781	rBV	1182175	2354625	100.00%	20.534%
5	25.738	2247	2254	2265	rBV	1060655	2198466	93.37%	19.172%
6	30.815	2802	2807	2813	rBV	119969	226594	9.62%	1.976%
7	33.799	3126	3132	3151	rBV	685700	1522677	64.67%	13.279%
8	38.086	3591	3599	3619	rBV2	376203	1129688	47.98%	9.852%

Sum of corrected areas: 11467074

1224.D GCMS0208.M Thu Feb 21 09:29:43 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB1502\1224.D
 Operator : 209 GALOS
 Acquired : 17 Feb 2002 12:24 am using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 1/17
 Misc Info :
 Vial Number: 33
 Quant File :GCMS0208.RES (RTE Integrator)

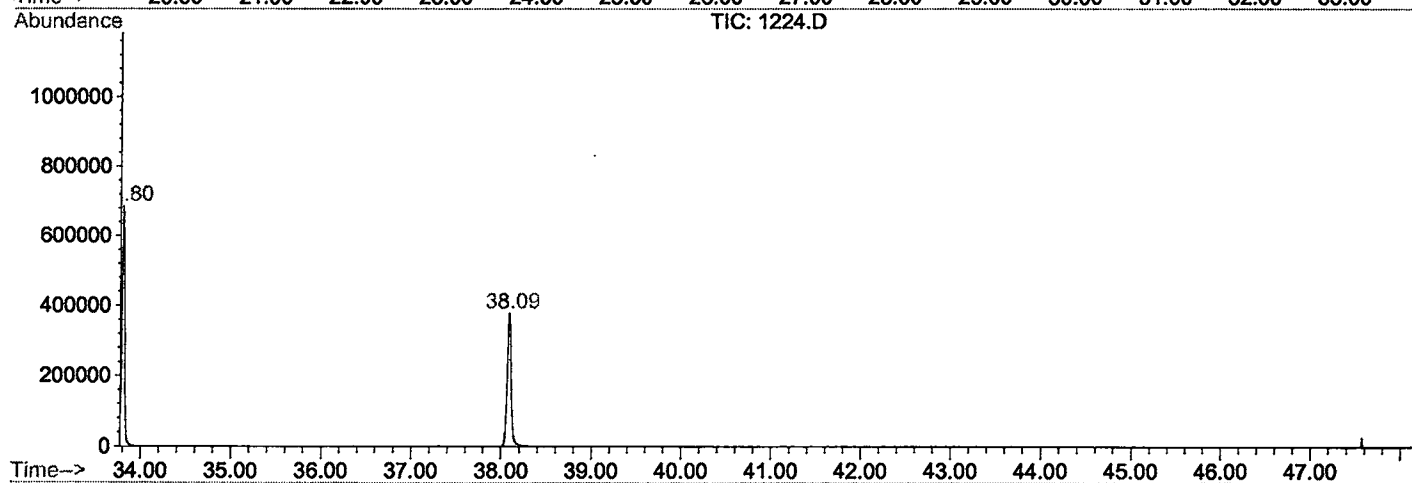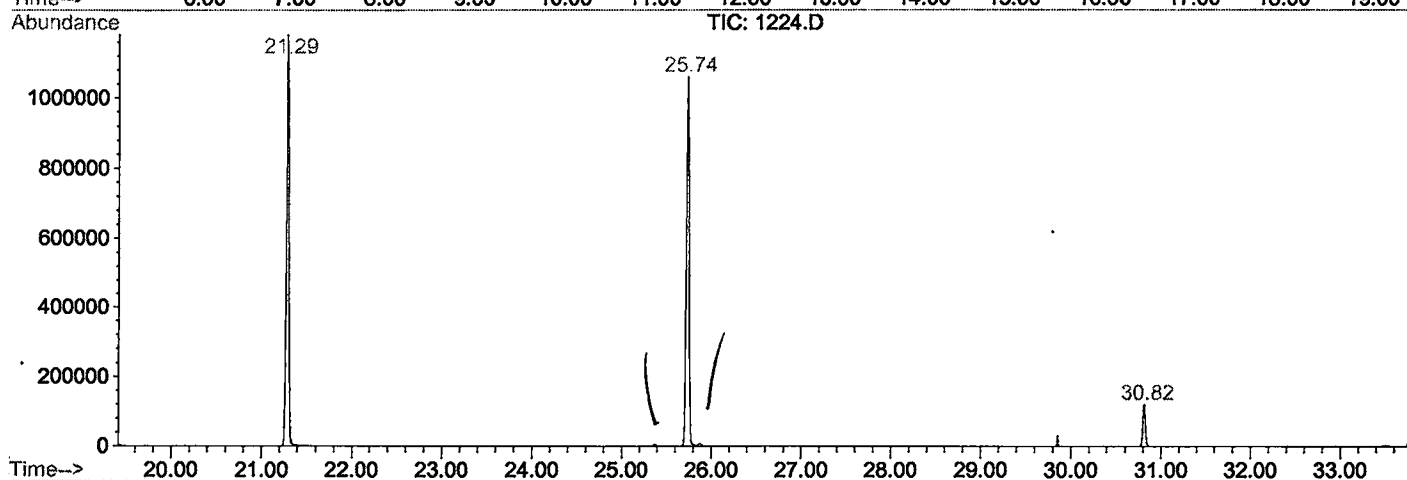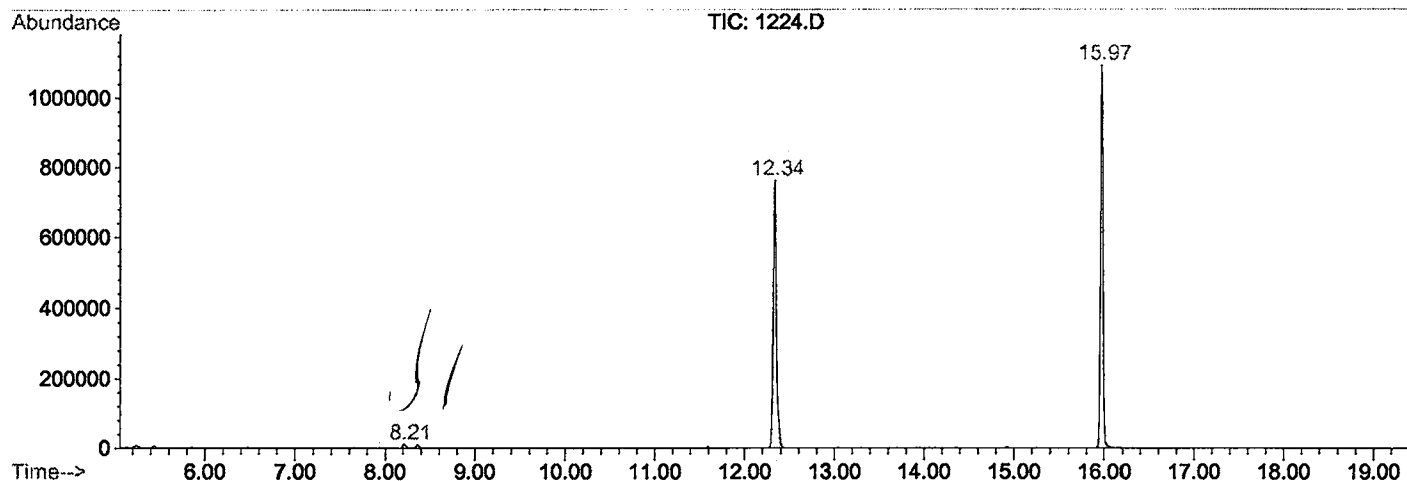

1224.D GCMS0208.M

Thu Feb 21 09:29:49 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB1502\1224.D
 Acq On : 17 Feb 2002 12:24 am
 Sample : gc/ms scan 1/17
 Misc :
 MS Integration Params: LSCINT.P










Vial: 33
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 N-Ethylformamide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.21	0.29 ug/l	26488	1,4-Dichlorobenzene-d4	12.34

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	N-Ethylformamide	73	C3H7NO	000627-45-2	4
2	3,4-Dimethyl-5-hexen-3-ol	128	C8H16O	000000-00-0	4
3	Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	4
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	4

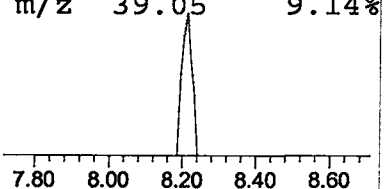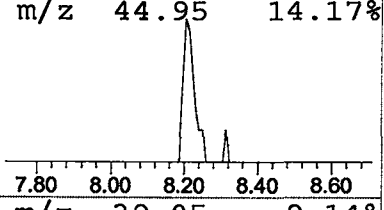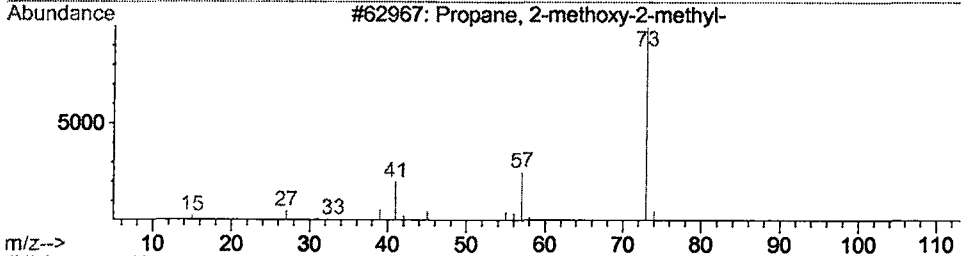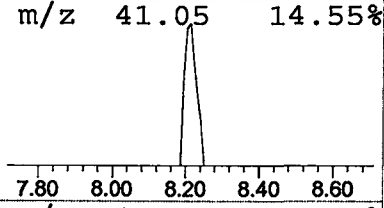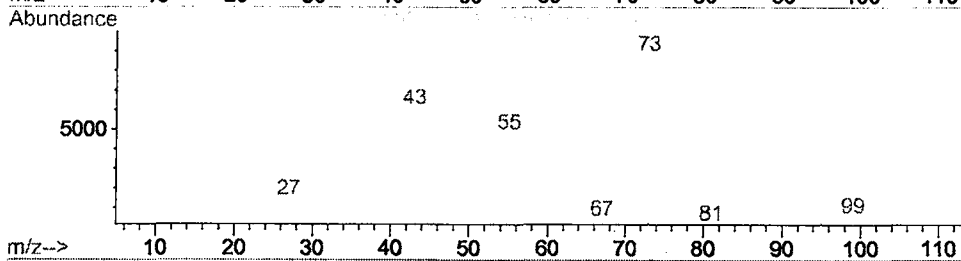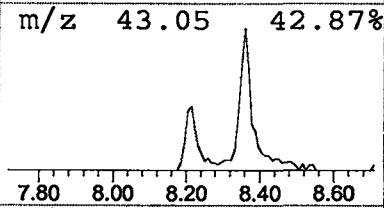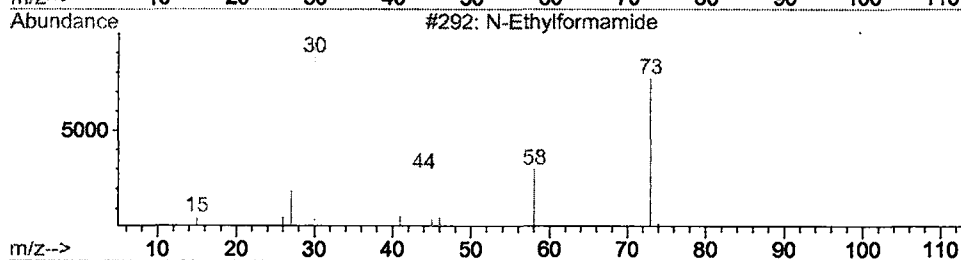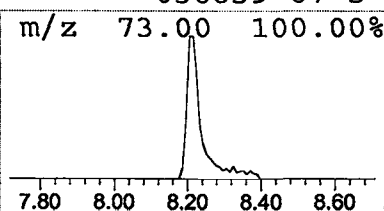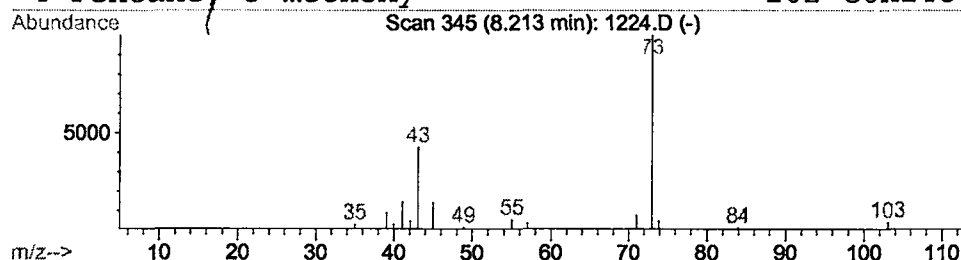

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 17 Feb 2002 12:24 am
 Data File: C:\HPCHEM\1\DATA\FEB1502\1224.D
 Name: gc/ms scan 1/17
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
N-Ethylformamide	8.21	0.3	ug/l	26488	ISTD01	12.34	1807810	20.0

1224.D GCMS0208.M Thu Feb 21 09:29:57 2002