

Method 508 Mod.

Date Extracted 1-22-02

Page 42

Ref

#GCHS-17079

weight added

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
L.B.		500ml		1ml			1ml	10B	7			
Ref.					0.5ml			10A				
1329								9A				
472								9B				
1435	F.B.							6A				
1436								6B				
1437								8B				
1438								8A				
1439								4B				
1440	see 2/25							4A				
1441								3A				
1442								3B				
1462	see 2/25	↓		↓			↓	2A	↓			
Remarks 472 Reextract Reviewed by, 												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type - Sep-Fun		Solv. lot# V39466	NaCl lot# V11599		Na2SO4 lot# V39A00							
STANDARD	INT STD LOG#											
CALIBRATION	HPD1302											
(REF)/SPIKE		91759										
MDL/MDRF												
Q. CHECK												
INT. STD.	HPD15022002											
SURROGATE	HPD	011602										
LPC												
ENDRIN/DDT												

Analyst A.D.
revision 4/12/01

Verified by My

Reviewed by DN
Date 3/6/2

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB2102\DFTPP.D

Acq On : 21 Feb 2002 12:29 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

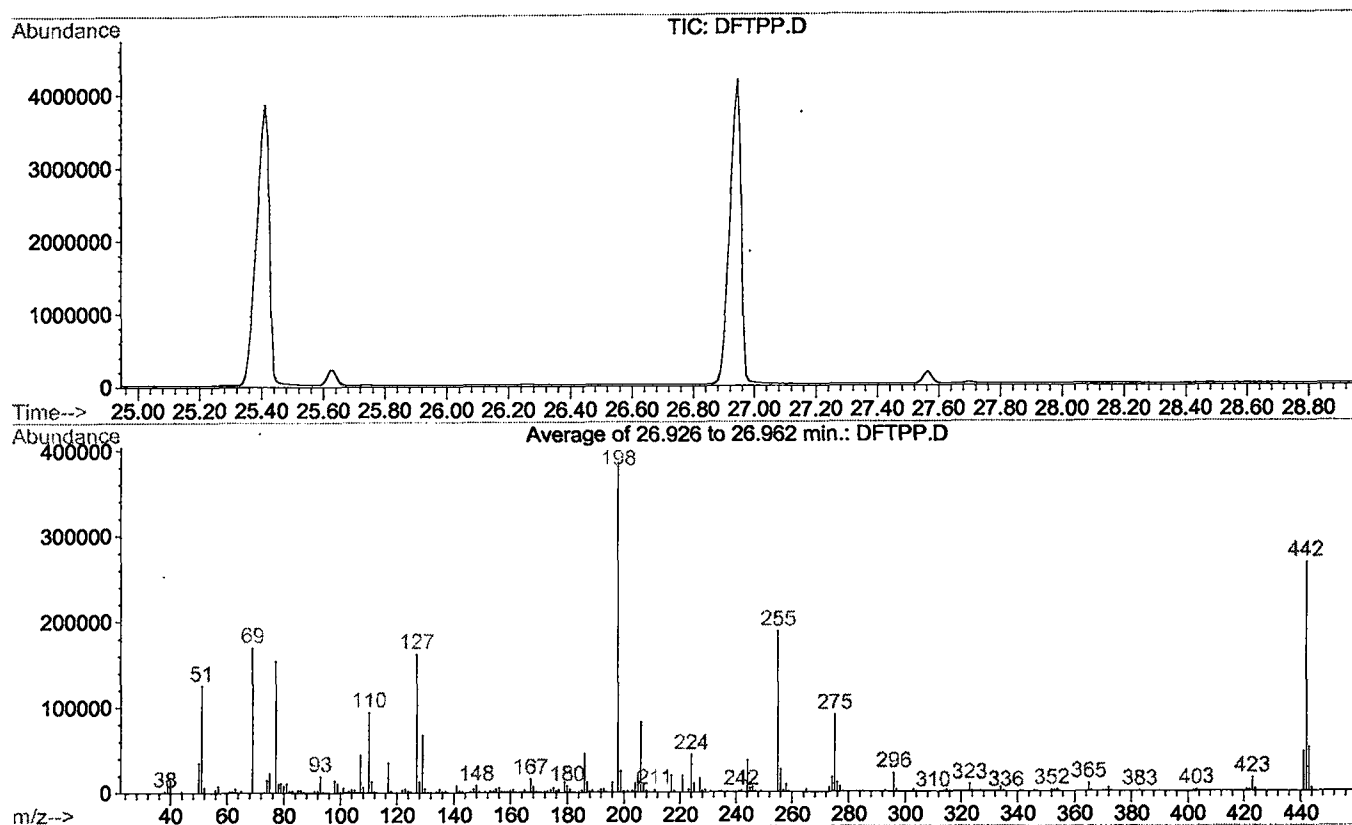

Spectrum Information: Average of 26.926 to 26.962 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.8	126262	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.3	170317	PASS
70	69	0.00	2	0.0	44	PASS
127	198	40	60	42.4	163022	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	384803	PASS
199	198	5	9	6.6	25295	PASS
275	198	10	30	23.7	91200	PASS
365	198	1	100	2.7	10254	PASS
441	443	0.01	100	91.3	47168	PASS
442	198	40	110	69.6	267712	PASS
443	442	17	23	19.3	51662	PASS

DFTPP.D GCMS0208.M

Fri Feb 22 08:27:21 2002