

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 03/06/2002 Time: 10:35:48

Sample: AE01442
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 3/6/02 10:35 Ended: 3/6/02 10:35 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		104		5.0

Comments for Sample AE01442 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-06-2002 Time: 10:37:33

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB2102\1442.D

Vial: 14

Acq On : 22 Feb 2002 2:54 am

Operator:

Sample : gc/ms scan 1/22

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 22 9:21 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Thu Feb 21 16:13:52 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.33	152	245347	20.00	ug/l	-0.02
10) Naphthalene-d8	15.97	136	936075	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.28	164	486299	20.00	ug/l	-0.03
29) Phenanthrene-d10	25.74	188	676733	20.00	ug/l	-0.03
38) Chrysene-d12	33.80	240	412642	20.00	ug/l	-0.05
44) Perylene-d12	38.08	264	261986	20.00	ug/l	-0.05

System Monitoring Compounds

37) 2,4-DDD	30.81	235	40680	5.20	ug/mL	0.32
Spiked Amount	5.000		Recovery	=	104.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.76	149	196	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#) = qualifier out of range (m) = manual integration

1442.D GCMS0208.M

Fri Feb 22 09:22:16 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB2102\1442.D

Vial: 14

Acq On : 22 Feb 2002 2:54 am

Operator:

Sample : gc/ms scan 1/22

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 22 9:21 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Thu Feb 21 16:13:52 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	27.70	149	4284	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.81	228	896	N.D.		
42) Bis(2-ethylhexyl)phthalate	34.00	149	1198	N.D.		
43) Chrysene	33.81	228	896	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.08	252	933	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

1442.D GCMS0208.M Fri Feb 22 09:22:20 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\FEB2102\1442.D
Acq On : 22 Feb 2002 2:54 am
Sample : gc/ms scan 1/22
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 22 9:21 2002

Vial: 14
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Thu Feb 21 16:13:52 2002
Response via : Initial Calibration

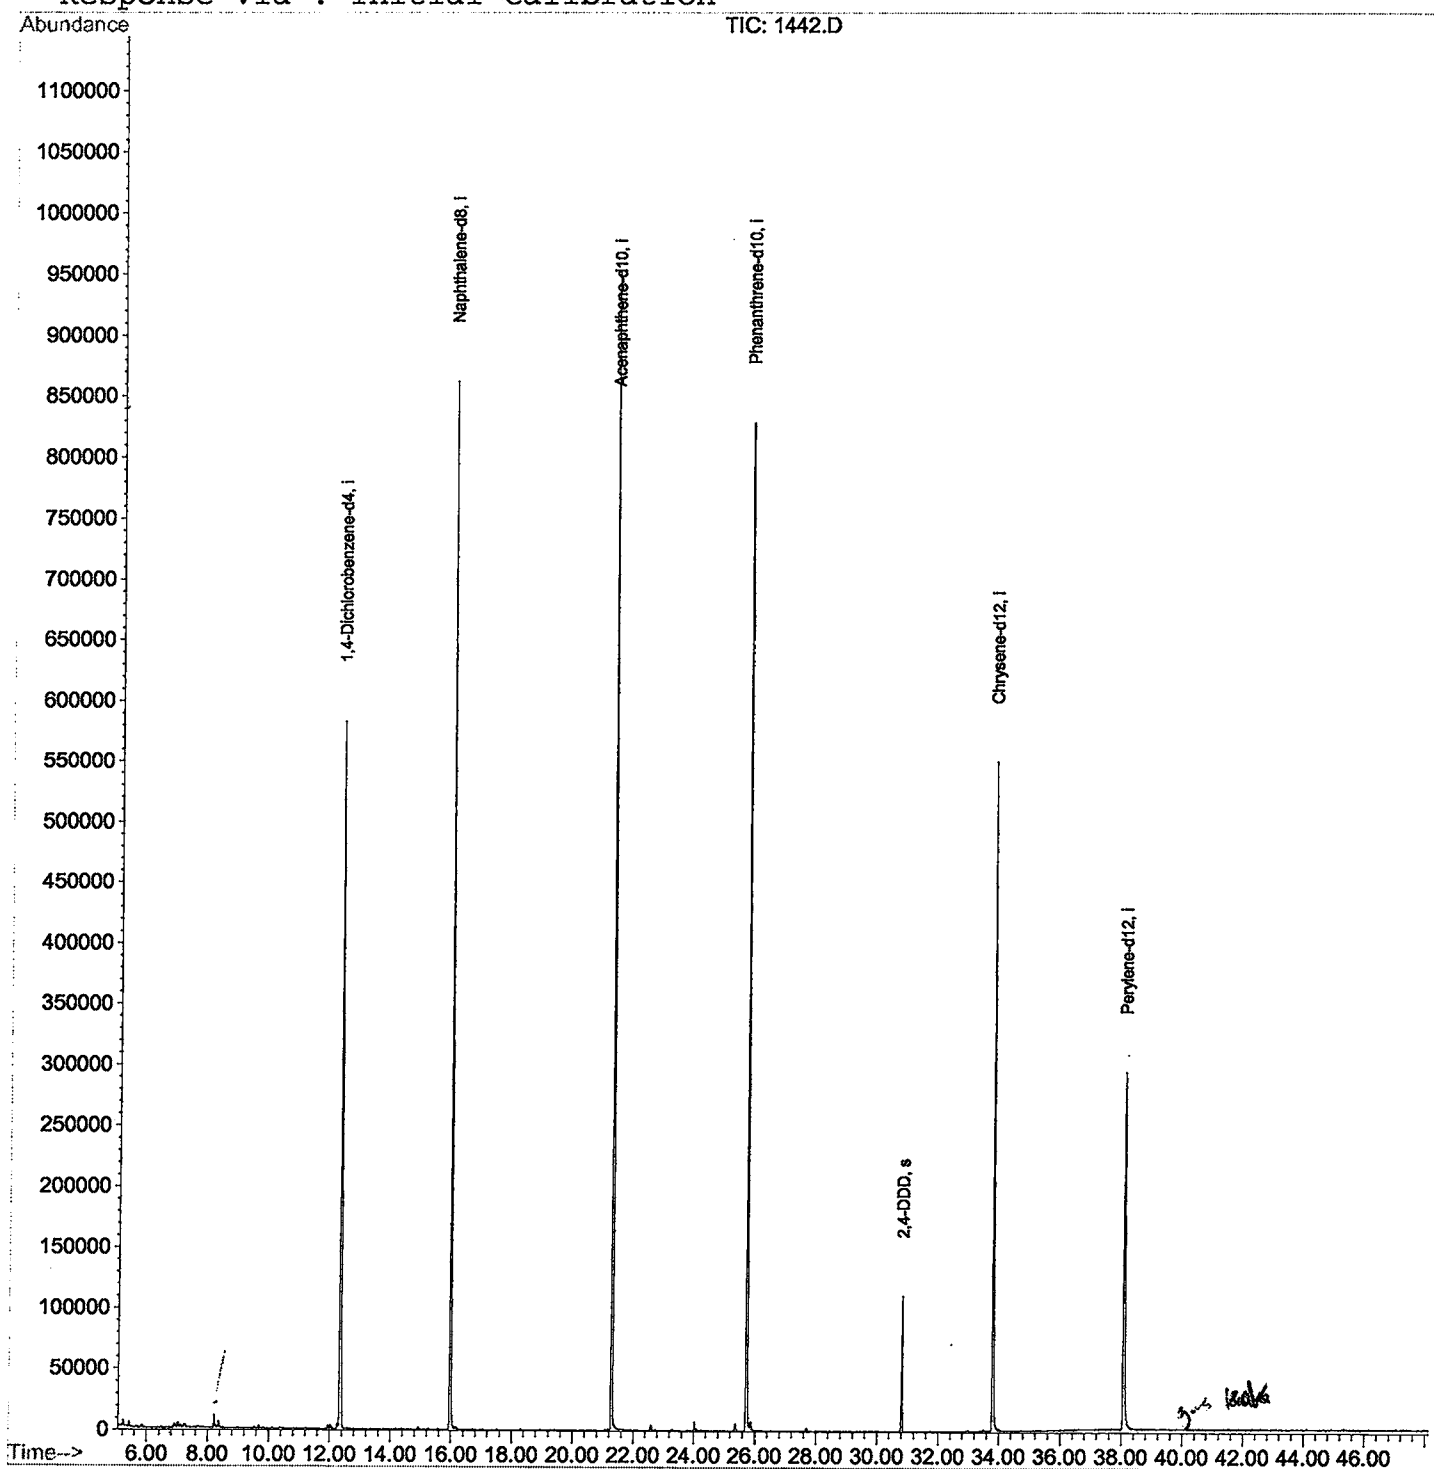

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB2102\1442.D

Vial: 14

Acq On : 22 Feb 2002 2:54 am

Operator:

Sample : gc/ms scan 1/22

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.203	341	344	351	rBV	10645	25531	1.32%	0.272%
2	12.334	788	794	810	rVB	582489	1399699	72.29%	14.903%
3	15.969	1184	1190	1203	rBV	861296	1823317	94.17%	19.413%
4	21.285	1763	1769	1787	rBV	952725	1936297	100.00%	20.616%
5	25.737	2247	2254	2265	rBV2	828483	1800813	93.00%	19.173%
6	30.814	2802	2807	2812	rVB	110795	212487	10.97%	2.262%
7	33.797	3125	3132	3146	rBV2	550192	1261973	65.17%	13.436%
8	38.076	3589	3598	3620	rBV2	292721	932200	48.14%	9.925%




Sum of corrected areas: 9392317

1442.D GCMS0208.M

Fri Feb 22 09:36:24 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB2102\1442.D
 Operator :
 Acquired : 22 Feb 2002 2:54 am using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 1/22
 Misc Info :
 Vial Number: 14
 Quant File :GCMS0208.RES (RTE Integrator)

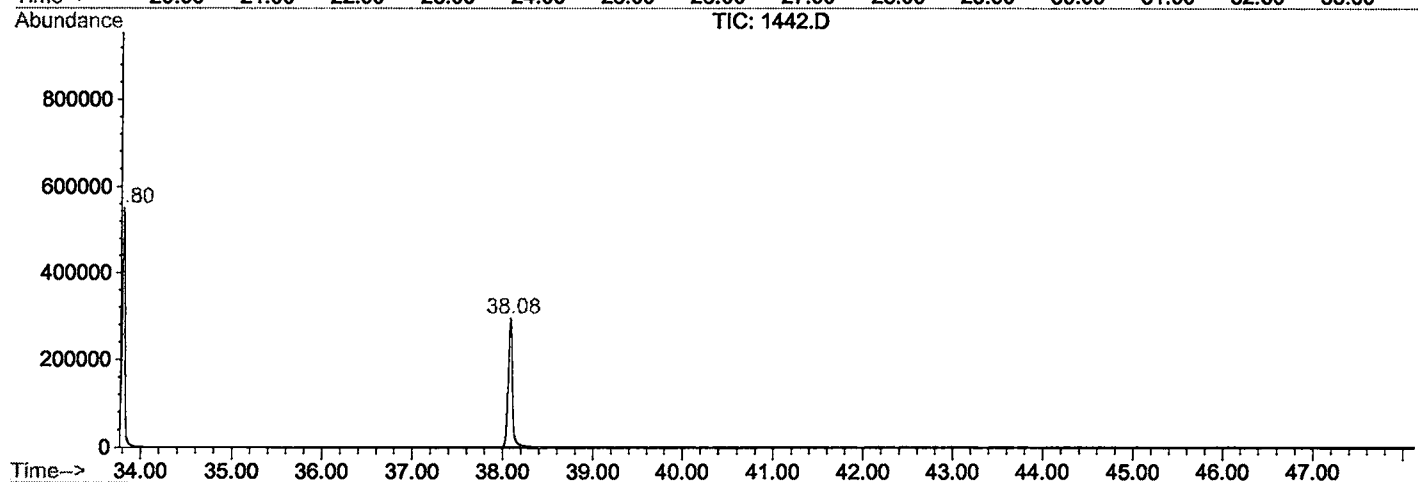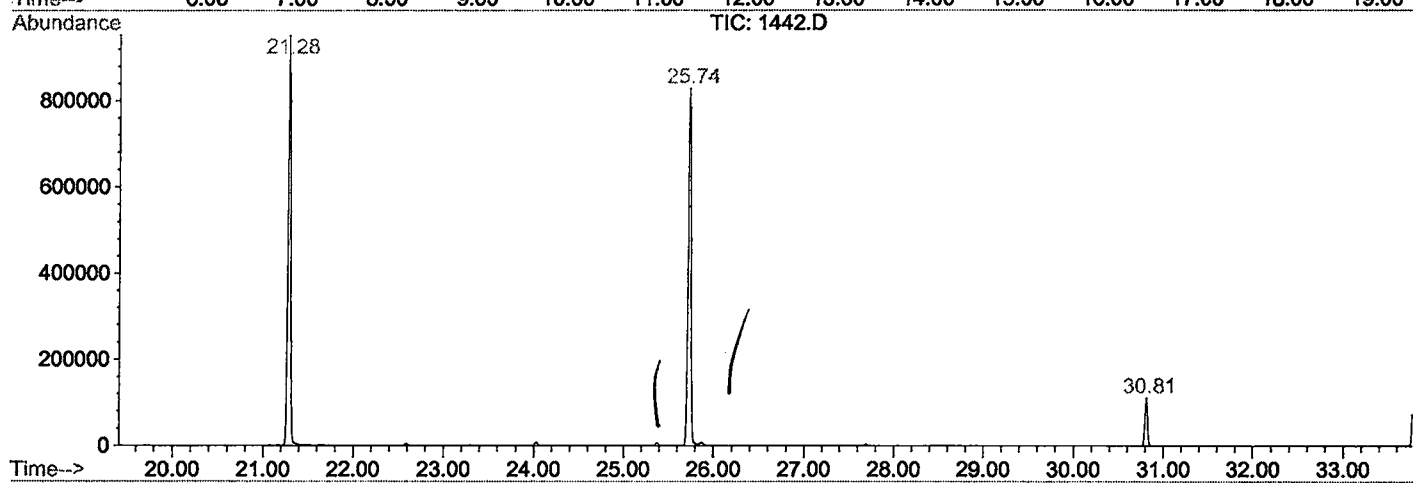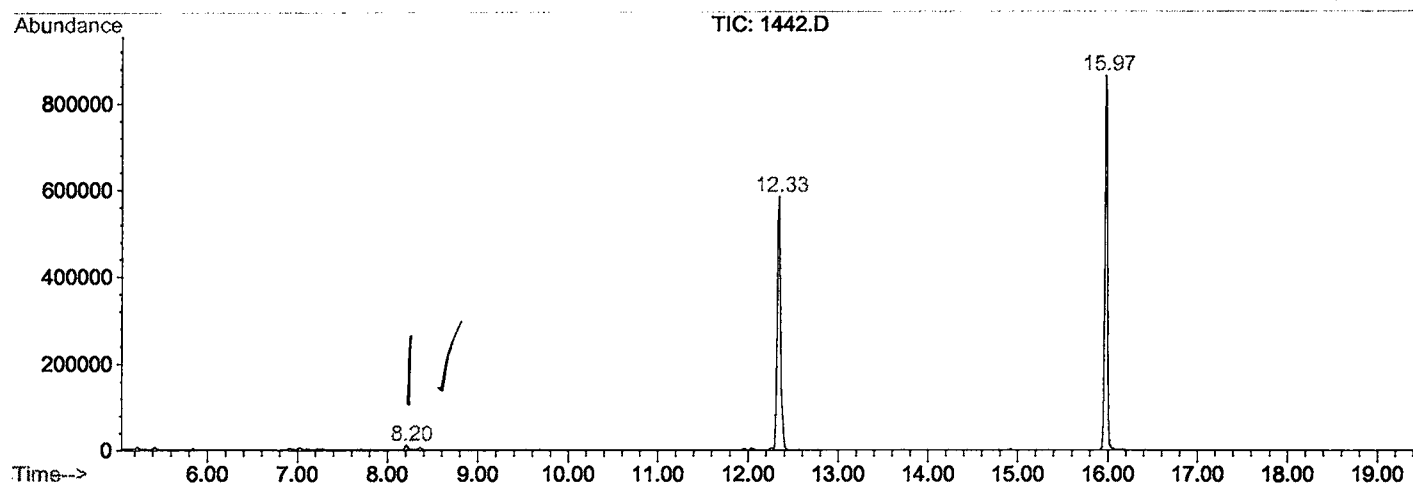

1442.D GCMS0208.M

Fri Feb 22 09:36:30 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB2102\1442.D
 Acq On : 22 Feb 2002 2:54 am
 Sample : gc/ms scan 1/22
 Misc :
 MS Integration Params: LSCINT.P


Vial: 14
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 1-Butanamine, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.20	0.36 ug/l	25531	1,4-Dichlorobenzene-d4	12.33

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9
2	1-Butanamine, 2-methyl-	87	C5H13N	000096-15-1	7
3	N-Ethylformamide	73	C3H7NO	000627-45-2	5
4	Formamide, N,N-dimethyl-	73	C3H7NO	000068-12-2	5

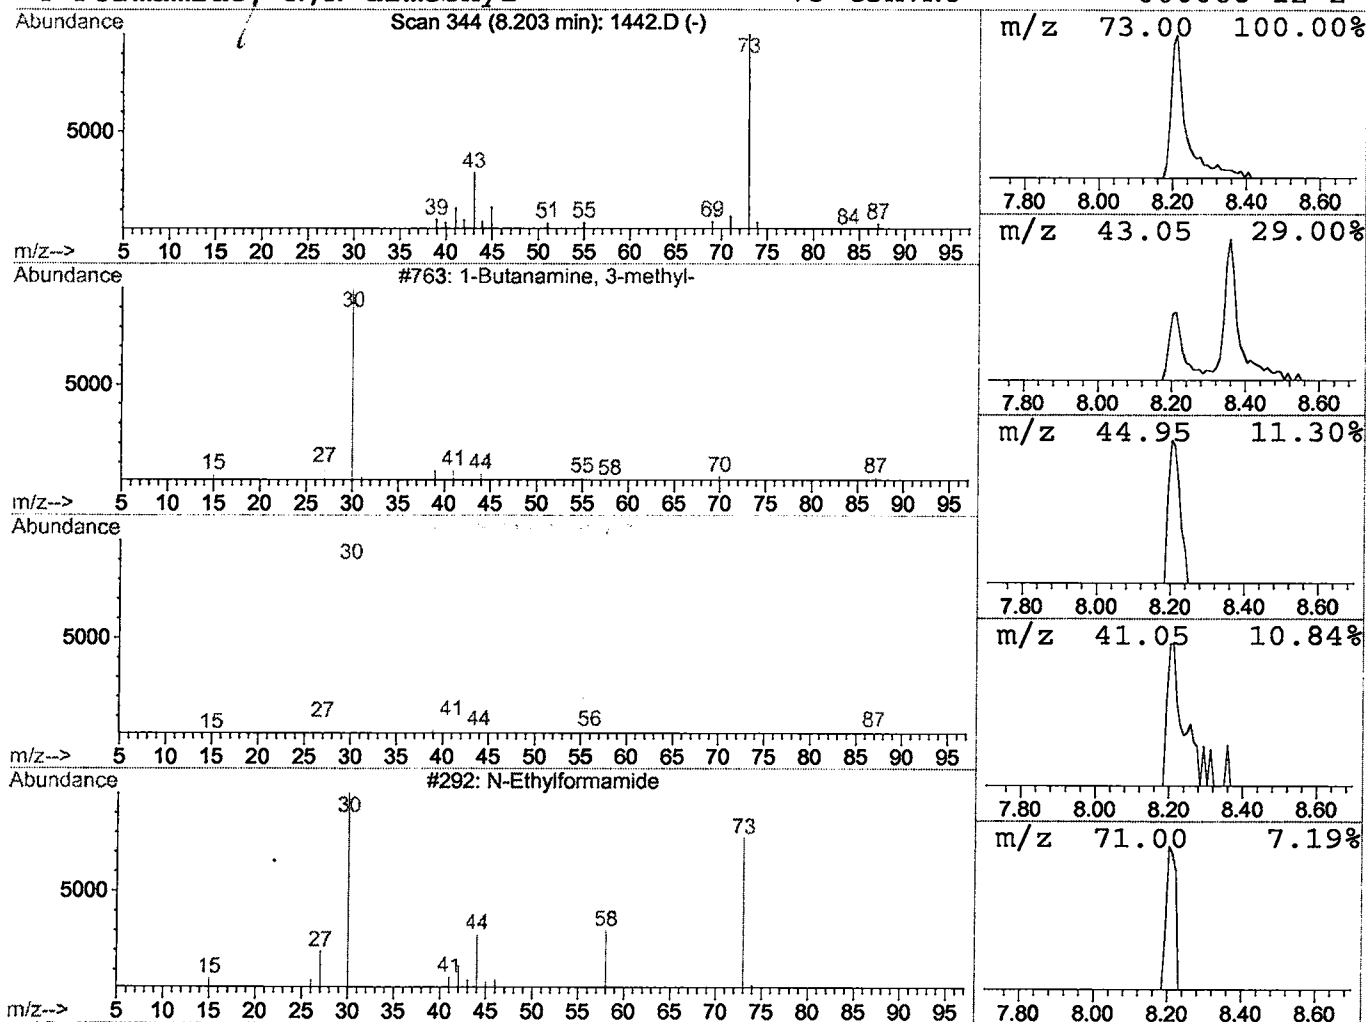

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 22 Feb 2002 2:54 am
 Data File: C:\HPCHEM\1\DATA\FEB2102\1442.D
 Name: gc/ms scan 1/22
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
1-Butanamine, 3-meth	8.20	0.4	ug/l	25531	ISTD01	12.33	1399700	20.0
1442.D GCMS0208.M	Fri Feb 22 09:36:39 2002							