

Method 508 MOD.Date Extracted 1-23-02Page 43

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
L.B.		500 ml		1 ml			1 ml	10A	7			
Ref					0.5 ml			2A				
1506								2B				
1507								4B				
1508	F.B.							6B				
1509								7A				
1510								4A				
1511								1A				
1547								9B				
1548								6A				
1636								7B				
1637								10B				
1638								9A				
Remarks												
① 1548 REQUIRES RE-EXTRACTION DUE TO LOW Surr. REC.												
② BATCH # GCMS-17110												
Reviewed by: <u>JB 8/13/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type - Sep. Fun. Solv. lot# <u>V39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39400</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	91759											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	GCMS 01/16/02											
LPC												
ENDRIN/DDT												

Analyst A.D.
revision 4/12/01

Verified by _____

Reviewed by _____
Date 3/5/02

DFTPP

Data File : C:\MSDCHEM\1\5973N\02FEB21\0221DF.D

Vial: 1

Acq On : 21 Feb 2002 8:45 am

Operator:

Sample : dftpp

Inst : Instrume


Misc : February 21, 2002

Multiplr: 1.00

MS Integration Params: SPLIT.P

Method : C:\MSDCHEM\1\METHODS\METHODS\HP020702.M (RTE Integrator)

Title : 508 scan method

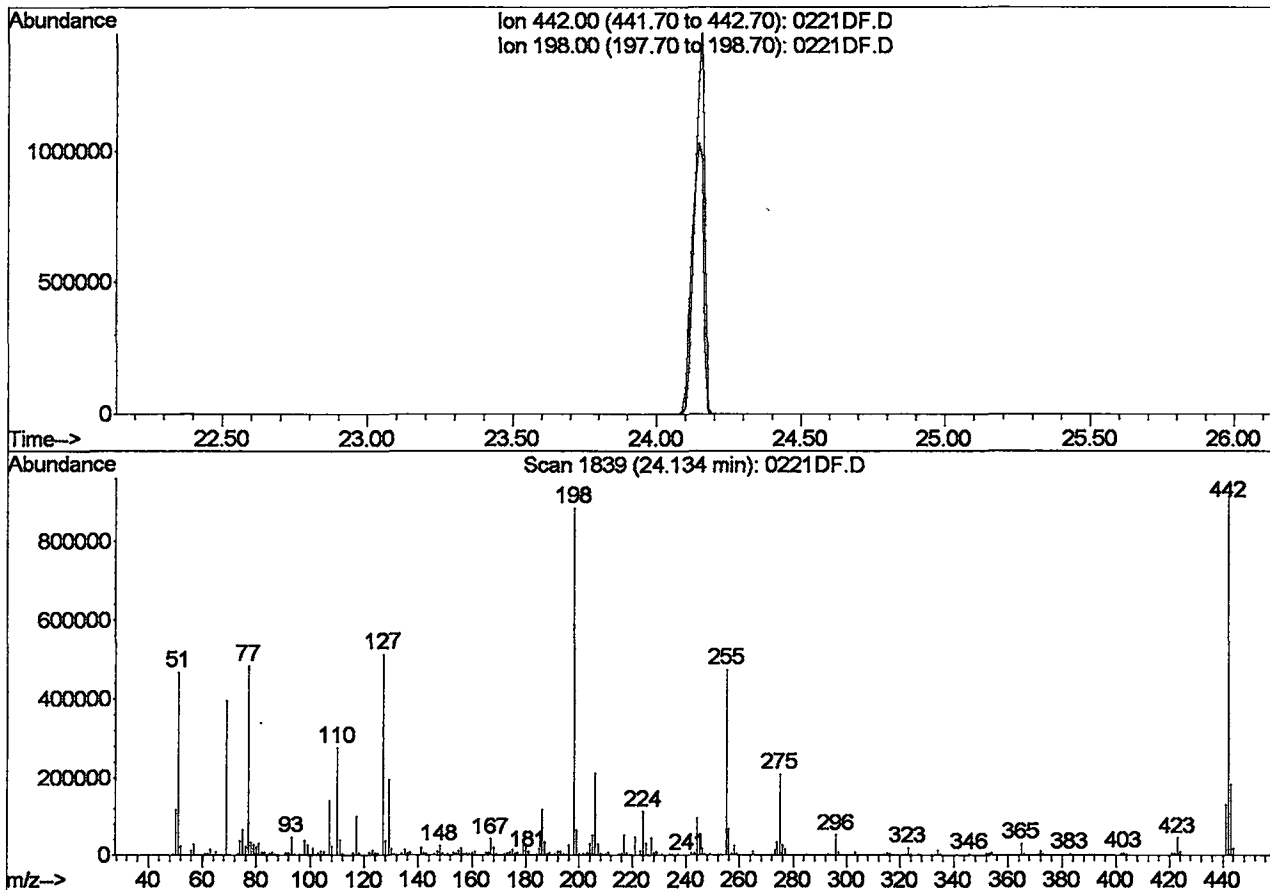

Spectrum Information: Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	52.9	468672	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.0	398336	PASS
70	69	0.00	2	0.5	2157	PASS
127	198	40	60	58.2	515008	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	885632	PASS
199	198	5	9	7.2	64208	PASS
275	198	10	30	23.7	209536	PASS
365	198	1	99	3.3	29120	PASS
441	443	1	99	72.9	133120	PASS
442	198	40	110	103.7	918464	PASS
443	442	17	23	19.9	182592	PASS

0221DF.D HP020702.M

Thu Feb 21 10:43:51 2002