

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 02/28/2002 Time: 09:36:41

Sample: AE01643
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 2/28/02 09:35 Ended: 2/28/02 09:35 Analyst: MG
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	n-Nitrosodimethylamine		< MDL		2.0
2	bis(2-Chloroethyl)ether		< MDL		2.0
3	1,3-Dichlorobenzene		< MDL		2.0
4	1,4-Dichlorobenzene		< MDL		2.0
5	1,2-Dichlorobenzene		< MDL		2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL		2.0
7	n-Nitrosodi-n-propylamine		< MDL		2.0
8	Hexachloroethane		< MDL		2.0
9	Nitrobenzene		< MDL		2.0
10	Isophorone		< MDL		2.0
11	bis(2-Chloroethoxy)methane		< MDL		2.0
12	1,2,4-Trichlorobenzene		< MDL		2.0
13	Naphthalene		< MDL		2.0
14	Hexachlorobutadiene		< MDL		2.0
15	2-Chloronaphthalene		< MDL		2.0
16	Dimethylphthalate		< MDL		2.0
17	2,6-Dinitrotoluene		< MDL		2.0
18	Acenaphthylene		< MDL		2.0
19	Acenaphthene		< MDL		2.0
20	2,4-Dinitrotoluene		< MDL		2.0
21	Diethylphthalate		< MDL		2.0
22	4-Chlorophenylphenylether		< MDL		2.0
23	Fluorene		< MDL		2.0
24	Azobenzene/1,2-Diphenylhydraz		< MDL		2.0
25	n-Nitrosodiphenylamine		< MDL		2.0
26	4-Bromophenylphenylether		< MDL		2.0
27	Hexachlorobenzene		< MDL		2.0
28	Phenanthrene		< MDL		2.0
29	Anthracene		< MDL		2.0
30	Di-n-butylphthalate		< MDL		2.0
31	Fluoranthene		< MDL		2.0
32	Pyrene		< MDL		2.0
33	Butylbenzylphthalate		< MDL		2.0
34	Benzo(a)anthracene		< MDL		2.0
35	bis(2-Ethylhexyl)phthalate		< MDL		2.0
36	Chrysene		< MDL		2.0
37	Di-n-octylphthalate		< MDL		2.0
38	Benzo(b)fluoranthene		< MDL		2.0
39	Benzo(k)fluoranthene		< MDL		2.0
40	Benzo(a)pyrene		< MDL		2.0
41	Indeno(1,2,3-cd)pyrene		< MDL		2.0
42	Dibenz(a,h)anthracene		< MDL		2.0
43	Benzo(g,h,i)perylene		< MDL		2.0

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB2502\LB.D

Vial: 3

Acq On : 25 Feb 2002 12:39 pm

Operator:

Sample : gc/ms scan 1/25

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 28 8:59 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 27 11:30:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.31	152	332465	20.00	ug/l	-0.04
10) Naphthalene-d8	15.96	136	1262537	20.00	ug/l	-0.04
17) Acenaphthene-d10	21.26	164	668222	20.00	ug/l	-0.05
29) Phenanthrene-d10	25.72	188	922402	20.00	ug/l	-0.05
38) Chrysene-d12	33.78	240	551241	20.00	ug/l	-0.07
44) Perylene-d12	38.05	264	358356	20.00	ug/l	-0.08

System Monitoring Compounds

37) 2,4-DDD	30.79	235	54621	5.67	ug/mL	0.30
Spiked Amount	5.000		Recovery	= 113.40%		

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	16.01	128	691	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)=qualifier out of range (m)=manual integration

LB.D GCMS0208.M Thu Feb 28 09:00:33 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB2502\LB.D
 Acq On : 25 Feb 2002 12:39 pm
 Sample : gc/ms scan 1/25
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Feb 28 8:59 2002

Vial: 3
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Feb 27 11:30:15 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	25.72	178	300	N.D.	
34) Anthracene	25.72	178	300	N.D.	
35) Di-n-butylphthalate	27.68	149	23047	0.30 ug/l	99
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo(a)anthracene	33.78	228	2418	N.D.	
42) Bis(2-ethylhexyl)phthalate	33.99	149	953	N.D.	
43) Chrysene	33.85	228	1344	N.D.	
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo(b)fluoranthene	36.85	252	729	N.D.	
47) Benzo(k)fluoranthene	36.85	252	1564	N.D.	
48) Benzo(a)pyrene	37.86	252	261	N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

 (#) = qualifier out of range (m) = manual integration

LB.D GCMS0208.M Thu Feb 28 09:00:37 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\FEB2502\LB.D
Acq On : 25 Feb 2002 12:39 pm
Sample : gc/ms scan 1/25
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 28 8:59 2002

Vial: 3
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 27 11:30:15 2002
Response via : Initial Calibration

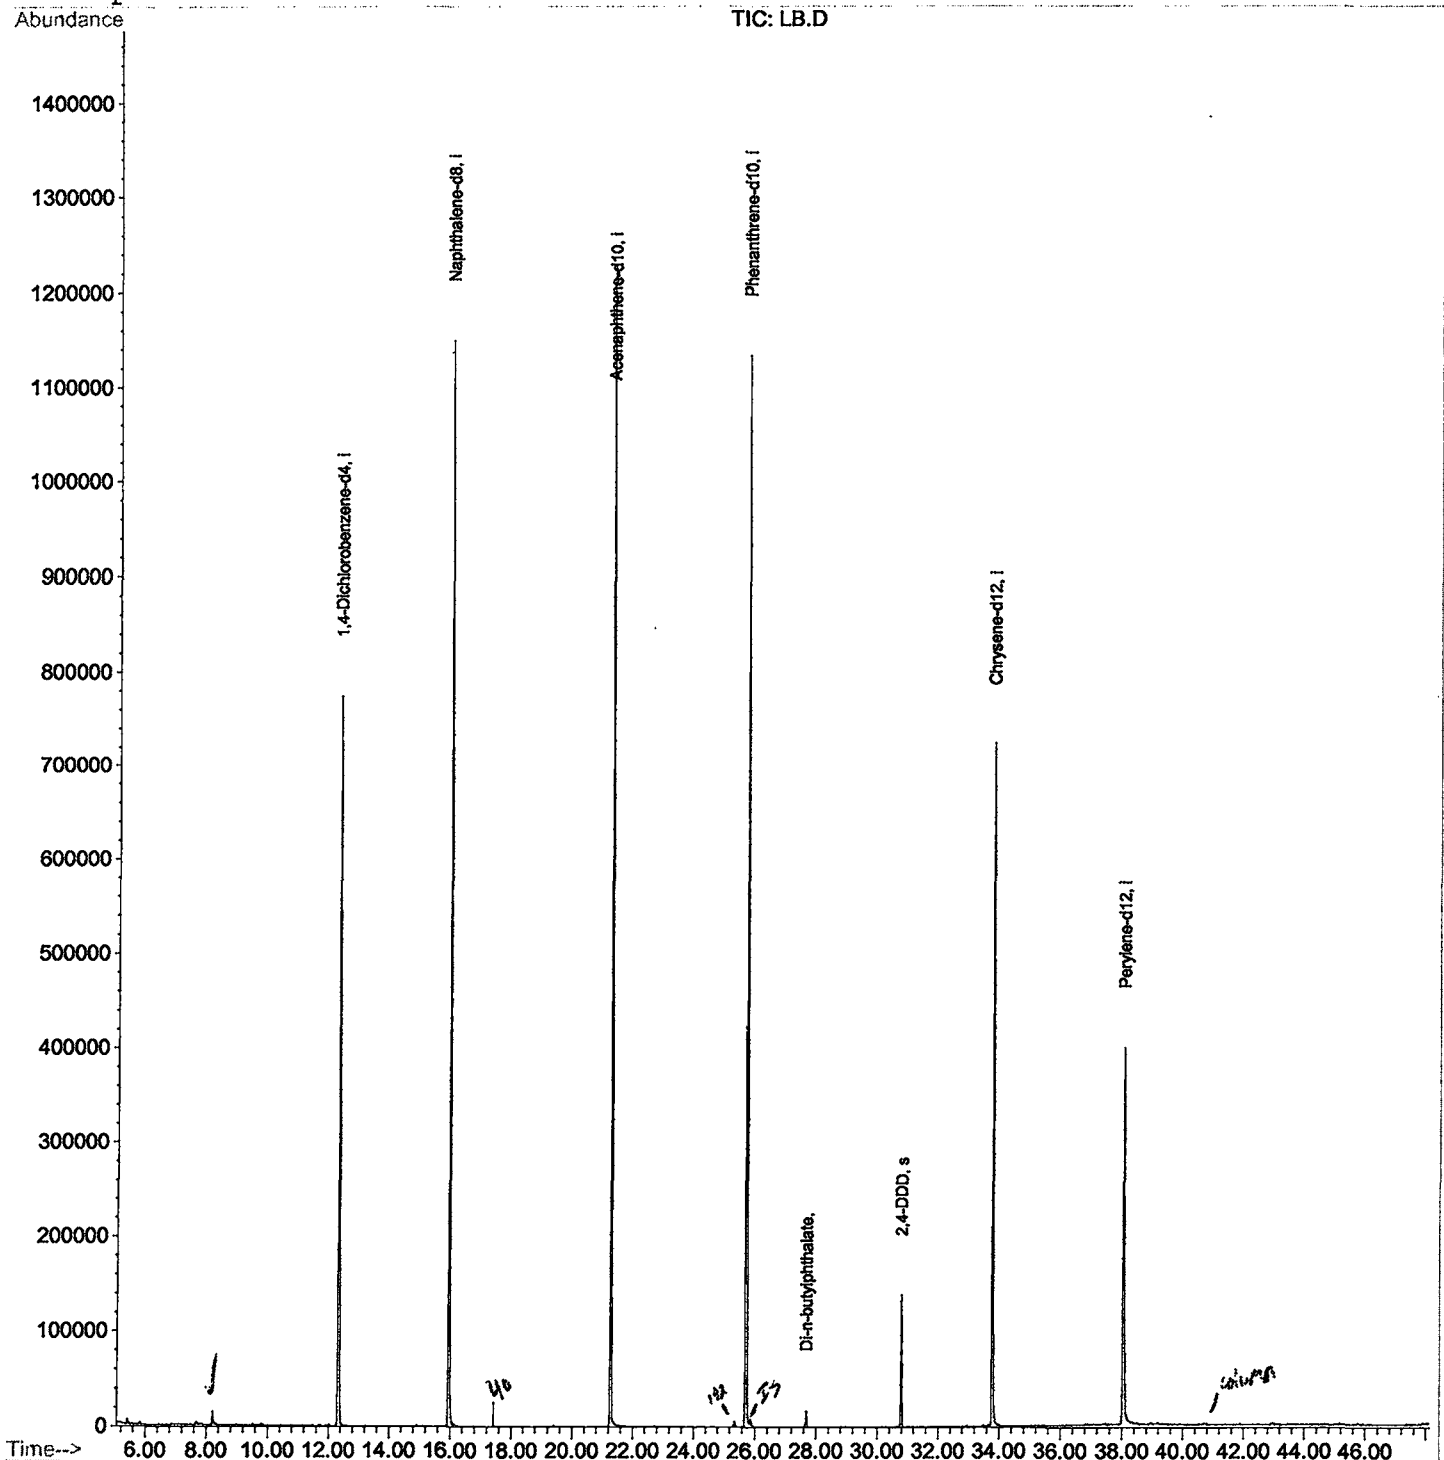

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB2502\LB.D
 Acq On : 25 Feb 2002 12:39 pm
 Sample : gc/ms scan 1/25
 Misc :
 MS Integration Params: LSCINT.P

Vial: 3
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.201	340	344	367	rVB	14900	44428	1.68%	0.352%
2	12.314	787	792	809	rVB	773709	1852019	70.09%	14.668%
3	15.958	1183	1189	1206	rBV	1150206	2449283	92.70%	19.398%
4	21.264	1761	1767	1784	rBV	1230274	2642245	100.00%	20.926%
5	25.717	2245	2252	2263	rBV2	1134542	2428489	91.91%	19.233%
6	27.681	2458	2466	2475	rBV	17039	34905	1.32%	0.276%
7	30.794	2800	2805	2811	rBV	138433	273623	10.36%	2.167%
8	33.777	3123	3130	3146	rBV2	723294	1649017	62.41%	13.060%
9	38.046	3587	3595	3610	rBV2	398650	1252379	47.40%	9.919%

Sum of corrected areas: 12626388

LB.D GCMS0208.M Thu Feb 28 09:36:09 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB2502\LB.D
 Operator :
 Acquired : 25 Feb 2002 12:39 pm using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 1/25
 Misc Info :
 Vial Number: 3
 Quant File :GCMS0208.RES (RTE Integrator)

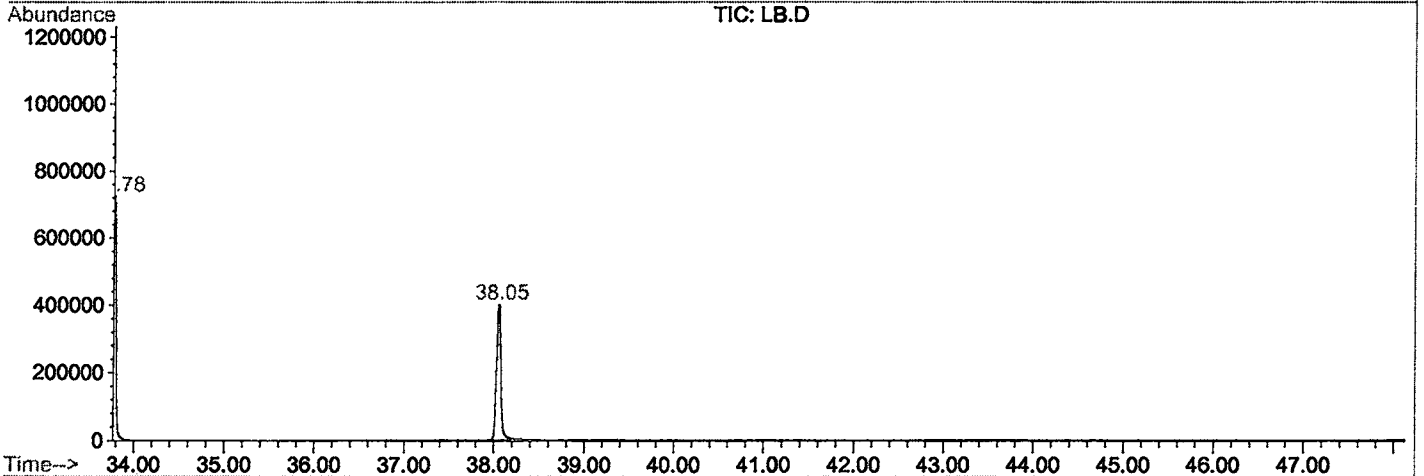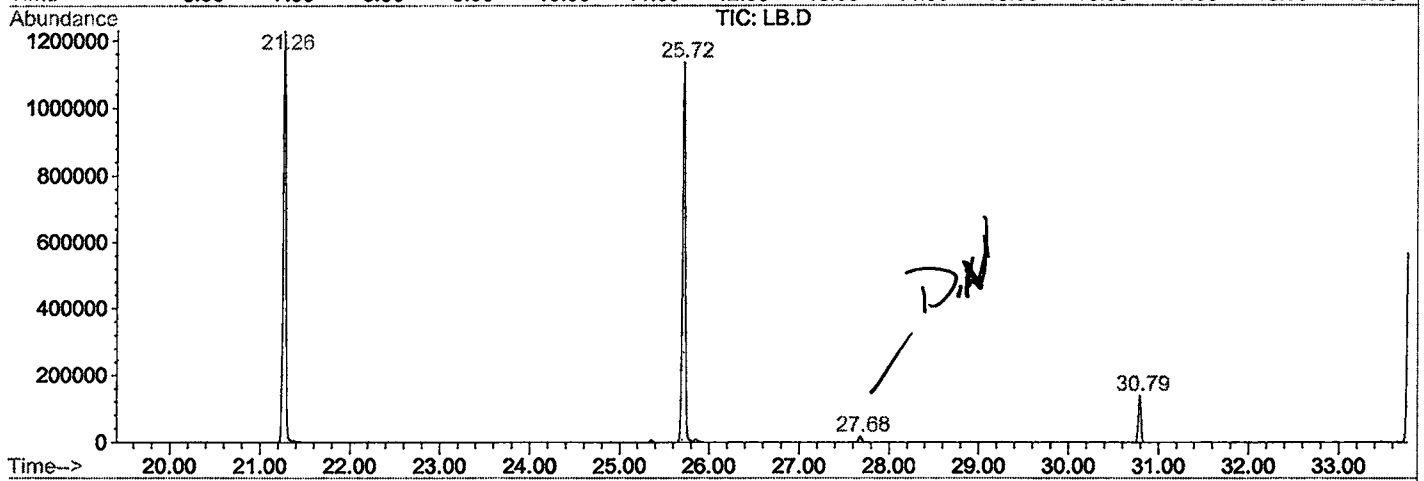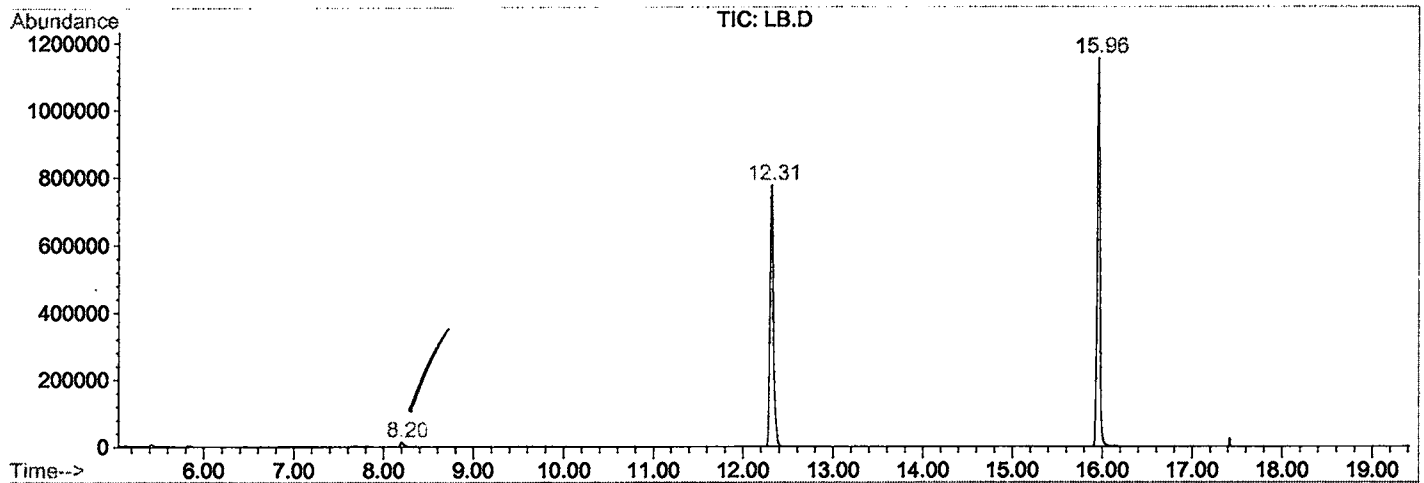

LB.D GCMS0208.M

Thu Feb 28 09:36:15 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB2502\LB.D
Acq On : 25 Feb 2002 12:39 pm
Sample : gc/ms scan 1/25
Misc :
MS Integration Params: LSCINT.P








Vial: 3
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 3-Pentanol, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.20	0.48 ug/l	44428	1,4-Dichlorobenzene-d4	12.31

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	28
2			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9
3			1-Hexanol, 6-amino-	117	C6H15NO	004048-33-3	9
4			Silane/tetramethyl-	88	C4H12Si	000075-76-3	9

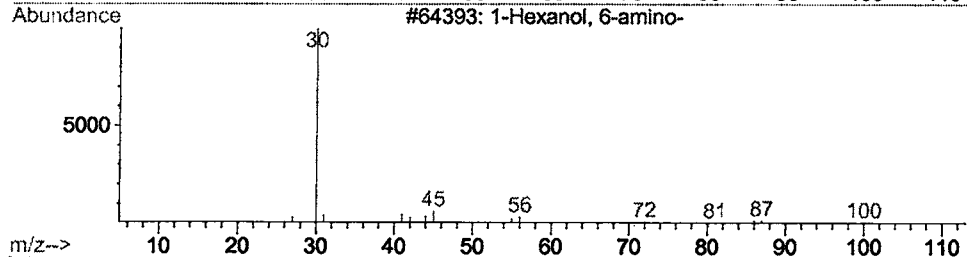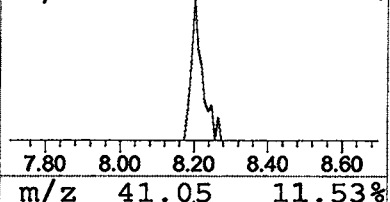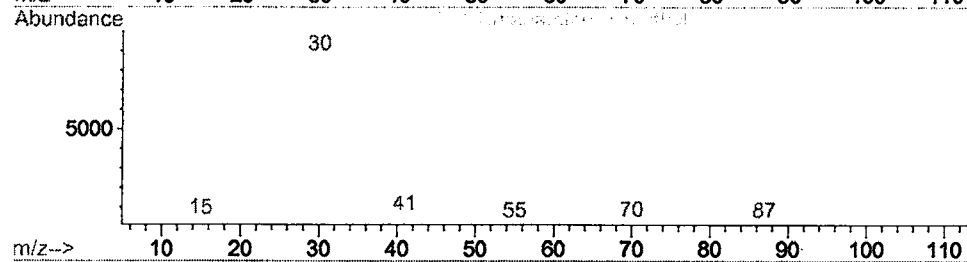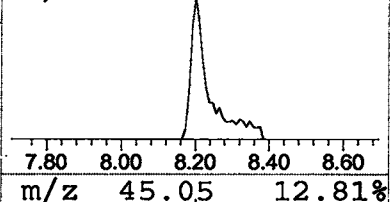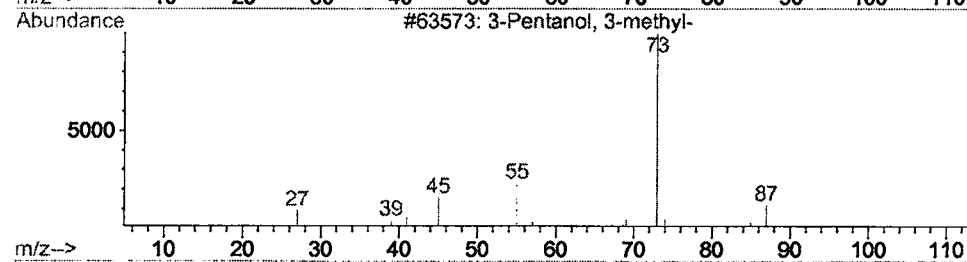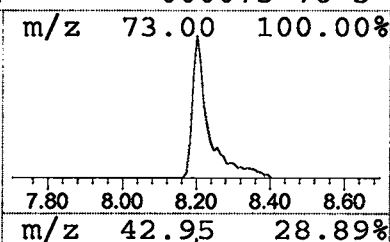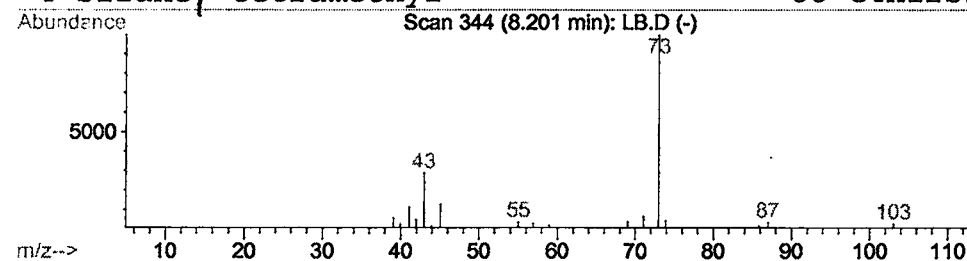

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 25 Feb 2002 12:39 pm
 Data File: C:\HPCHEM\1\DATA\FEB2502\LB.D
 Name: gc/ms scan 1/25
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
----- 3-Pentanol, 3-methyl	8.20	0.5	ug/l	44428	ISTD01	12.31	1852020	20.0

LB.D GCMS0208.M Thu Feb 28 09:36:24 2002