

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 03/04/2002 Time: 15:21:18

Sample: AE01687
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 3/4/02 15:20 Ended: 3/4/02 15:20 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		102		5.0

Comments for Sample AE01687 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-04-2002 Time: 15:21:21

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 1 of the 43 compounds in the LCS Standard was below its acceptance range.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB2502\1687.D

Vial: 8

Acq On : 25 Feb 2002 6:24 pm

Operator:

Sample : gc/ms scan 1/25

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 28 9:09 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 27 11:30:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.32	152	242448	20.00	ug/l	-0.04
10) Naphthalene-d8	15.95	136	911241	20.00	ug/l	-0.05
17) Acenaphthene-d10	21.27	164	477030	20.00	ug/l	-0.05
29) Phenanthrene-d10	25.71	188	629084	20.00	ug/l	-0.06
38) Chrysene-d12	33.78	240	351059	20.00	ug/l	-0.06
44) Perylene-d12	38.05	264	226814	20.00	ug/l	-0.07

System Monitoring Compounds

37) 2,4-DDD	30.79	235	33400	5.08	ug/mL	0.29
Spiked Amount	5.000		Recovery	=	101.60%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	16.02	128	463	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)= qualifier out of range (m) = manual integration

1687.D GCMS0208.M

Thu Feb 28 09:10:52 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB2502\1687.D

Vial: 8

Acq On : 25 Feb 2002 6:24 pm

Operator:

Sample : gc/ms scan 1/25

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 28 9:09 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 27 11:30:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	27.68	149	8174	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.78	228	610	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.98	149	1388	N.D.		
43) Chrysene	33.78	228	610	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.05	252	721	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

1687.D GCMS0208.M Thu Feb 28 09:10:56 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\FEB2502\1687.D
 Acq On : 25 Feb 2002 6:24 pm
 Sample : gc/ms scan 1/25
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Feb 28 9:09 2002

Vial: 8
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Feb 27 11:30:15 2002
 Response via : Initial Calibration

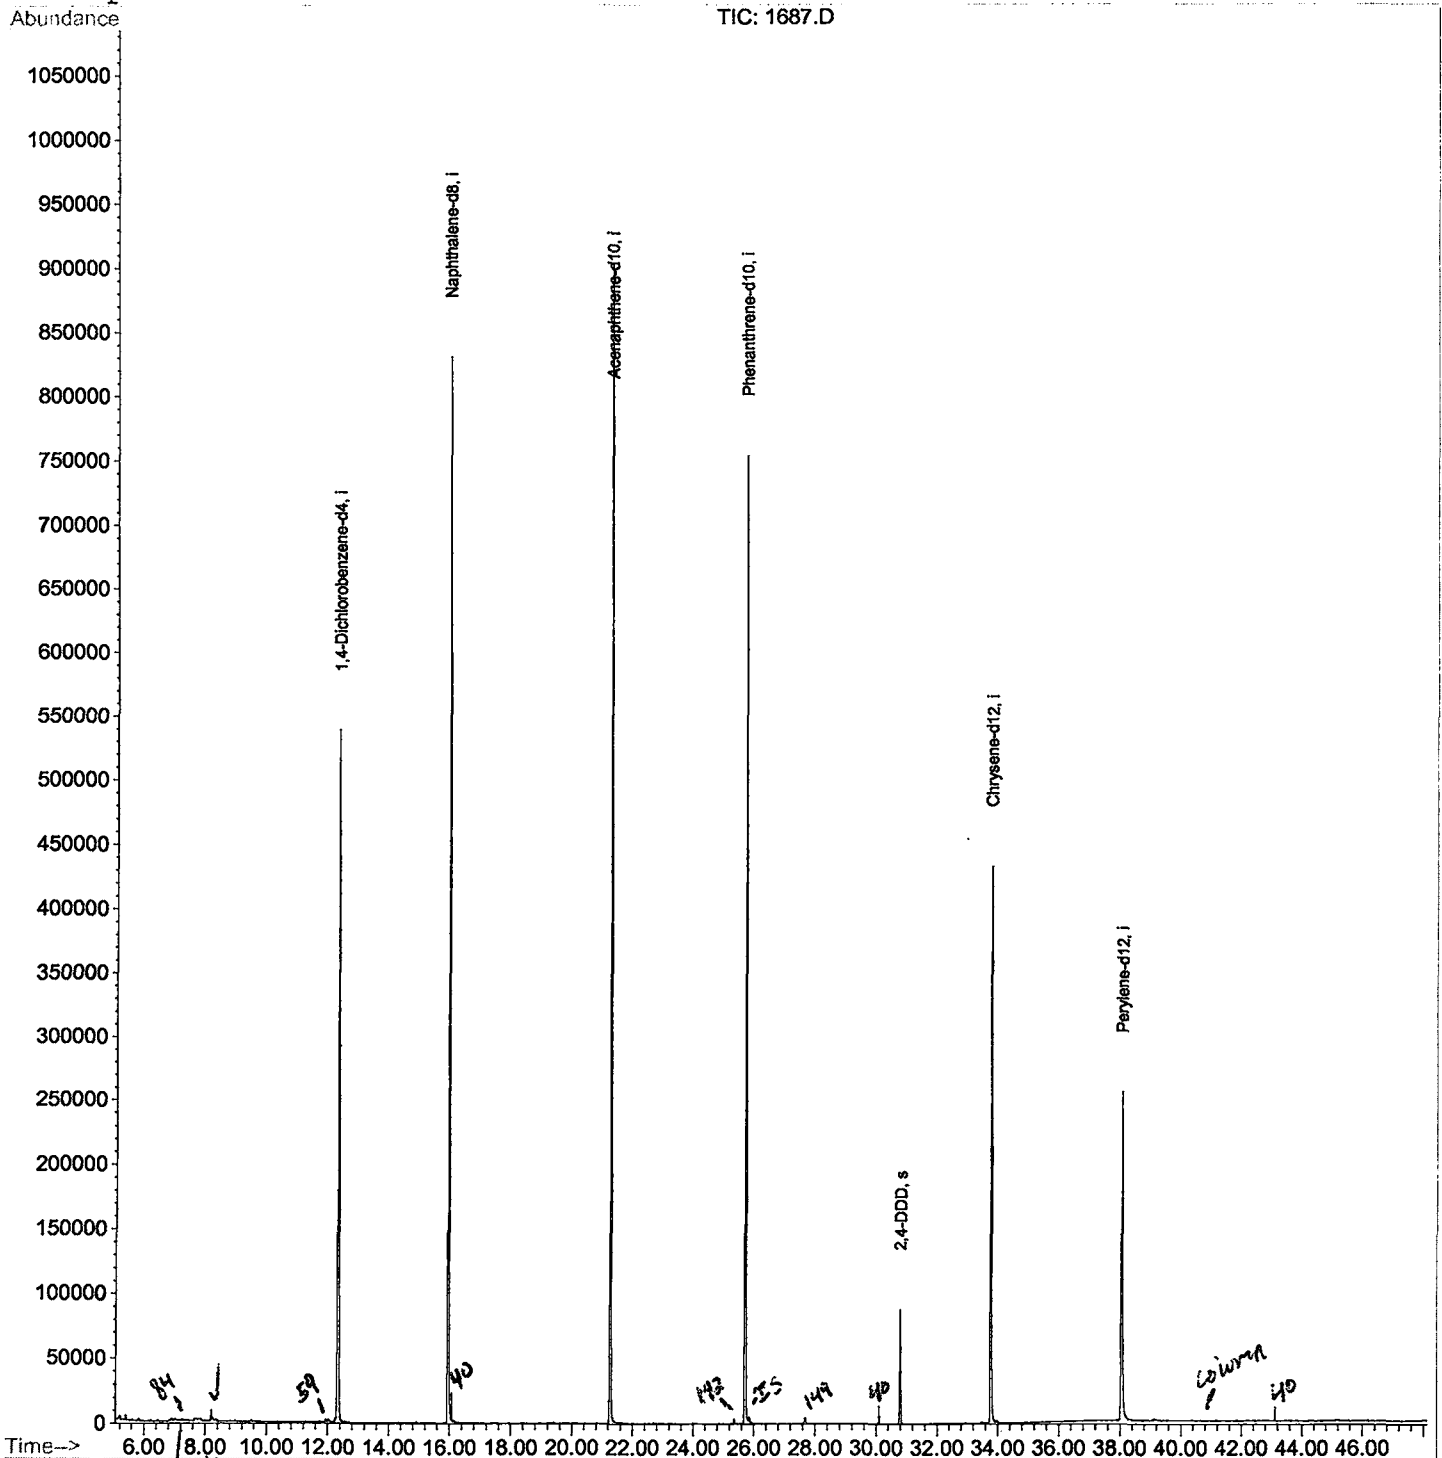

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB2502\1687.D
 Acq On : 25 Feb 2002 6:24 pm
 Sample : gc/ms scan 1/25
 Misc :
 MS Integration Params: LSCINT.P

Vial: 8
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.195	339	343	348	rBV	8801	19431	1.04%	0.224%
2	12.317	787	792	806	rVB	537377	1366253	72.82%	15.772%
3	15.952	1182	1188	1200	rBV	830586	1765397	94.09%	20.380%
4	21.268	1761	1767	1780	rBV	903173	1876270	100.00%	21.660%
5	25.711	2245	2251	2263	rBV2	753696	1633811	87.08%	18.861%
6	30.788	2800	2804	2811	rBV	88464	168188	8.96%	1.942%
7	33.780	3123	3130	3145	rBV2	432090	1042893	55.58%	12.039%
8	38.049	3587	3595	3609	rBV2	254780	790080	42.11%	9.121%

Sum of corrected areas: 8662323

1687.D GCMS0208.M Thu Feb 28 09:31:16 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB2502\1687.D
Operator :
Acquired : 25 Feb 2002 6:24 pm using AcqMethod GCMS0208
Instrument : GC/MS 209
Sample Name: gc/ms scan 1/25
Misc Info :
Vial Number: 8
Quant File :GCMS0208.RES (RTE Integrator)

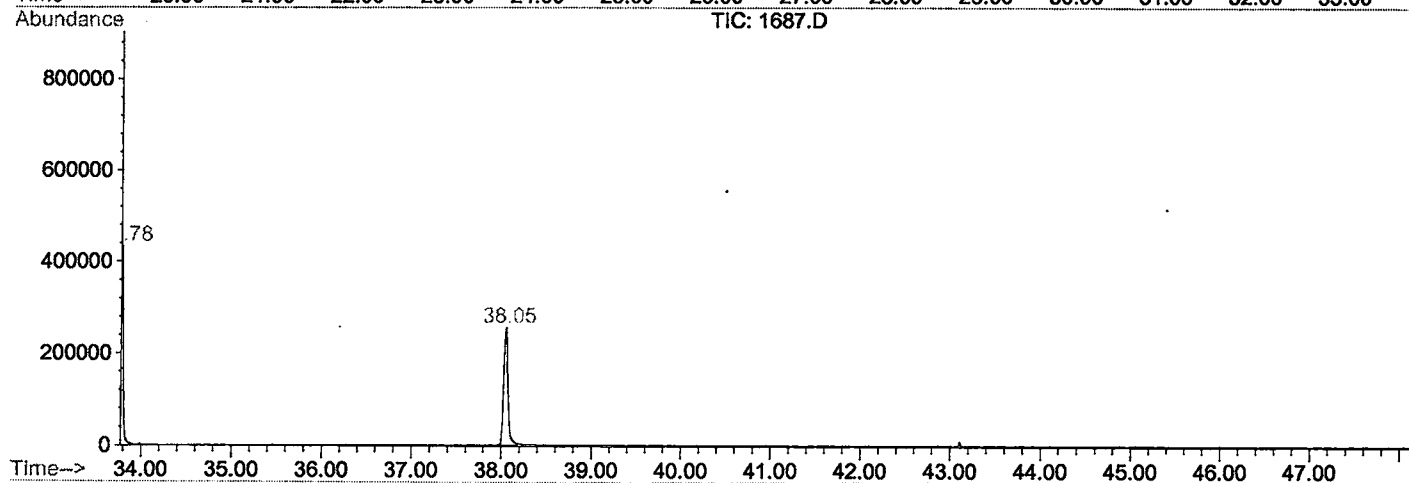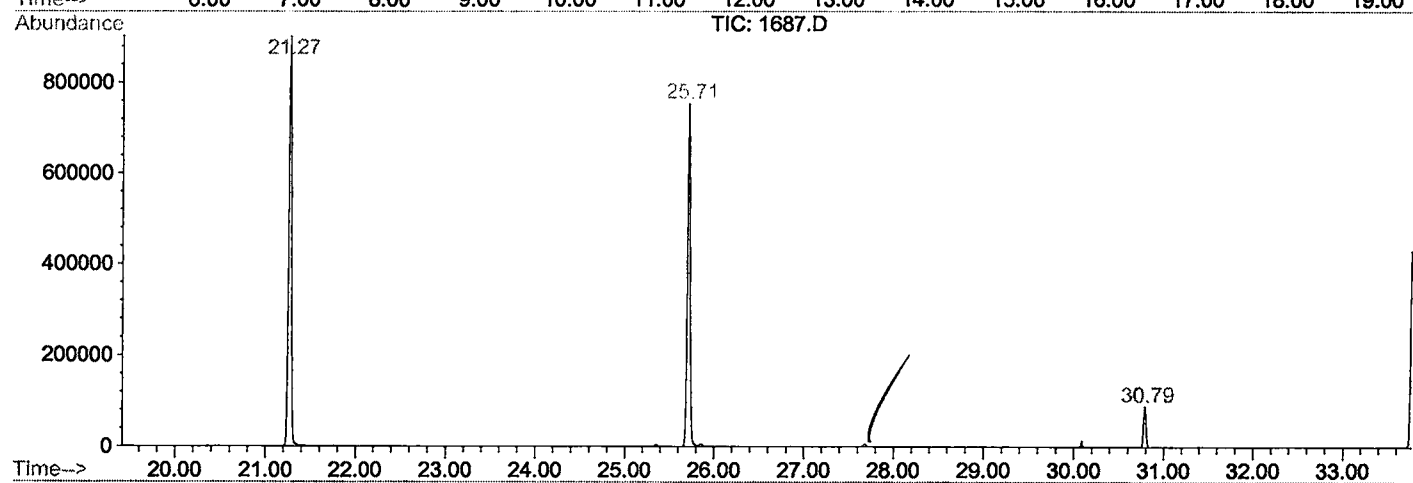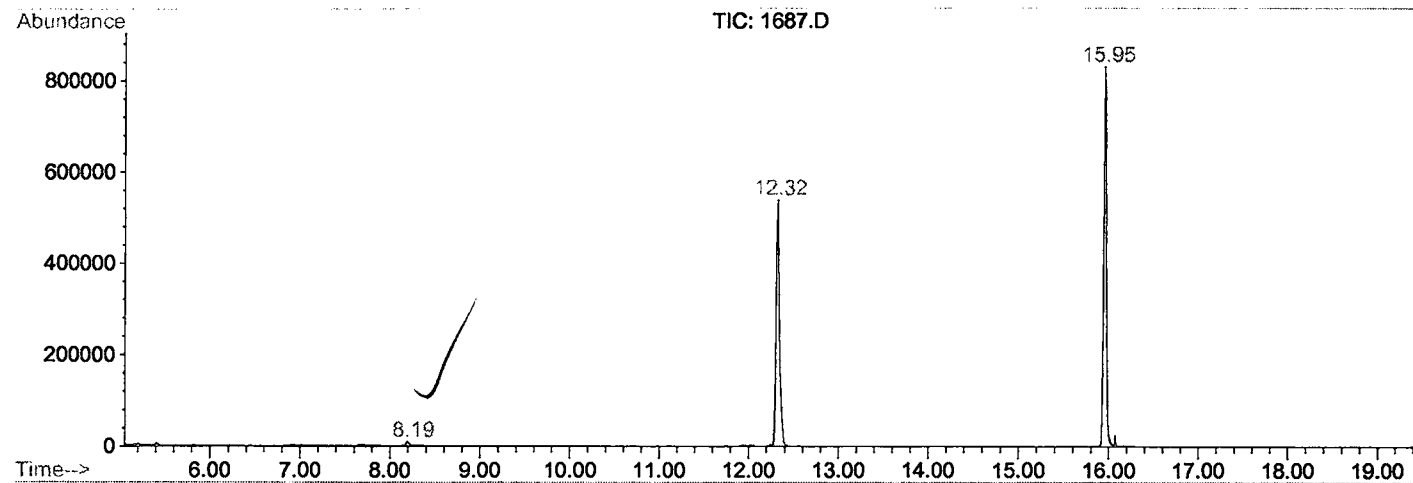

1687.D GCMS0208.M

Thu Feb 28 09:31:21 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\FEB2502\1687.D
 Acq On : 25 Feb 2002 6:24 pm
 Sample : gc/ms scan 1/25
 Misc :
 MS Integration Params: LSCINT.P


Vial: 8
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Methyl-5-hexen-3-ol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.19	0.28 ug/l	19431	1,4-Dichlorobenzene-d4	12.32

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	23
2	N-Ethylformamide	73	C3H7NO	000627-45-2	5
3	Formic acid, ethyl ester	74	C3H6O2	000109-94-4	5
4	1,3-Dioxolane	74	C3H6O2	000646-06-0	4

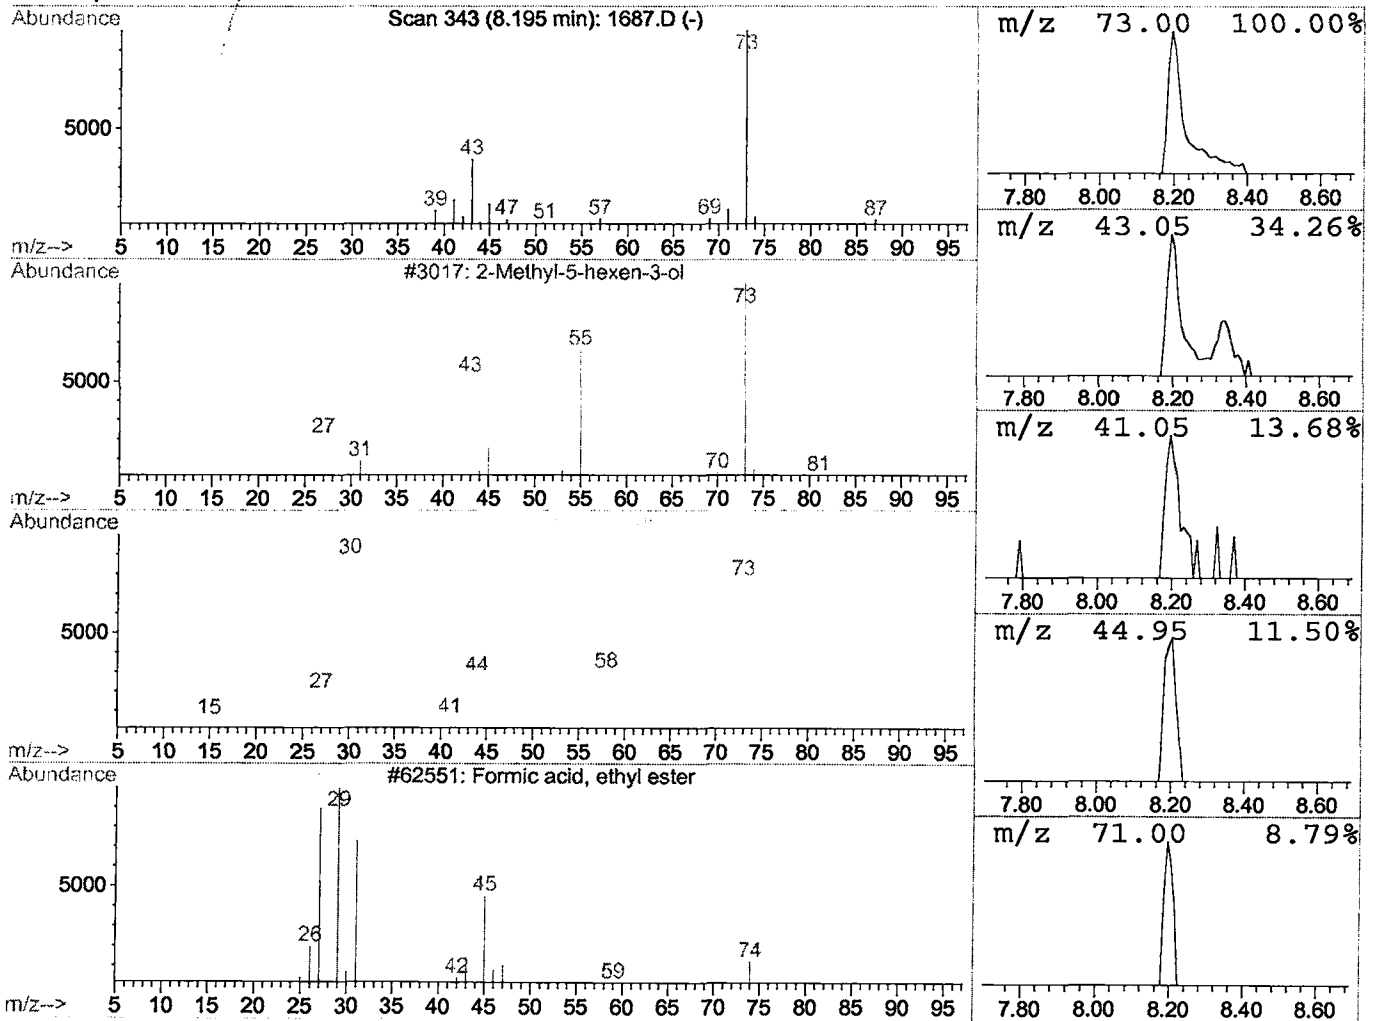

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 25 Feb 2002 6:24 pm
 Data File: C:\HPCHEM\1\DATA\FEB2502\1687.D
 Name: gc/ms scan 1/25
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Methyl-5-hexen-3-ol	8.19	0.3	ug/l	19431	ISTD01	12.32	1366250	20.0

1687.D GCMS0208.M Thu Feb 28 09:31:30 2002