

Method 508 MOD.

Date Extracted 3-5-02

Reextraction

Page 127

All - Reextracts

Ref

H.G.C.M.S. 17561

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
<i>L.B.</i>		<i>500 ml</i>		<i>1 ml</i>			<i>1 ml</i>	<i>10 A</i>	<i>7</i>			
<i>Ref 1</i>					<i>1 ml</i>			<i>7 B</i>				
<i>Ref 2</i>					<i>1 ml</i>			<i>9 A</i>				
<i>1960</i>								<i>7 A</i>				
<i>1961</i>	<i>Q</i>							<i>10 B</i>				
<i>1962</i>								<i>2 B</i>				
<i>1963</i>								<i>6 A</i>				
<i>1964</i>	<i>Q</i>							<i>2 A</i>				
<i>1966</i>								<i>8 A</i>				
<i>1967</i>	<i>FB</i>							<i>8 B</i>				
<i>1968</i>								<i>10 B</i>				
<i>1969</i>								<i>9 B</i>				
<i>1970</i>	<i>FB</i>							<i>1 A</i>				
Remarks Reviewed by, <i>[Signature]</i> 8/15/02												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - <i>SEP. Flm</i> Solv. lot# <i>V 16469</i> NaCl lot# <i>V 39618</i> Na2SO4 lot# <i>V 46623</i>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF SPIKE	<i>2193</i>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<i>030102</i>											
SURROGATE	<i>20602</i>											
LPC												
ENDRIN/DDT												

Analyst A.D.
revision 4/12/01

Verified by _____

Reviewed by *[Signature]*

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAR1902.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\mar1902\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

(X) Full Method

(X) Inject Anyway

() Reprocessing Only

() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0308	
2	Sample	2	CAL10	GCMS0308	
3	Sample	30	LB625	GCMS0308	1b 625bn
4	Sample	31	6470	GCMS0308	625bn
5	Sample	32	6471	GCMS0308	625bn
6	Sample	33	6472	GCMS0308	625bn
7	Sample	34	REFA	GCMS0308	625bn
8	Sample	35	REFB	GCMS0308	625bn
9	Sample	1	DFTPP1	GCMS0308	
10	Sample	2	CAL10A	GCMS0308	
11	Sample	3	LB	GCMS0308	gc/ms scan 3/5
12	Sample	4	REF1	GCMS0308	gc/ms scan 3/5
13	Sample	5	REF2	GCMS0308	gc/ms scan 3/5
14	Sample	6	1960	GCMS0308	gc/ms scan 3/5
15	Sample	7	1961	GCMS0308	gc/ms scan 3/5
16	Sample	8	1962	GCMS0308	gc/ms scan 3/5
17	Sample	9	1963	GCMS0308	gc/ms scan 3/5
18	Sample	10	1964	GCMS0308	gc/ms scan 3/5
19	Sample	1	DFTPP2	GCMS0308	
20	Sample	2	CAL40	GCMS0308	new
21	Sample	31	6470A	GCMS0308	625bn
22	Sample	32	6471A	GCMS0308	625bn
23	Sample	33	6472A	GCMS0308	625bn
24	Sample	11	1966	GCMS0308	gc/ms scan 3/5
25	Sample	30	CAL40BZ	GCMS0308	gc/ms scan 3/4
26	Sample	12	1967	GCMS0308	gc/ms scan 3/5 fb
27	Sample	13	1968	GCMS0308	gc/ms scan 3/5
28	Sample	14	1969	GCMS0308	gc/ms scan 3/5
29	Sample	15	1970	GCMS0308	gc/ms scan 3/5 fb
30	Sample	16	LBA1	GCMS0308	gc/ms scan 3/4
31	Sample	17	REFA1	GCMS0308	gc/ms scan 3/4
32	Sample	18	REFA2	GCMS0308	gc/ms scan 3/4
33	Sample	19	2460	GCMS0308	gc/ms scan 3/4 fb
34	Sample	20	2561	GCMS0308	gc/ms scan 3/4
35	Sample	21	2565	GCMS0308	gc/ms scan 3/4
36	Sample	22	2567	GCMS0308	gc/ms scan 3/4
37	Sample	23	2568	GCMS0308	gc/ms scan 3/4 fb
38	Sample	24	2575	GCMS0308	gc/ms scan 3/4
39	Sample	25	2576	GCMS0308	gc/ms scan 3/4
40	Sample	26	2577	GCMS0308	gc/ms scan 3/4
41	Sample	27	2578	GCMS0308	gc/ms scan 3/4 fb
42	Sample	28	2579	GCMS0308	gc/ms scan 3/4

Last Modified: Thu Mar 21 08:53:36 2002

Page: 1

43, Sample 29 4336 GCMS0308 gc/ms scan 3/4

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR1902\DFTPP1.D

Acq On : 19 Mar 2002 11:07 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

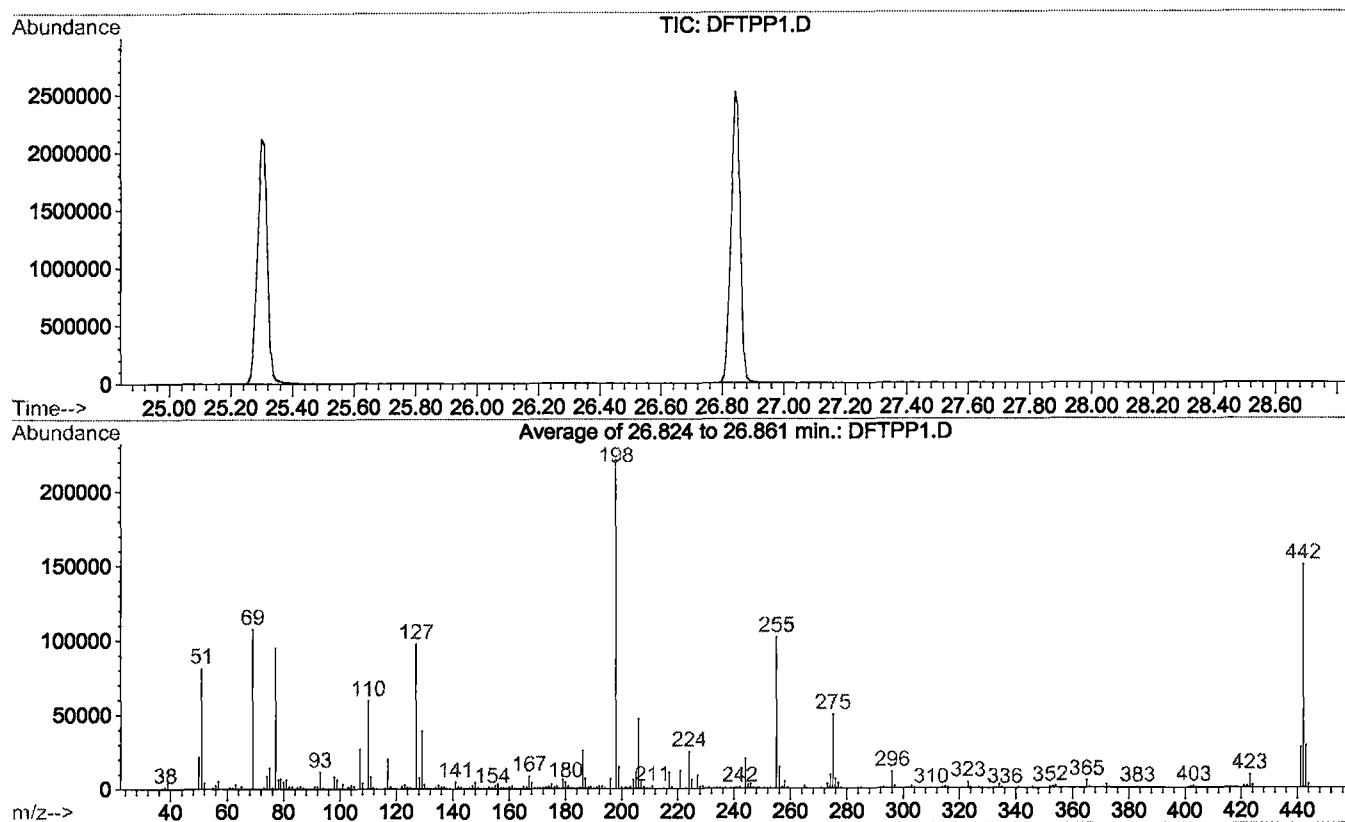

Spectrum Information: Average of 26.824 to 26.861 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.8	81301	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.7	107606	PASS
70	69	0.00	2	0.1	60	PASS
127	198	40	60	44.1	97554	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	221134	PASS
199	198	5	9	6.8	15045	PASS
275	198	10	30	22.6	50018	PASS
365	198	1	100	2.4	5203	PASS
441	443	0.01	100	95.8	27790	PASS
442	198	40	110	67.9	150192	PASS
443	442	17	23	19.3	29022	PASS

DFTPP1.D GCMS0308.M

Thu Mar 21 08:48:52 2002