

Method 508 mod.

Date Extracted 1/31/02

Page 59

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500ml		1ml			1ml	1A	7			
REF					5ml			7B				
2152	FB							7A				
2334								5A				
2335								2A				
2336								6A				
2337								3A				
2338								5B				
2339								4B				
2340								1B				
2341	FB							2B				
2380								3B				
2381								4A				
Remarks												
Reviewed by, <u>CS 8/13/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type <u>Sep Fun</u> Solv. lot# <u>V41470</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39H00</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF SPIKE	<u>91759</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>15022202</u>											
SURROGATE	<u>GCMS</u> <u>011602</u>											
LPC												
ENDRIN/DDT												

Analyst EH
revision 4/12/01

Verified by

Reviewed by

DN
3/22/02

Sequence Name: C:\MSDCHEM\1\SEQUENCE\030402.S

Comment:

Operator: McLean

Data Path: C:\MSDCHEM\1\DATA\030402\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	508SCAN	DFTPP
2	Sample	2	CAL25X	508SCAN	CAL 25
3	Sample	4	0131REF	508SCAN	1/31
4	Sample	5	0131LB	508SCAN	1/31
5	Sample	6	2152	508SCAN	1/31
6	Sample	7	2335	508SCAN	1/31
7	Sample	8	2336	508SCAN	1/31
8	Sample	9	2337	508SCAN	1/31
9	Sample	10	2338	508SCAN	1/31
10	Sample	11	2339	508SCAN	1/31
11	Sample	12	2340	508SCAN	1/31
12	Sample	13	2341	508SCAN	1/31
13	Sample	14	2334	508SCAN	1/31
14	Sample	15	2380	508SCAN	1/31
15	Sample	16	2381	508SCAN	1/31
16	Sample	1	DFTPPB	508SCAN	1/31
17	Sample	2	CAL25	508SCAN	1/31
18	Sample	3	CAL10X	508SCAN	1/31
19	Sample	17	REF131B	508SCAN	1/31
20	Sample	18	LB131	508SCAN	1/31
21	Sample	19	2092	508SCAN	1/31
22	Sample	20	2093	508SCAN	1/31
23	Sample	21	2094	508SCAN	1/31
24	Sample	22	2095	508SCAN	1/31 FB
25	Sample	23	2145	508SCAN	1/31
26	Sample	24	2146	508SCAN	1/31
27	Sample	25	04881	508SCAN	UNKOWN
28	Sample	26	04882	508SCAN	UNKOWN

DFTPP

Data File : C:\MSDCHEM\1\DATA\030402\DFTPP.D

Acq On : 4 Mar 2002 6:00 am

Sample : DFTPP

Misc :

MS Integration Params: BENZO.P

Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)


Title : Quantitation For Method 508gcscan

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

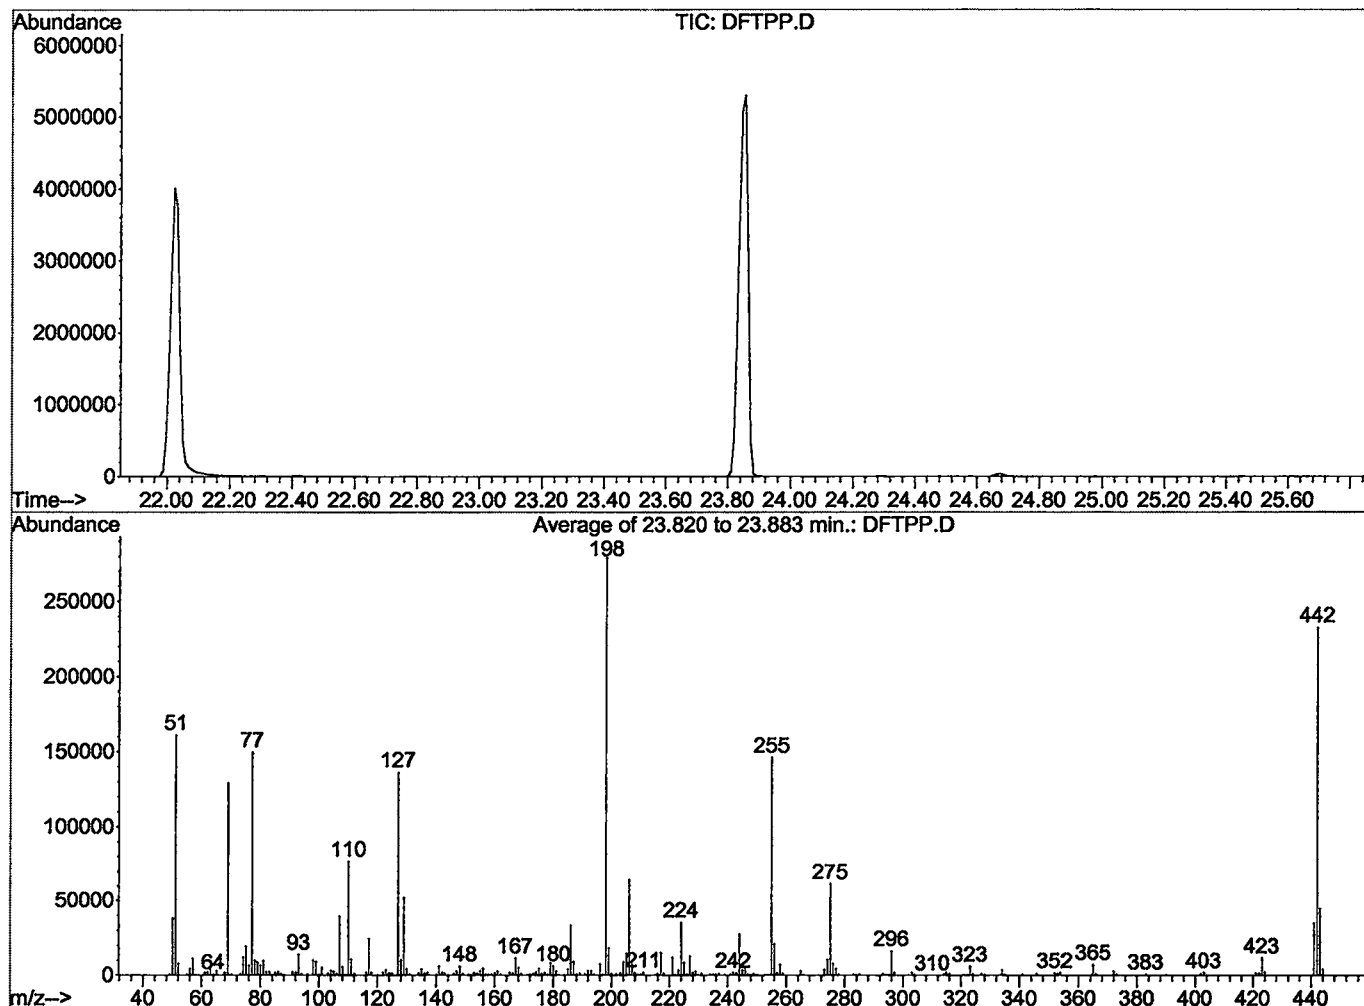

Spectrum Information: Average of 23.820 to 23.883 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.8	161267	PASS
68	69	0.00	2	1.4	1831	PASS
69	198	0.00	100	46.4	129443	PASS
70	69	0.00	2	0.4	520	PASS
127	198	10	80	48.9	136448	PASS
197	198	0.00	2	0.2	557	PASS
198	198	50	100	100.0	279083	PASS
199	198	5	9	6.6	18447	PASS
275	198	10	60	22.0	61482	PASS
365	198	1	100	2.6	7309	PASS
441	443	0.01	100	77.8	34826	PASS
442	198	50	100	83.4	232814	PASS
443	442	15	24	19.2	44746	PASS