

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR0102\3437.D

Vial: 49

Acq On : 3 Mar 2002 11:35 am

Operator:

Sample : gc/ms scan 2/4

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 6 11:43 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Mar 06 11:41:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

*John
to be
re-im*

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.32	152	722802	20.00	ug/l	-0.03
10) Naphthalene-d8	15.97	136	2808675	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.28	164	1486429	20.00	ug/l	-0.03
29) Phenanthrene-d10	25.72	188	2198457	20.00	ug/l	-0.04
38) Chrysene-d12	33.79	240	1493802	20.00	ug/l	-0.05
44) Perylene-d12	38.07	264	1023708	20.00	ug/l	-0.05

System Monitoring Compounds

37) 2,4-DDD	30.79	235	68538	2.99	ug/mL	0.29
Spiked Amount	5.000		Recovery	=	59.80%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	16.01	128	344	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)=qualifier out of range (m)=manual integration

3437.D GCMS0208.M

Mon Mar 25 12:14:36 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR0102\3437.D

Vial: 49

Acq On : 3 Mar 2002 11:35 am

Operator:

Sample : gc/ms scan 2/4

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 6 11:43 2002

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Mar 06 11:41:15 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.72	178	753	N.D.		
34) Anthracene	25.72	178	753	N.D.		
35) Di-n-butylphthalate	27.68	149	1118	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.79	228	3596	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.99	149	3986	N.D.		
43) Chrysene	33.79	228	3596	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.07	252	3914	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

3437.D GCMS0208.M Mon Mar 25 12:14:39 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAR0102\3437.D
 Acq On : 3 Mar 2002 11:35 am
 Sample : gc/ms scan 2/4
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Mar 6 11:43 2002

Vial: 49
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Feb 27 11:30:15 2002
 Response via : Initial Calibration

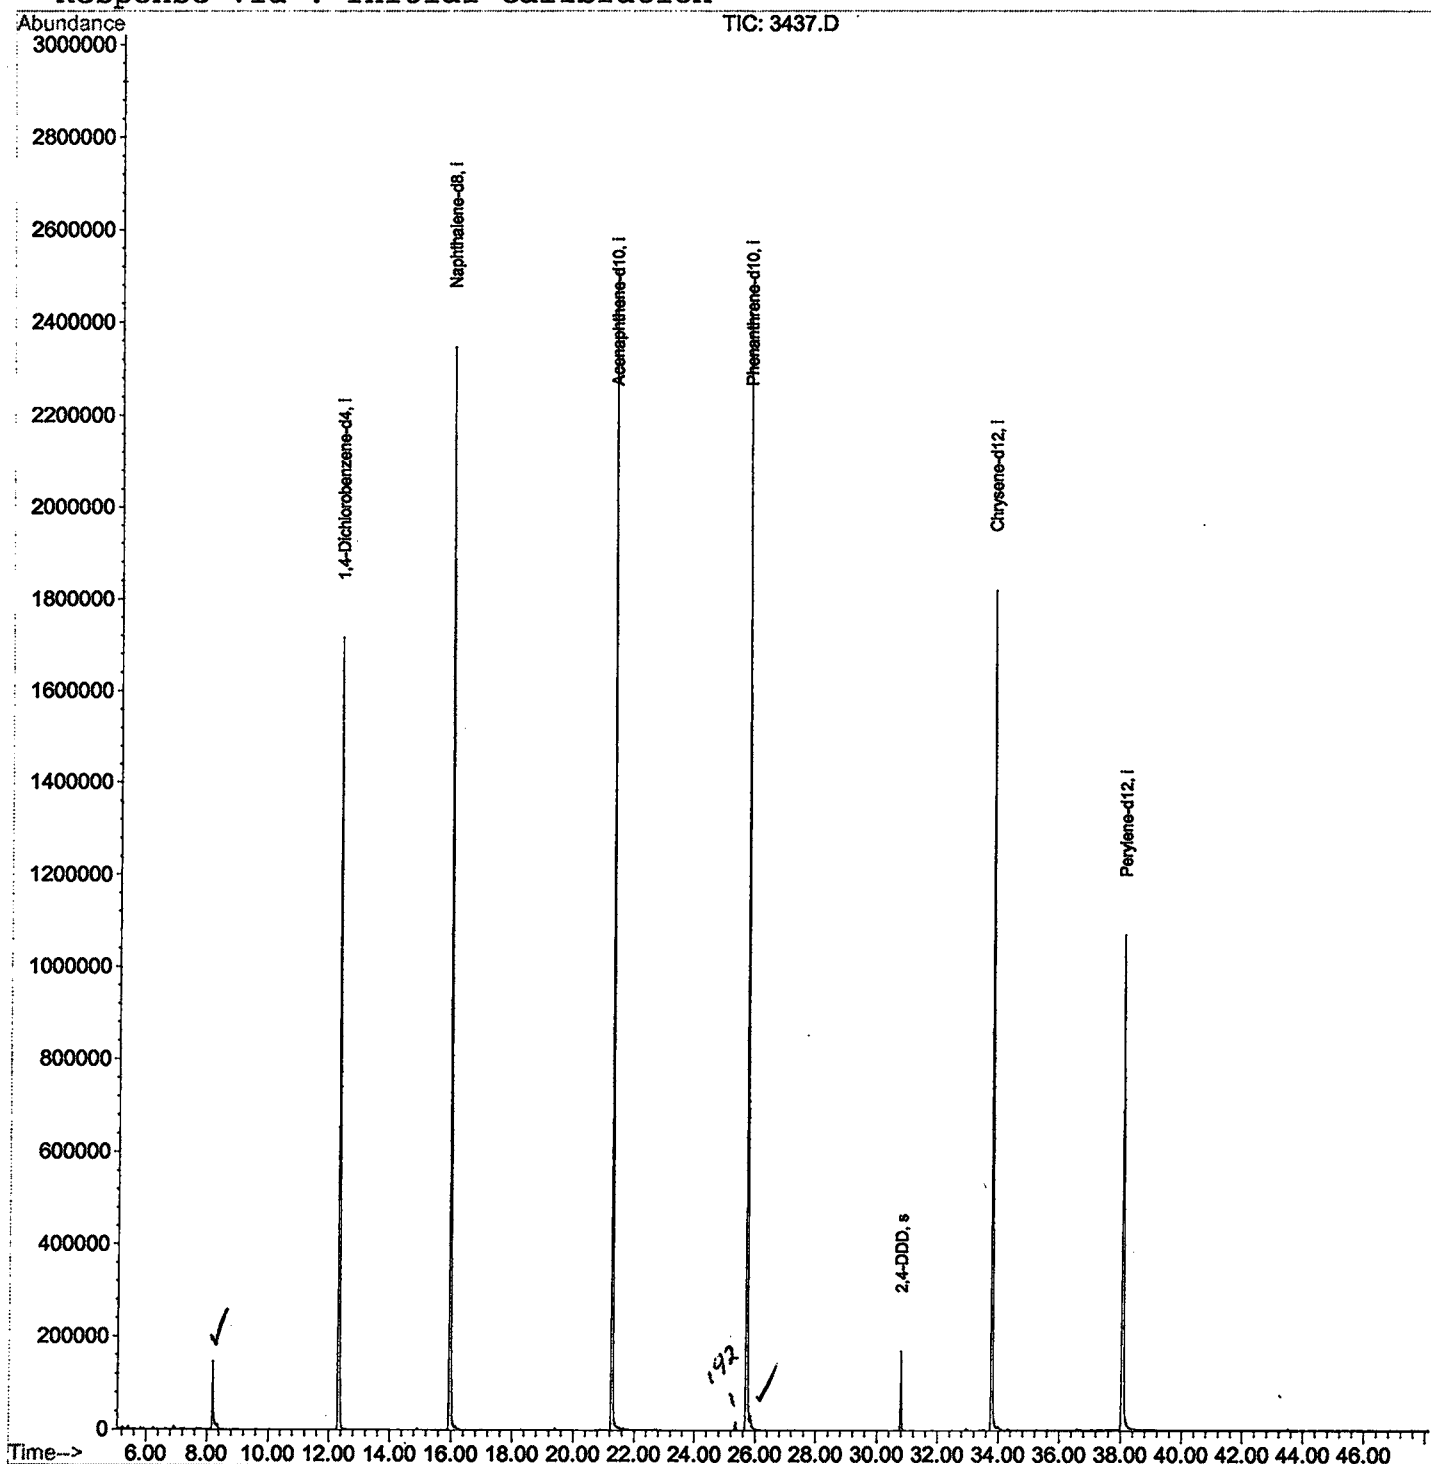

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAR0102\3437.D
 Acq On : 3 Mar 2002 11:35 am
 Sample : gc/ms scan 2/4
 Misc :
 MS Integration Params: LSCINT.P

Vial: 49
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.189	339	343	357	rBV	145984	371679	6.38%	1.240%
2	12.320	787	793	810	rBV	1714730	4081804	70.06%	13.619%
3	15.965	1183	1190	1206	rBV	2347073	5424582	93.10%	18.100%
4	21.280	1761	1769	1790	rBV	2515263	5826556	100.00%	19.441%
5	25.724	2245	2253	2264	rBV2	2418343	5726810	98.29%	19.108%
6	25.852	2264	2267	2279	rVB	28940	84401	1.45%	0.282%
7	30.791	2800	2805	2814	rBV	169358	348411	5.98%	1.163%
8	33.793	3124	3132	3149	rBV2	1819132	4491657	77.09%	14.987%
9	38.071	3586	3598	3624	rBV2	1067255	3614449	62.03%	12.060%

Sum of corrected areas: 29970349

3437.D GCMS0208.M Mon Mar 25 12:24:51 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAR0102\3437.D
 Operator :
 Acquired : 3 Mar 2002 11:35 am using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 2/4
 Misc Info :
 Vial Number: 49
 Quant File :GCMS0208.RES (RTE Integrator)

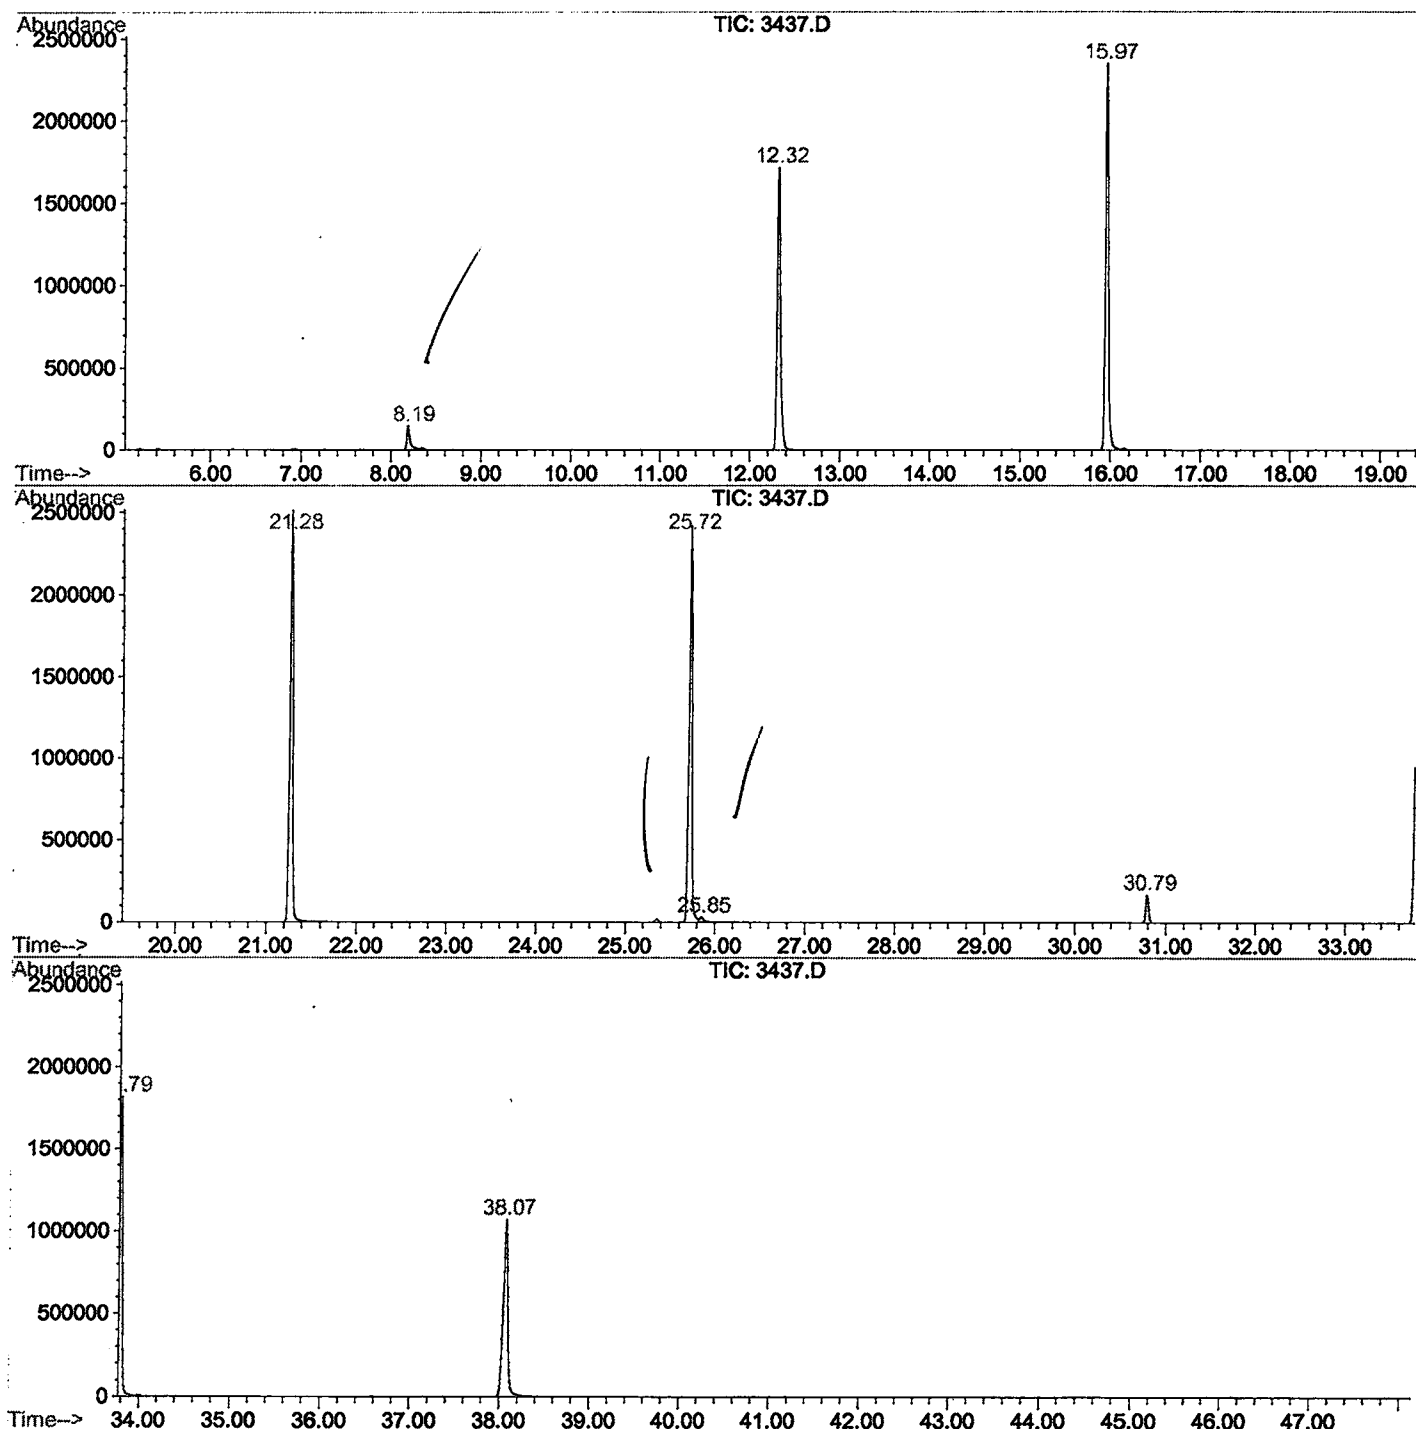

3437.D GCMS0208.M

Mon Mar 25 12:24:56 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR0102\3437.D
 Acq On : 3 Mar 2002 11:35 am
 Sample : gc/ms scan 2/4
 Misc :
 MS Integration Params: LSCINT.P


Vial: 49
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 Silane, tetramethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.19	1.82 ug/l	371679	1,4-Dichlorobenzene-d4	12.32

Hit# of	Tentative ID	MW	MolForm	CAS#	Qual
1	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
2	N-Ethylformamide	73	C3H7NO	000627-45-2	9
3	1,3-Dioxolane, 2-(3-bromo-5,5,5-tri	352	C10H16BrCl3O2	000000-00-0	9
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

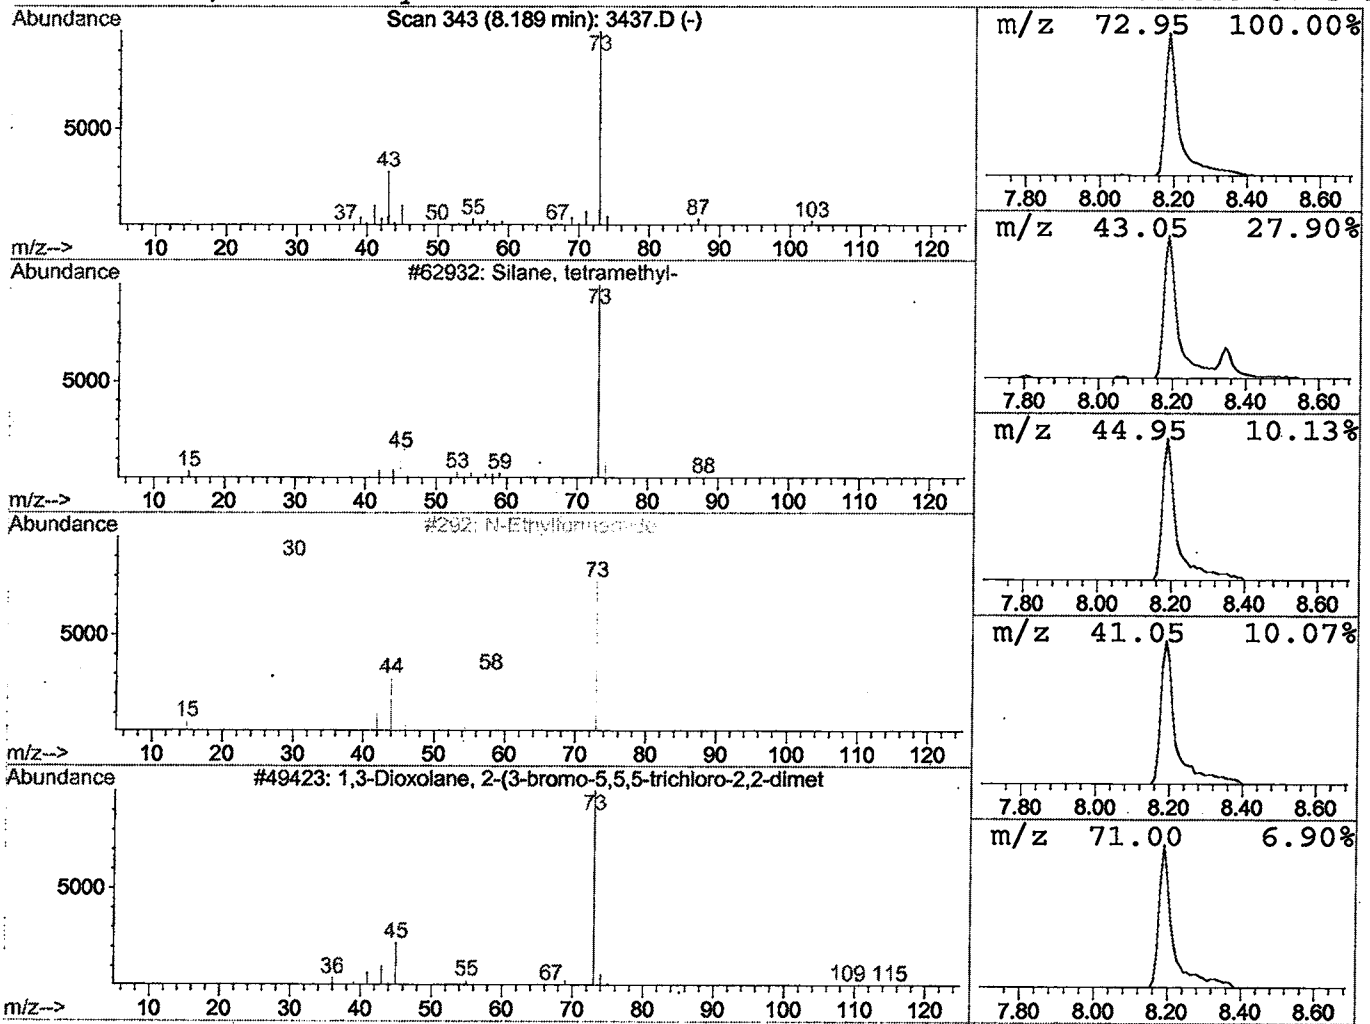

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR0102\3437.D
 Acq On : 3 Mar 2002 11:35 am
 Sample : gc/ms scan 2/4
 Misc :
 MS Integration Params: LSCINT.P


Vial: 49
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Anthracene-d10- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.85	0.29 ug/l	84401	Phenanthrene-d10	25.72

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Anthracene-d10-	188	C14D10	001719-06-8	91
2	Phenanthrene-d10	188	C14D10	001517-22-2	80
3	Naphthalene, 2,6-dimethoxy-	188	C12H12O2	005486-55-5	53
4	5-Oxazolecarboxamide, 2-phenyl-	188	C10H8N2O2	039819-42-6	40

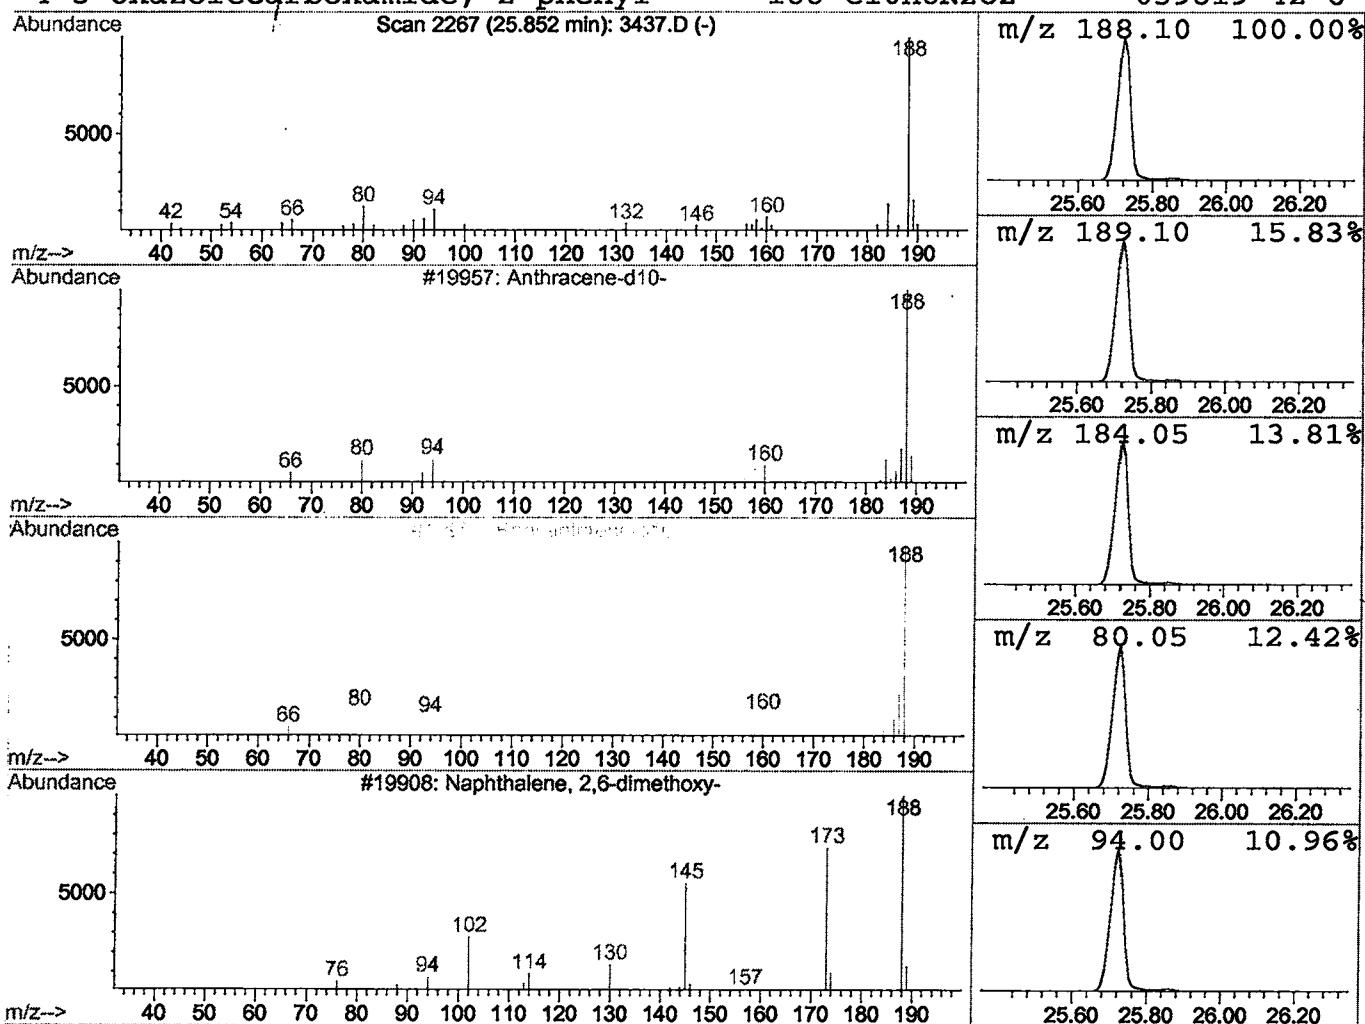

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 3 Mar 2002 11:35 am
 Data File: C:\HPCHEM\1\DATA\MAR0102\3437.D
 Name: gc/ms scan 2/4
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Silane, tetramethyl-	8.19	1.8	ug/l	371679	ISTD01	12.32	4081800	20.0
Anthracene-d10-	25.85	0.3	ug/l	84401	ISTD04	25.72	5726810	20.0

3437.D GCMS0208.M Mon Mar 25 12:25:09 2002