

Method 508 MOD.Date Extracted 2-28-02Page 115

Ref

#GCM5-17679

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
L.B.		500 mL		1 mL			1 mL	4B	7			
Ref 1					1 mL			8B				
Ref 2					1 mL			8A				
4385								4A				
4386								1B				
4387								7A				
4388	F.B.							7B				
4410								3B				
4411								1A				
4412								3A				
4413								2B				
4414								2A				
4415								6A				
Remarks												
Reviewed by, <i>[Signature]</i> 8/13/02												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type - SEP. F.W.		Solv. lot# V13 E18		NaCl lot# V39618		Na2SO4 lot# V46623						
STANDARD	INT STD LOG#											
CALIBRATION	15803010V											
REF SPIKE	2193											
MDL/MDRF												
Q. CHECK												
INT. STD.	62332 1503150V											
SURROGATE	21602											
LPC												
ENDRIN/DDT												

Analyst AD
revision 4/12/01Verified by *[Signature]*Reviewed by *[Signature]*
Date 4/13/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAR2502.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\mar2502\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0308	
2	Sample	7	REF1	GCMS0308	re-inject
3	Sample	8	REF2	GCMS0308	re-inject
4	Sample	2	CAL5A	GCMS0308	gc/ms scan
5	Sample	3	CAL5B	GCMS0308	gc/ms scan
6	Sample	4	CAL5C	GCMS0308	gc/ms scan
7	Sample	5	CAL5D	GCMS0308	gc/ms scan
8	Sample	6	CAL5E	GCMS0308	gc/ms scan
9	Sample	9	LB	GCMS0308	gc/ms scan 2/28
10	Sample	10	REF	GCMS0308	gc/ms scan 2/28
11	Sample	11	REF2A	GCMS0308	gc/ms scan 2/28
12	Sample	12	4385	GCMS0308	gc/ms scan 2/28
13	Sample	13	4386	GCMS0308	gc/ms scan 2/28
14	Sample	14	4387	GCMS0308	gc/ms scan 2/28
15	Sample	15	4388	GCMS0308	gc/ms scan 2/28 fb
16	Sample	16	4410	GCMS0308	gc/ms scan 2/28
17	Sample	17	4411	GCMS0308	gc/ms scan 2/28
18	Sample	18	4412	GCMS0308	gc/ms scan 2/28
19	Sample	19	4413	GCMS0308	gc/ms scan 2/28
20	Sample	20	4414	GCMS0308	gc/ms scan 2/28
21	Sample	21	4415	GCMS0308	gc/ms scan 2/28

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR2502\DFTPP.D

Vial: 1

Acq On : 25 Mar 2002 10:10 am

Operator:

Sample :

Inst : GC/MS 209


Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

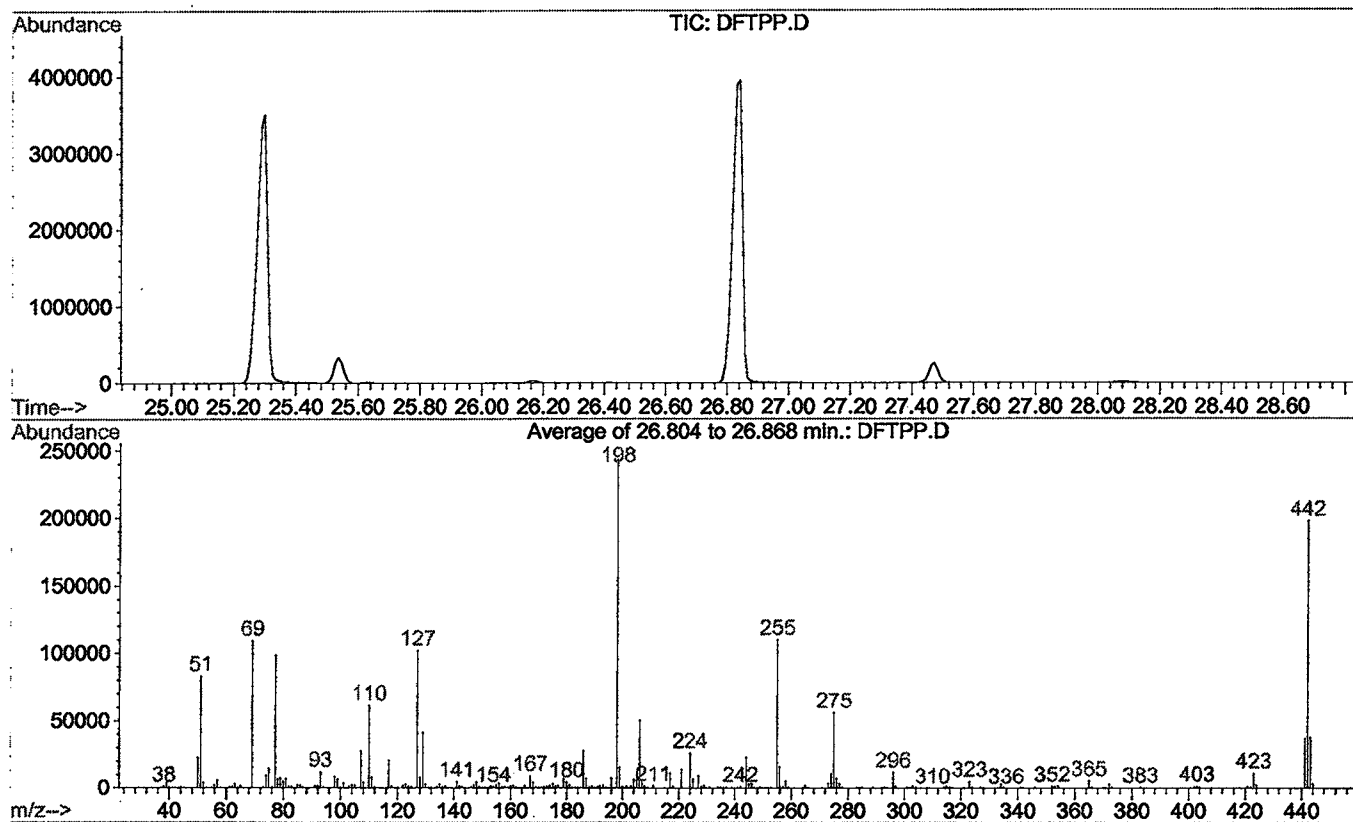

Spectrum Information: Average of 26.804 to 26.868 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.3	83355	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.1	109653	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.1	102366	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	242910	PASS
199	198	5	9	6.6	15945	PASS
275	198	10	30	23.1	56173	PASS
365	198	1	100	2.4	5745	PASS
441	443	0.01	100	98.6	37421	PASS
442	198	40	110	81.5	197935	PASS
443	442	17	23	19.2	37947	PASS

DFTPP.D GCMS0308.M

Thu Mar 28 10:25:16 2002