

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\5973N\02FEB27\02384.D
Acq On : 27 Feb 2002 2:03 pm
Sample : 508 scan
Misc : February 27, 2002
MS Integration Params: SPLIT.P
Quant Time: Feb 28 08:37:46 2002

Vial: 5
Operator:
Inst : Instrumen
Multiplr: 1.00

Quant Results File: HP022102.RES

Quant Method : C:\MSDCHEM\1...\HP022102.M (RTE Integrator)
Title : 508 scan method
Last Update : Mon Feb 25 10:47:59 2002
Response via : Initial Calibration
DataAcq Meth : HP020702

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.72	152	1842712	20.00	ug/L	0.00
10) Naphthalene-d8	13.20	136	8123161	20.00	ug/L	0.00
17) Acenaphthene-d10	18.34	164	4068697	20.00	ug/L	0.00
29) Phenanthrene-d10	22.64	188	6875994	20.00	ug/L	0.00
38) Chrysene-d12	30.50	240	5304932	20.00	ug/L	-0.02
44) Perylene-d12	34.42	264	3750202	20.00	ug/L	-0.03

System Monitoring Compounds

37) 2,4-DDD	27.72	235	239465	2.61	ug/L	0.00
Spiked Amount	5.000		Recovery	=	52.20%	

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration
02384.D HP031802.M Fri Mar 22 14:17:44 2002

Page 1

Quantitation Report


(QT Reviewed)

Data File : C:\MSDCHEM\1\5973N\02FEB27\02384.D
Acq On : 27 Feb 2002 2:03 pm
Sample : 508 scan
Misc : February 27, 2002
MS Integration Params: SPLIT.P
Quant Time: Mar 22 14:17 2002

Vial: 5
Operator:
Inst : Instrumen
Multiplr: 1.00

Quant Results File: HP022102.R

Method : C:\MSDCHEM\1\METHODS\METHODS\HP031802.M (RTE Integrator)
Title : VOC method 8260
Last Update : Wed Mar 20 10:59:46 2002
Response via : Initial Calibration

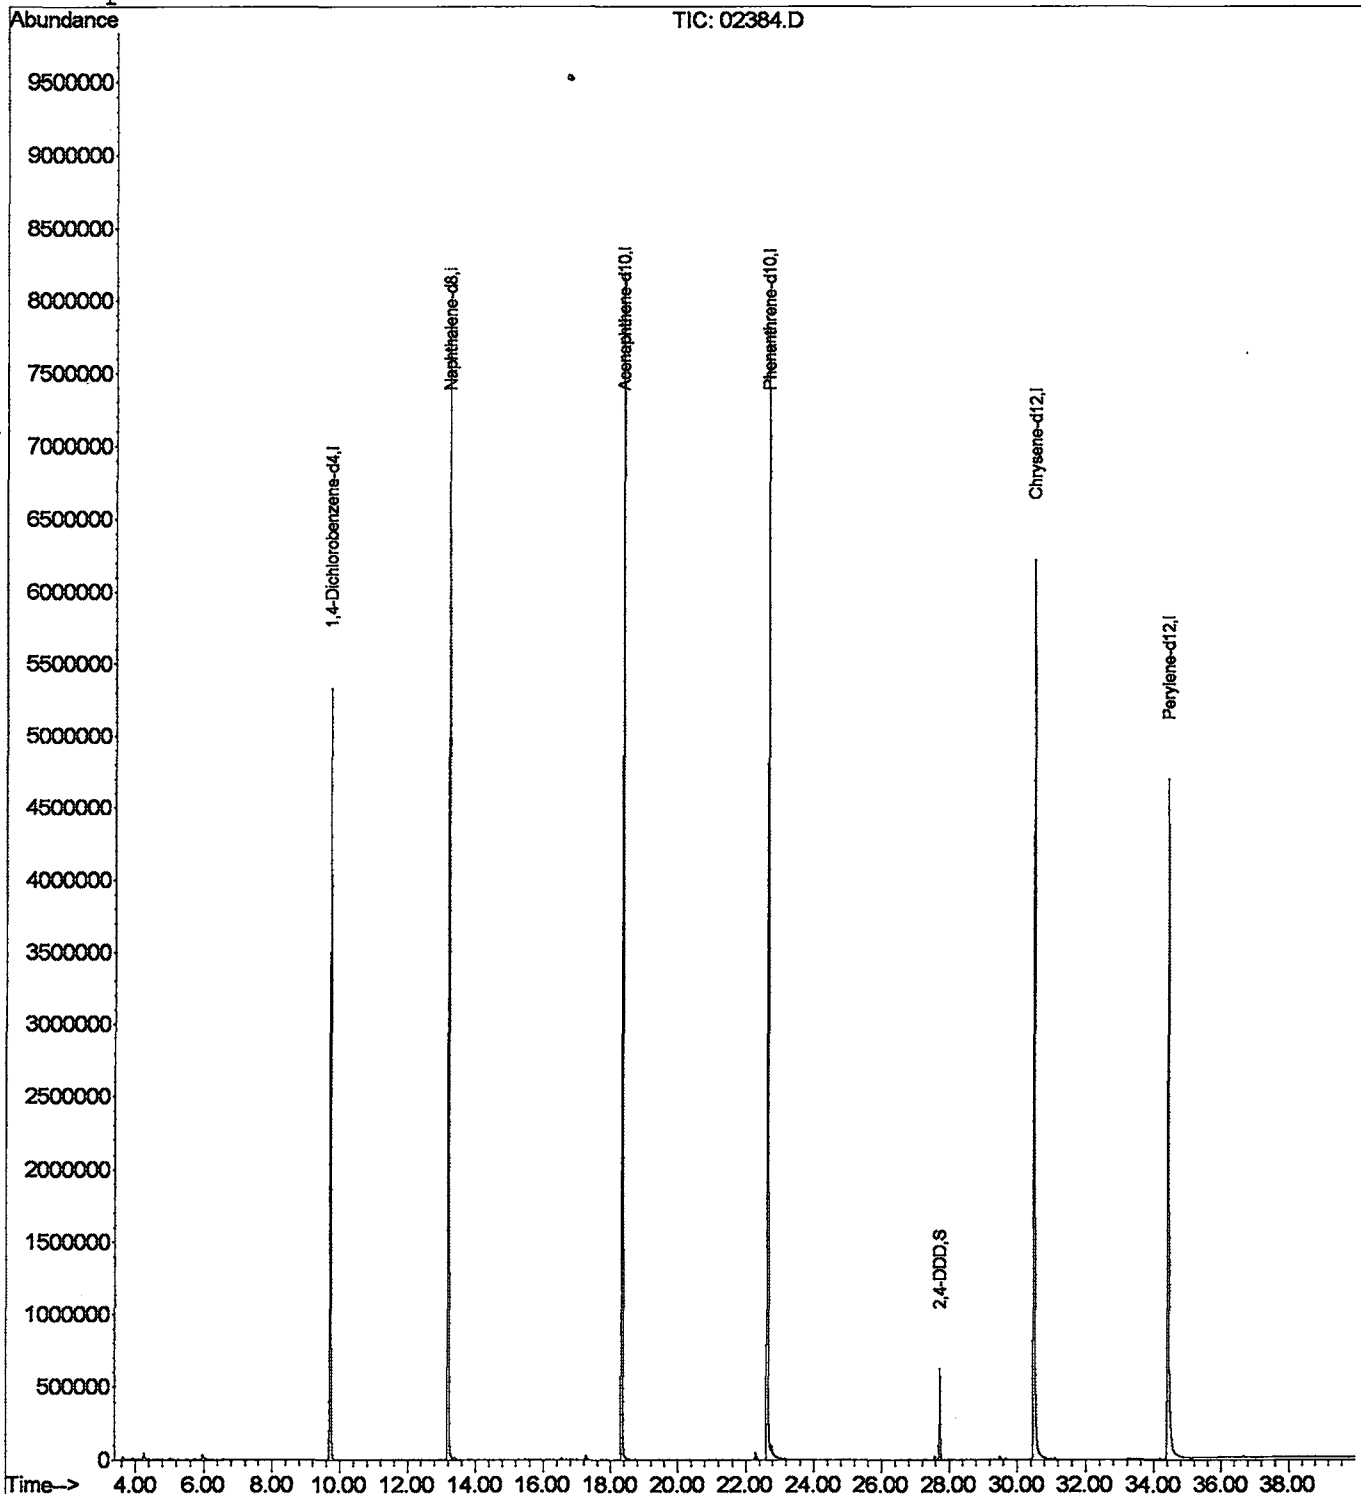

LSC Area Percent Report

.. Data File : C:\MSDCHEM\1\5973N\02FEB27\02384.D
Acq On : 27 Feb 2002 2:03 pm
Sample : 508 scan
Misc : February 27, 2002
MS Integration Params: LSCINT.P

Vial: 5
Operator:
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\METHODS\METHODS\HP031802.M (RTE Integrator)
Title : VOC method 8260
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.718	558	562	574	rBV	5332404	10386851	59.52%	11.569%
2	13.195	866	870	884	rBV	7876223	15413705	88.33%	17.168%
3	18.343	1321	1326	1330	rBV	8191253	16553034	94.86%	18.437%
4	22.644	1702	1707	1716	rBV2	7809970	17449847	100.00%	19.436%
5	22.768	1716	1718	1741	rVB	93260	379900	2.18%	0.423%
6	27.724	2153	2157	2164	rVB	622548	1152290	6.60%	1.283%
7	30.501	2397	2403	2425	rBV	6218202	15671944	89.81%	17.456%
8	34.418	2744	2750	2781	rBV	4690194	12774377	73.21%	14.228%

Sum of corrected areas: 89781948

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\5973N\02FEB27\02384.D
 Operator :
 Acquired : 27 Feb 2002 2:03 pm using AcqMethod HP020702
 Instrument : Instrumen
 Sample Name: 508 scan
 Misc Info : February 27, 2002
 Vial Number: 5
 Quant File :HP022102.RES (RTE Integrator)

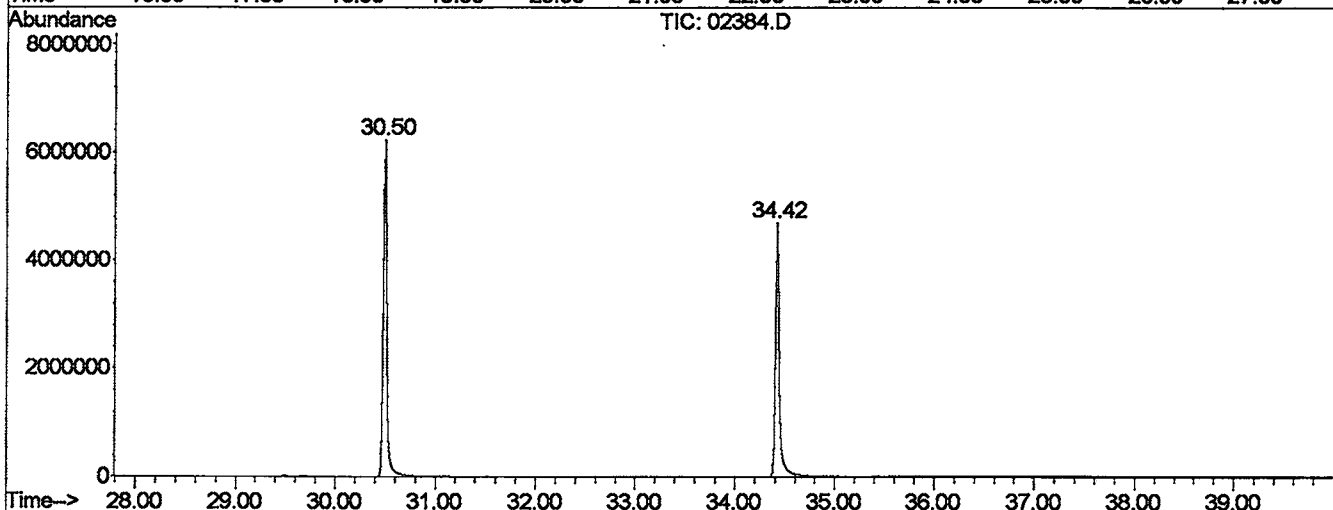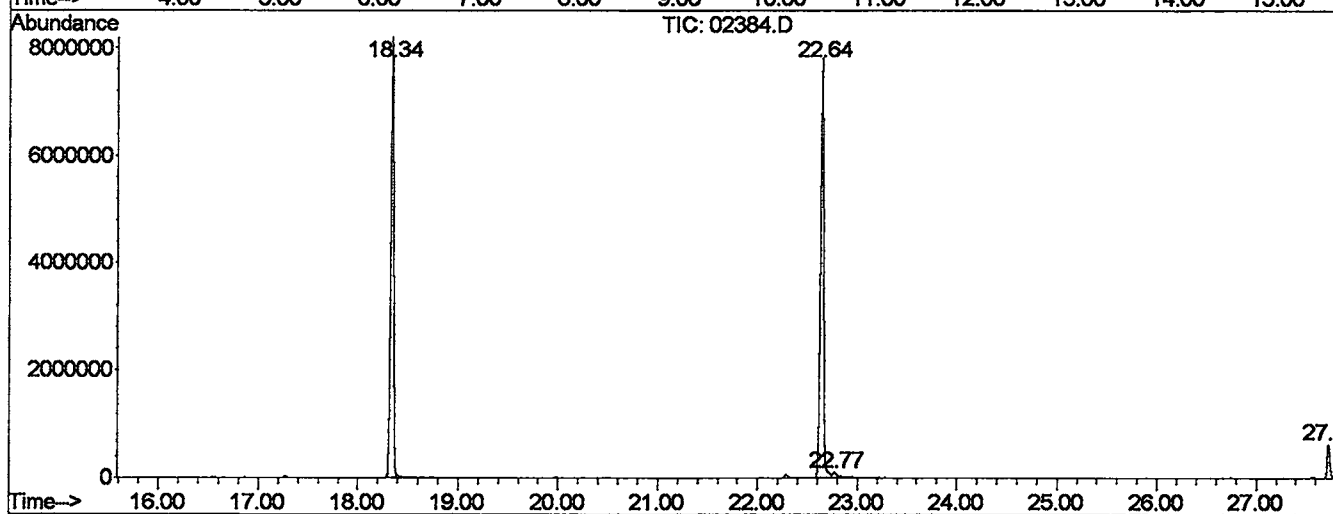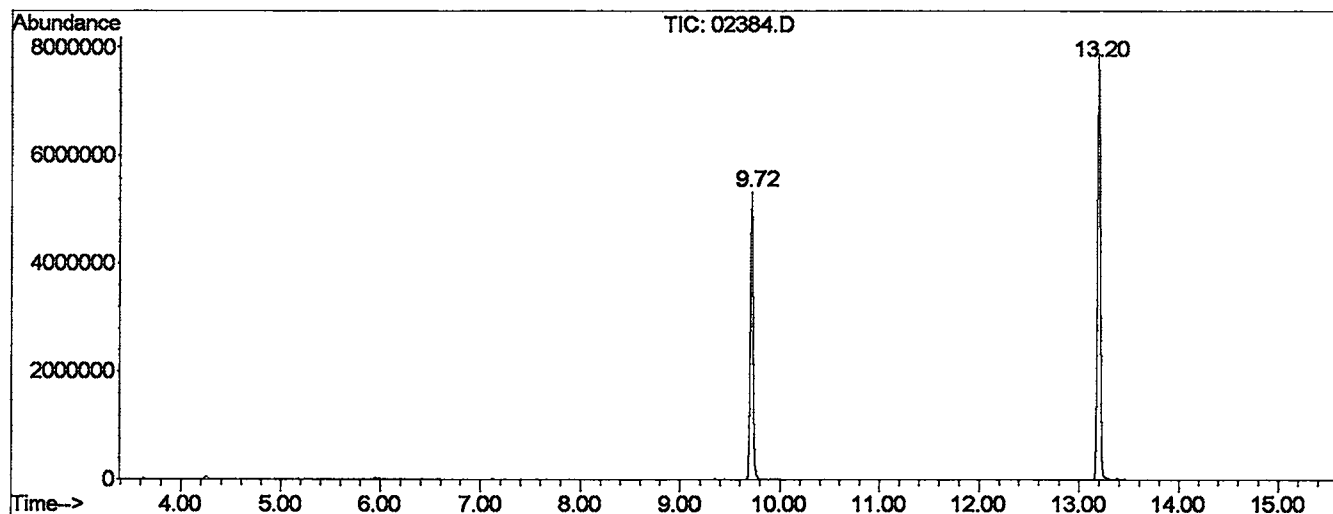

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 27 Feb 2002 2:03 pm
 Data File: C:\MSDCHEM\1\5973N\02FEB27\02384.D
 Name: 508 scan
 Misc: February 27, 2002
 Method: C:\MSDCHEM\1\METHODS\METHODS\HP022102.M (RTE Integrator)
 Title: VOC method 8260
 Library Searched: demo.1

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
