

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\5973N\02FEB26\02087.D
Acq On : 26 Feb 2002 5:16 pm
Sample : 508 scan
Misc : February 26, 2002
MS Integration Params: SPLIT.P
Quant Time: Feb 27 08:30:40 2002

Vial: 4
Operator:
Inst : Instrumen
Multiplr: 1.00

Quant Results File: HP022102.RES

Quant Method : C:\MSDCHEM\1...\HP022102.M (RTE Integrator)
Title : 508 scan method
Last Update : Mon Feb 25 10:47:59 2002
Response via : Initial Calibration
DataAcq Meth : HP020702

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.72	152	1714513	20.00	ug/L	0.00
10) Naphthalene-d8	13.19	136	7336298	20.00	ug/L	0.00
17) Acenaphthene-d10	18.34	164	3690268	20.00	ug/L	0.00
29) Phenanthrene-d10	22.63	188	6461932	20.00	ug/L	-0.01
38) Chrysene-d12	30.49	240	4677199	20.00	ug/L	-0.03
44) Perylene-d12	34.41	264	3051939	20.00	ug/L	-0.04

System Monitoring Compounds

37) 2,4-DDD	27.72	235	273176	3.17	ug/L	0.00
Spiked Amount	5.000		Recovery	=	63.40%	

Target Compounds

Qvalue


(#) = qualifier out of range (m) = manual integration
02087.D HP031802.M Fri Mar 22 14:18:57 2002

Data File : C:\MSDCHEM\1\5973N\02FEB26\02087.D
 Acq On : 26 Feb 2002 5:16 pm
 Sample : 508 scan
 Misc : February 26, 2002
 MS Integration Params: SPLIT.P
 Quant Time: Feb 27 8:30 2002

Vial: 4
 Operator:
 Inst : Instrumen
 Multiplr: 1.00

Quant Results File: HP022102.R

Method : C:\MSDCHEM\1\METHODS\METHODS\HP031802.M (RTE Integrator)
 Title : VOC method 8260
 Last Update : Wed Mar 20 10:59:46 2002
 Response via : Initial Calibration

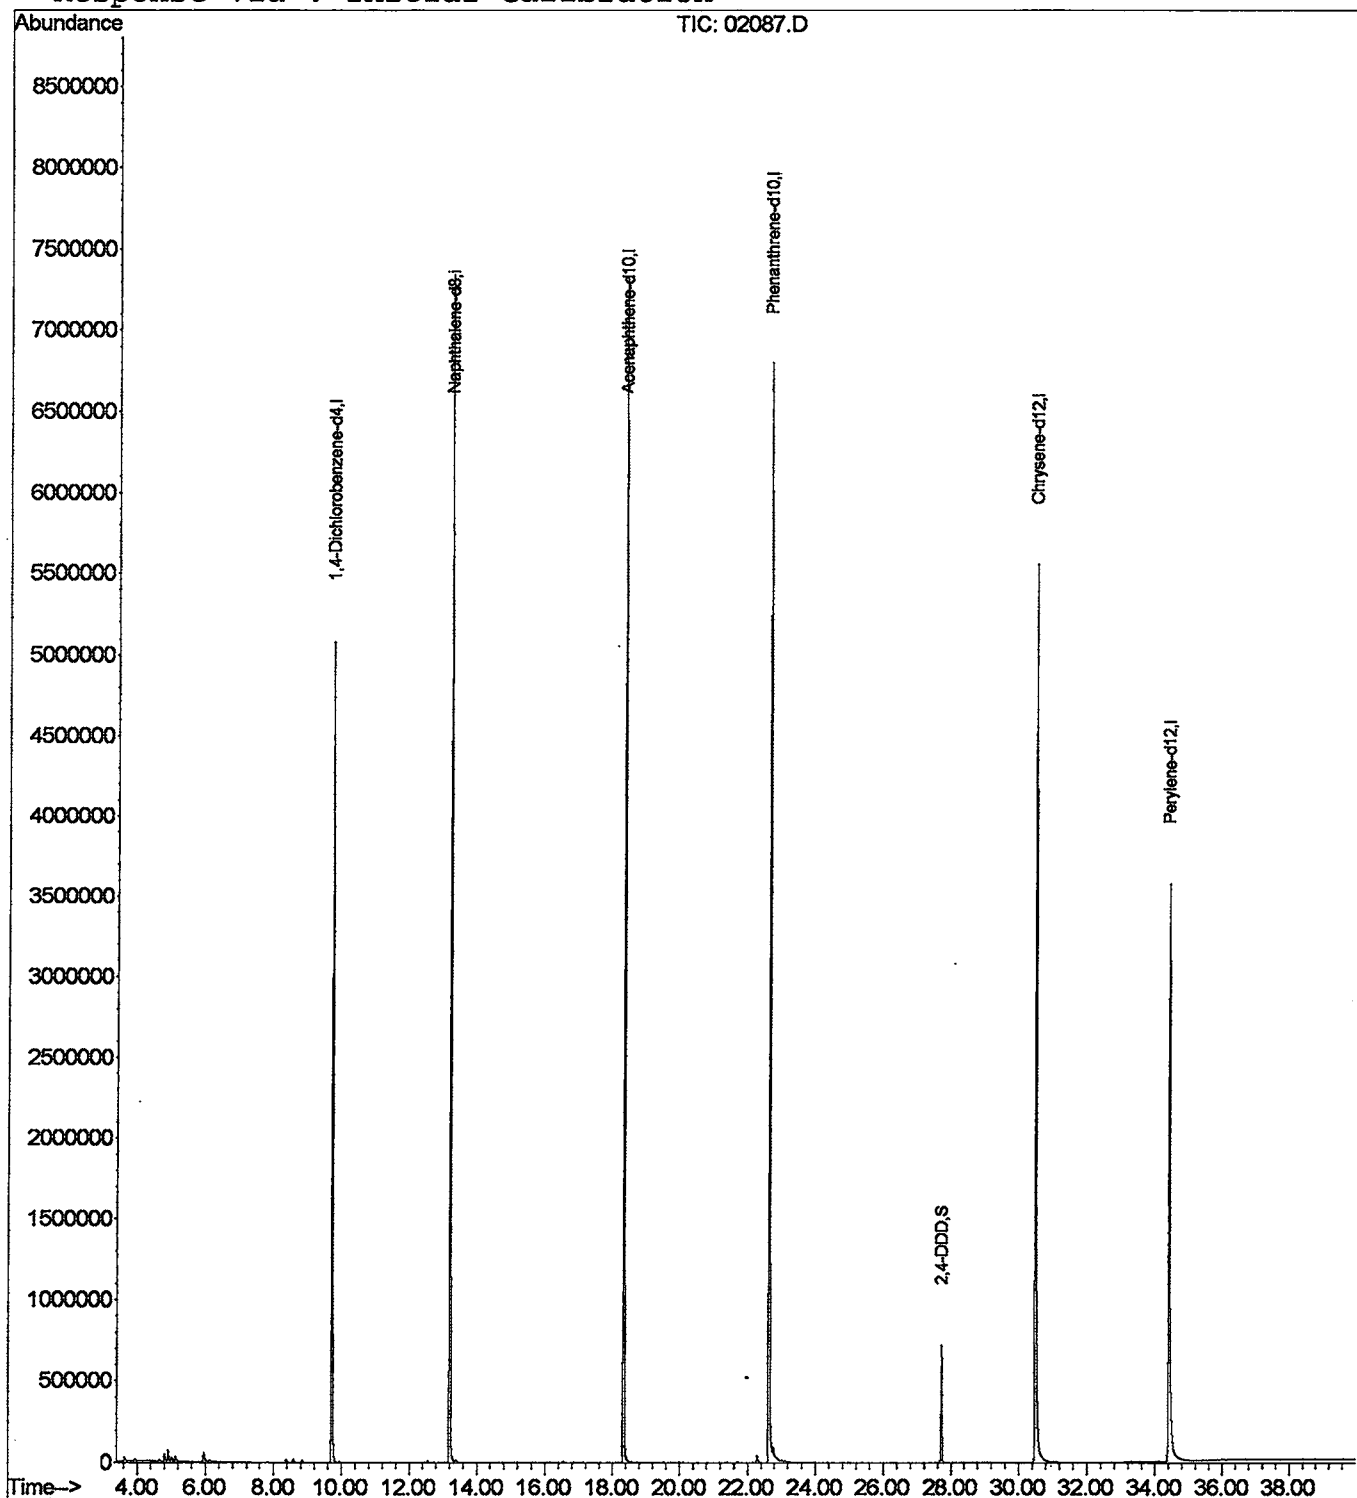

LSC Area Percent Report

Data File : C:\MSDCHEM\1\5973N\02FEB26\02087.D
 Acq On : 26 Feb 2002 5:16 pm
 Sample : 508 scan
 Misc : February 26, 2002
 MS Integration Params: LSCINT.P

Vial: 4
 Operator:
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\METHODS\METHODS\HP031802.M (RTE Integrator)
 Title : VOC method 8260
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.947	226	228	241	rBV	57707	163027	1.00%	0.201%
2	9.718	558	562	575	rVB	5081022	9582031	58.93%	11.828%
3	13.195	866	870	883	rVB	7333777	13833577	85.08%	17.076%
4	18.343	1321	1326	1340	rBV	7322131	15187164	93.41%	18.746%
5	22.644	1701	1707	1716	rBV2	6803161	16258794	100.00%	20.069%
6	22.768	1716	1718	1732	rVB2	82642	318140	1.96%	0.393%
7	27.724	2153	2157	2164	rBV	722211	1326329	8.16%	1.637%
8	30.490	2397	2402	2429	rBV2	5553142	13866343	85.29%	17.116%
9	34.407	2743	2749	2780	rBV	3569868	10478665	64.45%	12.934%

Sum of corrected areas: 81014070

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\5973N\02FEB26\02087.D
 Operator :
 Acquired : 26 Feb 2002 5:16 pm using AcqMethod HP020702
 Instrument : Instrumen
 Sample Name: 508 scan
 Misc Info : February 26, 2002
 Vial Number: 4
 Quant File :HP022102.RES (RTE Integrator)

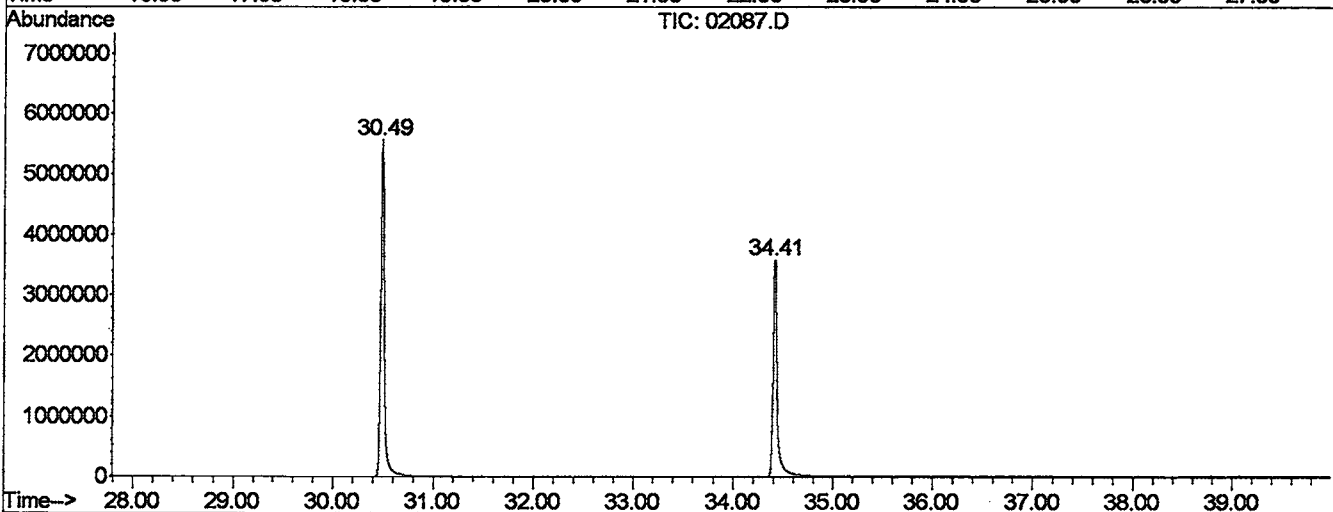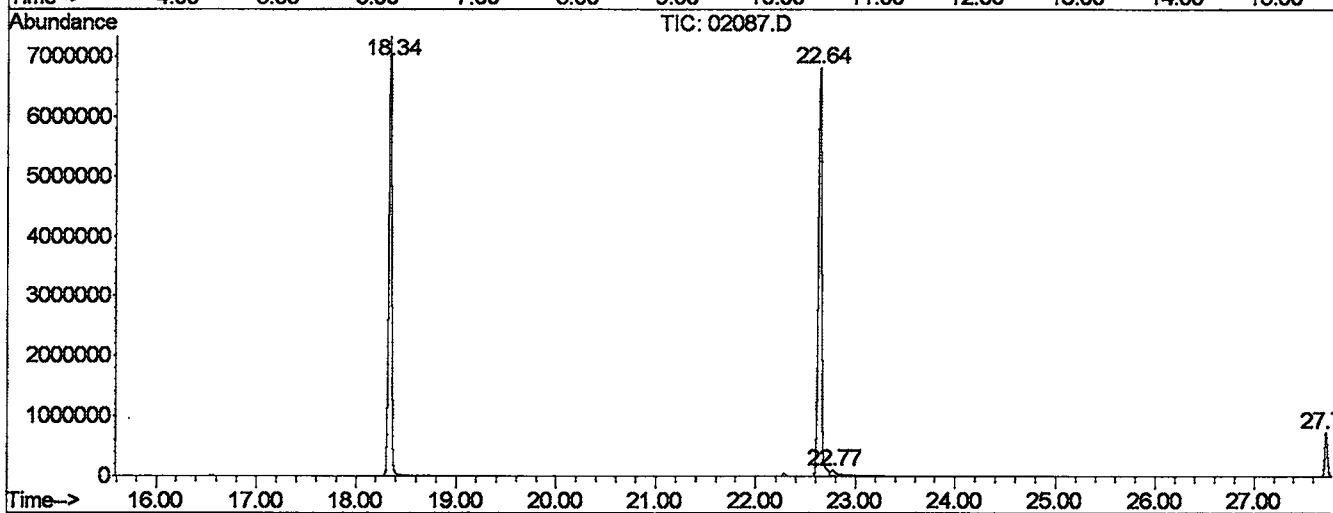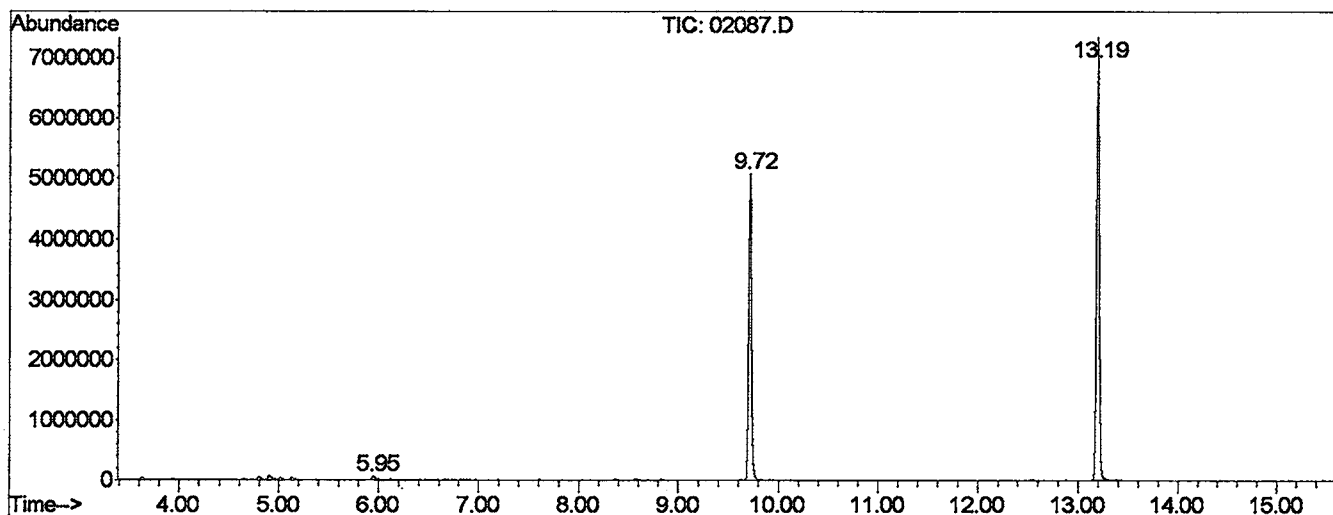

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 26 Feb 2002 5:16 pm
Data File: C:\MSDCHEM\1\5973N\02FEB26\02087.D
Name: 508 scan
Misc: February 26, 2002
Method: C:\MSDCHEM\1\METHODS\METHODS\HP022102.M (RTE Integrator)
Title: VOC method 8260
Library Searched: demo.1

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
