

Method GCMS ScanDate Extracted 3/1/02Page 122~~GCMS-17579~~ GCMS-17579

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
	LB	500mL		1mL			1mL	4B	7	
	Ref 1				1mL			4A		
	Ref 2				1mL			1B		
	939							1A		
	1153							2B		
	4417							2A		
	4418							10B 9A		
	4419							10A 10B		
	4420							10A 7B		
	4449							7B 7A		
	4450							7A 8A		
	4451							8A		
	4508							8B		
Remarks										
Reviewed by <u>C/S</u> 8/13/02										
drip rate must be between 5-15 ml/min for liq-liq extractors										
drip rate -										
Extraction type - <u>Seppia</u> Solv. lot# <u>V39466</u> NaCl lot# <u>V39618</u> Na2SO4 lot# <u>V46623</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	2193									
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	21602									
LPC										
ENDRIN/DDT										

Analyst ML
revision 4/12/01

Verified by _____

Reviewed by DN
Date _____

```

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAR2102.S
Comment:
Operator:
Data Path: C:\HPCHEM\1\DATA\mar2102\
Pre-Seq Cmd:
Post-Seq Cmd:

```

```

Method Sections To Run      On A Barcode Mismatch
(X) Full Method              (X) Inject Anyway
( ) Reprocessing Only        ( ) Don't Inject

```

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0308	
2	Sample	2	CAL40	GCMS0308	
3	Sample	3	LB	GCMS0308	gc/ms scan 3/1
4	Sample	4	REF1	GCMS0308	gc/ms scan 3/1
5	Sample	5	REF2	GCMS0308	gc/ms scan 3/1
6	Sample	6	939	GCMS0308	re-extract
7	Sample	7	1153	GCMS0308	re-extract
8	Sample	8	4417	GCMS0308	gc/ms scan 3/1
9	Sample	9	4418	GCMS0308	gc/ms scan 3/1
10	Sample	10	4419	GCMS0308	gc/ms scan 3/1
11	Sample	11	4420	GCMS0308	gc/ms scan 3/1
12	Sample	12	4449	GCMS0308	gc/ms scan 3/1
13	Sample	13	4450	GCMS0308	gc/ms scan 3/1
14	Sample	14	4451	GCMS0308	gc/ms scan 3/1
15	Sample	15	4508	GCMS0308	gc/ms scan 3/1
16	Sample	16	LBA	GCMS0308	gc/ms scan 3/13
17	Sample	17	REFA1	GCMS0308	gc/ms scan 3/13
18	Sample	18	REFA2	GCMS0308	gc/ms scan 3/13
19	Sample	19	1156	GCMS0308	re-extract
20	Sample	20	1331	GCMS0308	re-extract
21	Sample	21	3735	GCMS0308	re-extract
22	Sample	22	3507	GCMS0308	re-extract
23	Sample	1	DFTPP2	GCMS0308	
24	Sample	2	CAL40A	GCMS0308	
25	Sample	23	5895	GCMS0308	gc/ms scan 3/13
26	Sample	24	5896	GCMS0308	gc/ms scan 3/13
27	Sample	25	5897	GCMS0308	gc/ms scan 3/13
28	Sample	26	5898	GCMS0308	gc/ms scan 3/13 fb
29	Sample	27	5899	GCMS0308	gc/ms scan 3/13

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR2102\DFTPP.D

Acq On : 21 Mar 2002 11:16 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

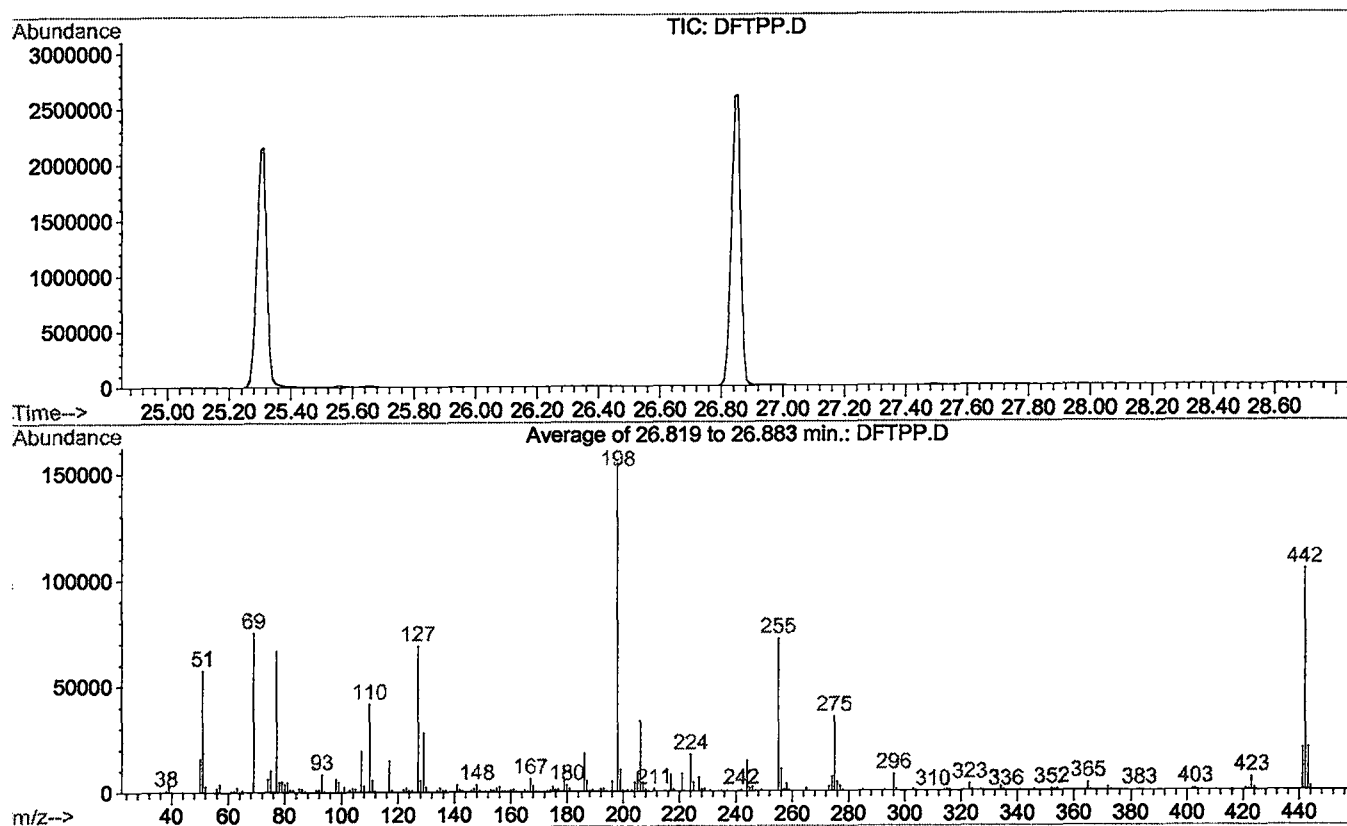

Spectrum Information: Average of 26.819 to 26.883 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	37.3	57552	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.7	75138	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	44.6	68857	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	154276	PASS
199	198	5	9	6.7	10398	PASS
275	198	10	30	22.8	35125	PASS
365	198	1	100	2.4	3705	PASS
441	443	0.01	100	98.3	19796	PASS
442	198	40	110	67.4	104054	PASS
443	442	17	23	19.4	20140	PASS

DFTPP.D GCMS0308.M

Fri Mar 22 08:34:14 2002