

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/04/2002 Time: 09:05:46

Sample: AE04449
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/4/02 09:05 Ended: 4/4/02 09:05 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		108		5.0

Comments for Sample AE04449 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-04-2002 Time: 09:05:49

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR2102\4449.D

Vial: 12

Acq On : 21 Mar 2002 10:08 pm

Operator:

Sample : gc/ms scan 3/1

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 22 9:27 2002

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Mar 08 08:54:27 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0308

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.26	152	583782	20.00	ug/l	-0.09
10) Naphthalene-d8	15.91	136	2265913	20.00	ug/l	-0.09
17) Acenaphthene-d10	21.21	164	1212750	20.00	ug/l	-0.10
29) Phenanthrene-d10	25.66	188	1821479	20.00	ug/l	-0.10
38) Chrysene-d12	33.72	240	1120628	20.00	ug/l	-0.12
44) Perylene-d12	37.97	264	663888	20.00	ug/l	-0.15

System Monitoring Compounds

37) 2,4-DDD	30.73	235	71746	5.42	ug/mL	0.23
Spiked Amount	5.000		Recovery	= 108.40%		

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.96	128	261	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.69	149	496	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)= qualifier out of range (m)= manual integration

4449.D GCMS0308.M Fri Mar 22 09:48:22 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR2102\4449.D
 Acq On : 21 Mar 2002 10:08 pm
 Sample : gc/ms scan 3/1
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Mar 22 9:27 2002

Vial: 12
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Mar 08 08:54:27 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0308

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.65	178	487	N.D.		
34) Anthracene	25.65	178	487	N.D.		
35) Di-n-butylphthalate	27.63	149	2346	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.72	228	2534	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.93	149	3723	N.D.		
43) Chrysene	33.72	228	2534	N.D.		
45) Di-n-Octylphthalate	35.67	149	192	N.D.		
46) Benzo(b)fluoranthene	36.78	252	316	N.D.		
47) Benzo(k)fluoranthene	36.78	252	316	N.D.		
48) Benzo(a)pyrene	37.97	252	2698	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

4449.D GCMS0308.M Fri Mar 22 09:48:26 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAR2102\4449.D
Acq On : 21 Mar 2002 10:08 pm
Sample : gc/ms scan 3/1
Misc :
MS Integration Params: GOOFY.P
Quant Time: Mar 22 9:27 2002

Vial: 12
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0308.RES

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Mar 08 08:54:27 2002
Response via : Initial Calibration

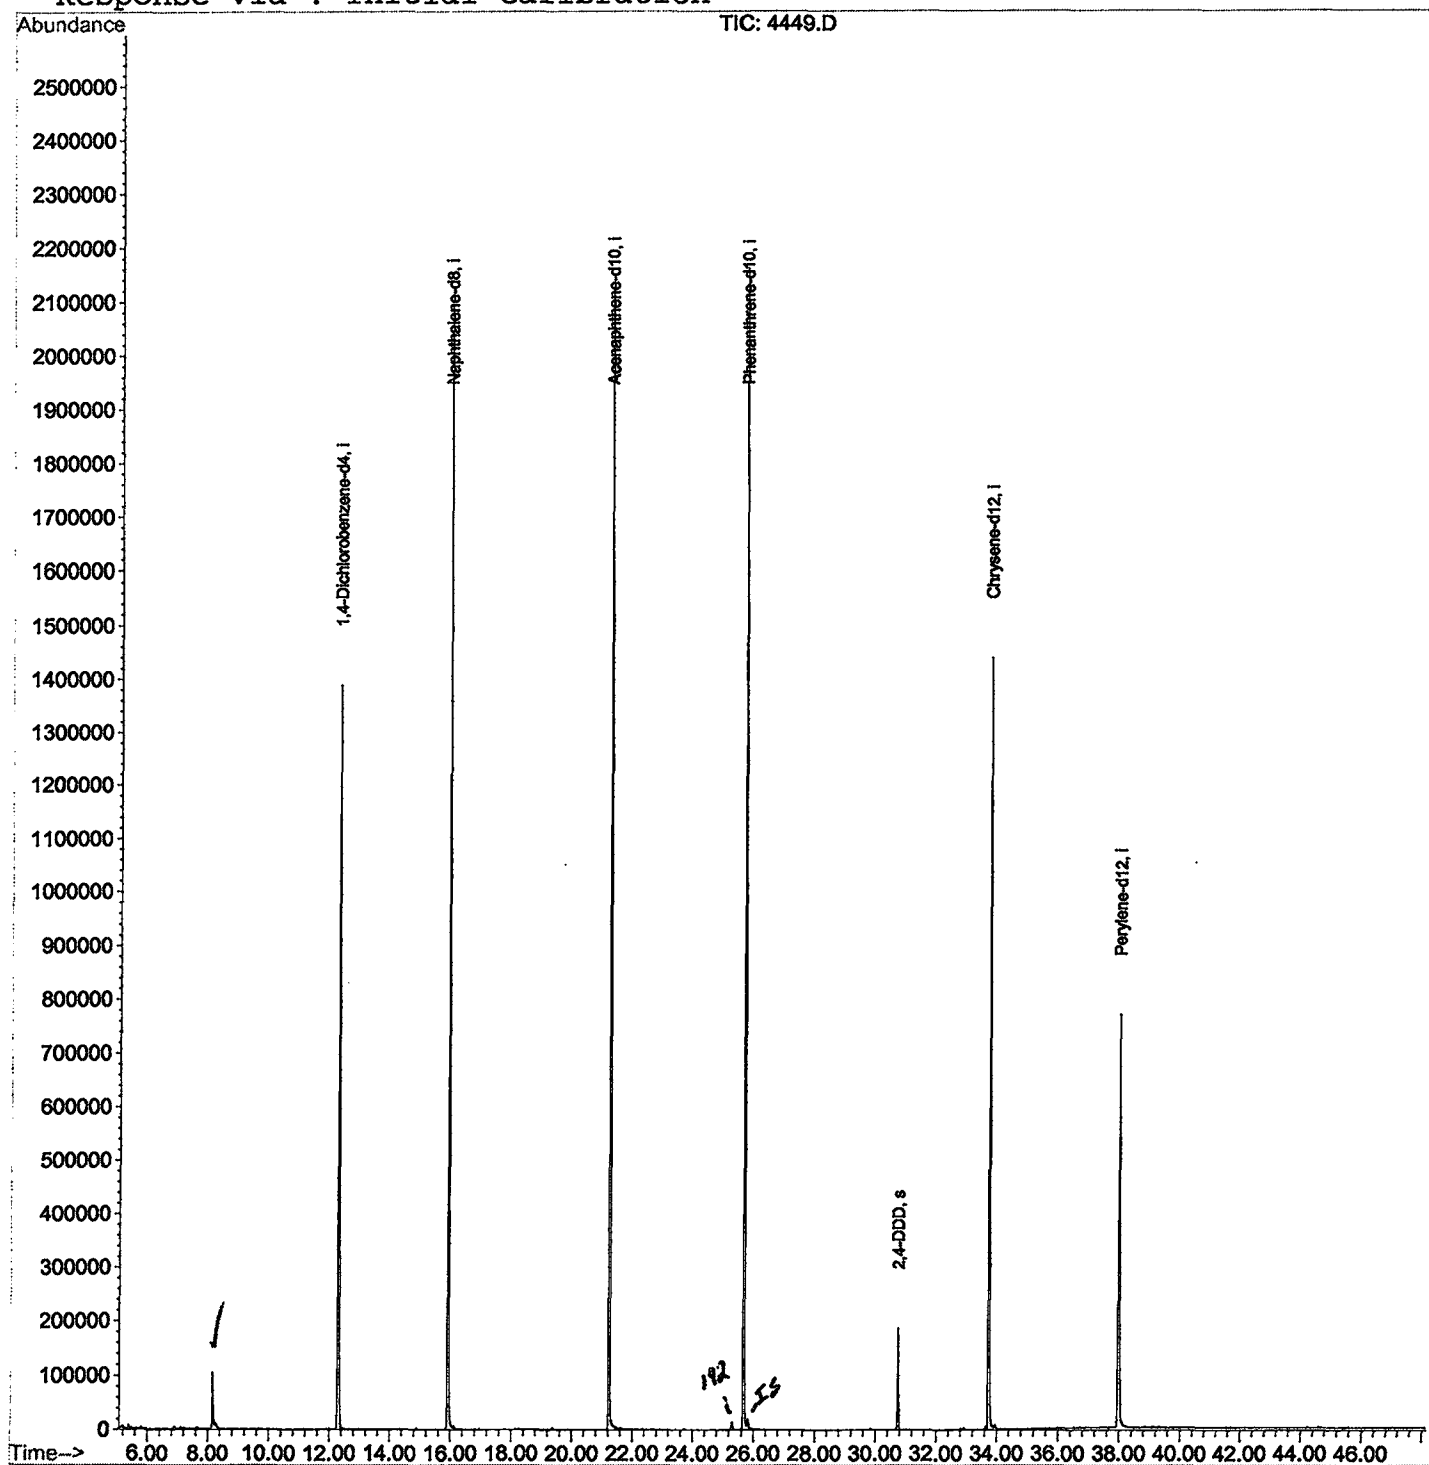

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAR2102\4449.D
 Acq On : 21 Mar 2002 10:08 pm
 Sample : gc/ms scan 3/1
 Misc :
 MS Integration Params: LSCINT.P

Vial: 12
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.139	333	337	346	rBV	104578	239324	5.14%	1.045%
2	12.261	781	786	802	rBV	1387482	3201252	68.80%	13.972%
3	15.905	1177	1183	1200	rBV	2092386	4285800	92.11%	18.705%
4	21.211	1755	1761	1780	rBV	2126862	4652683	100.00%	20.307%
5	25.664	2239	2246	2257	rBV	2161794	4561783	98.05%	19.910%
6	30.731	2793	2798	2806	rBV	186909	359763	7.73%	1.570%
7	33.724	3117	3124	3142	rBV2	1437989	3309107	71.12%	14.443%
8	37.975	3578	3587	3606	rBV2	767137	2302366	49.48%	10.049%

Sum of corrected areas: 22912078

4449.D GCMS0308.M Fri Mar 22 09:43:26 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAR2102\4449.D
Operator :
Acquired : 21 Mar 2002 10:08 pm using AcqMethod GCMS0308
Instrument : GC/MS 209
Sample Name: gc/ms scan 3/1
Misc Info :
Vial Number: 12
Quant File :GCMS0308.RES (RTE Integrator)

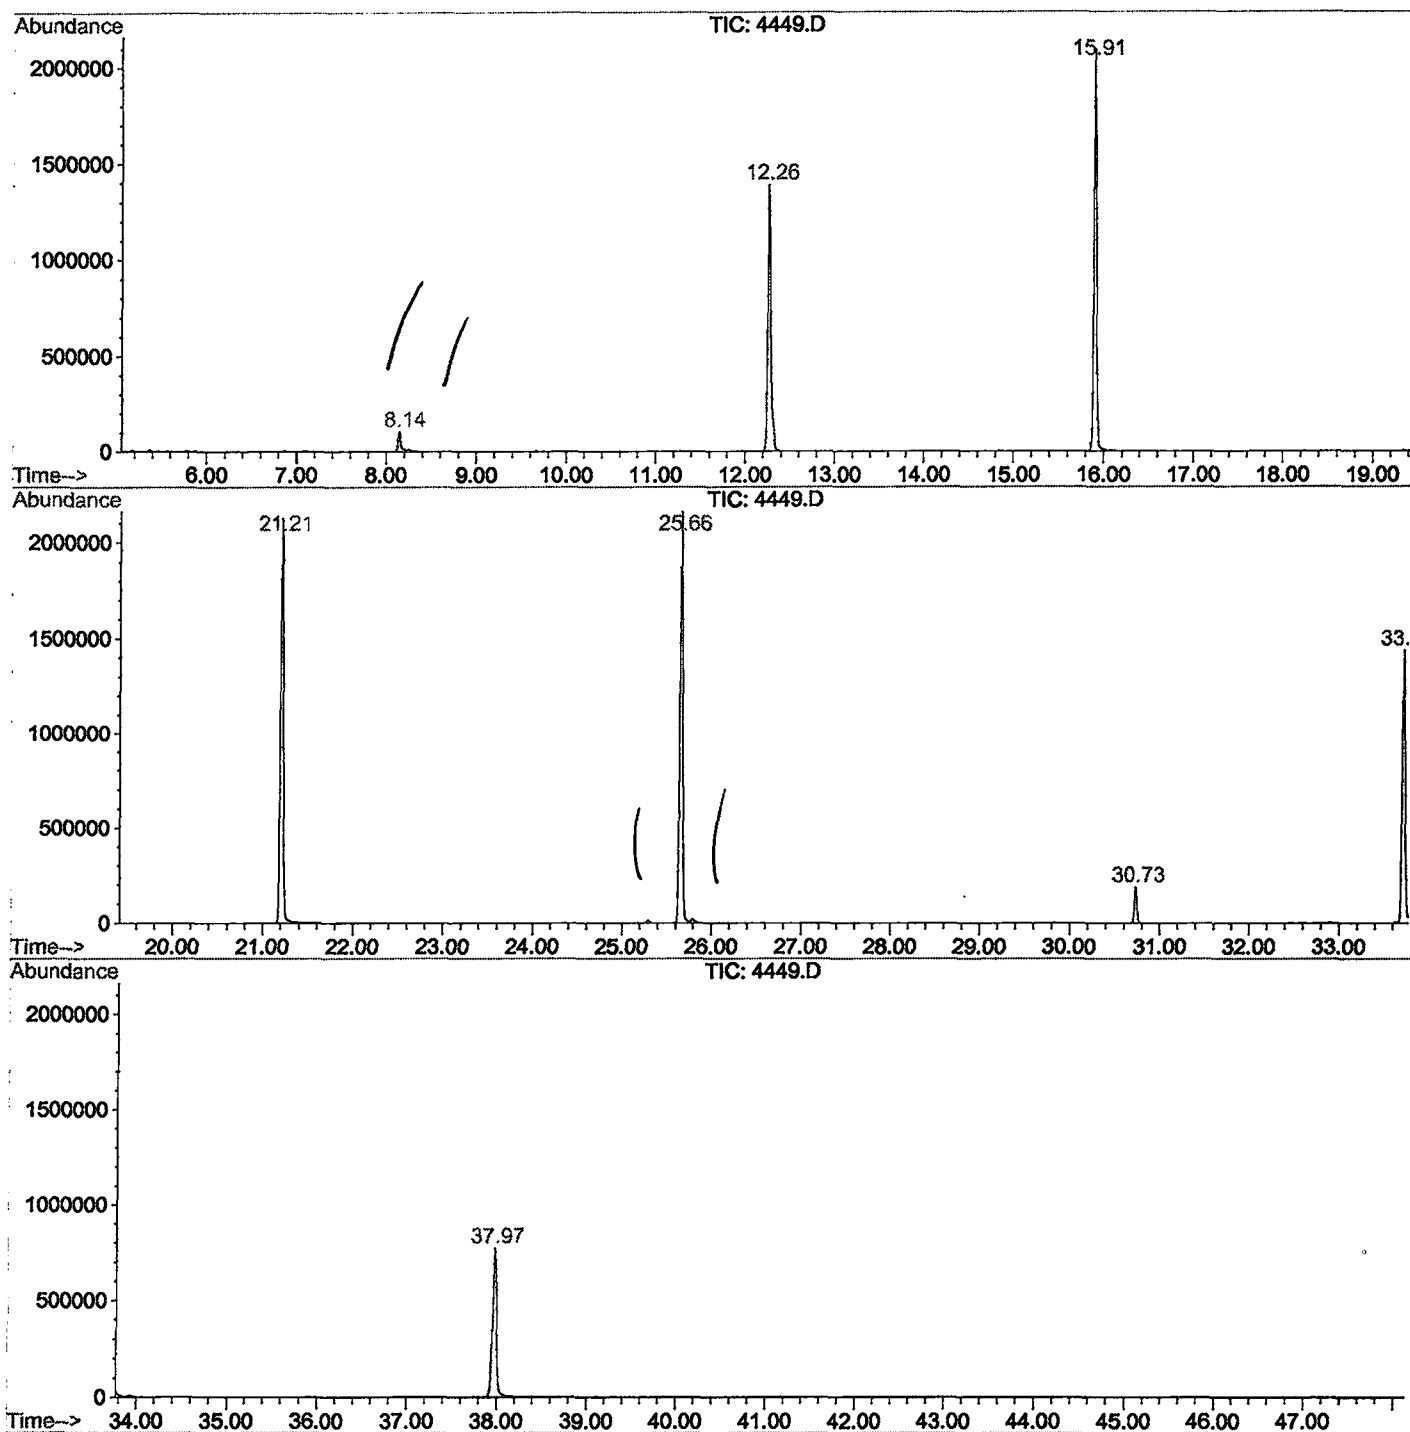

4449.D GCMS0308.M

Fri Mar 22 09:43:31 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR2102\4449.D
 Acq On : 21 Mar 2002 10:08 pm
 Sample : gc/ms scan 3/1
 Misc :
 MS Integration Params: LSCINT.P


Vial: 12
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 N-Ethylformamide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.14	1.50 ug/l	239324	1,4-Dichlorobenzene-d4	12.26

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	N-Ethylformamide	73	C3H7NO	000627-45-2	9	
2	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9	
3	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9	
4	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9	

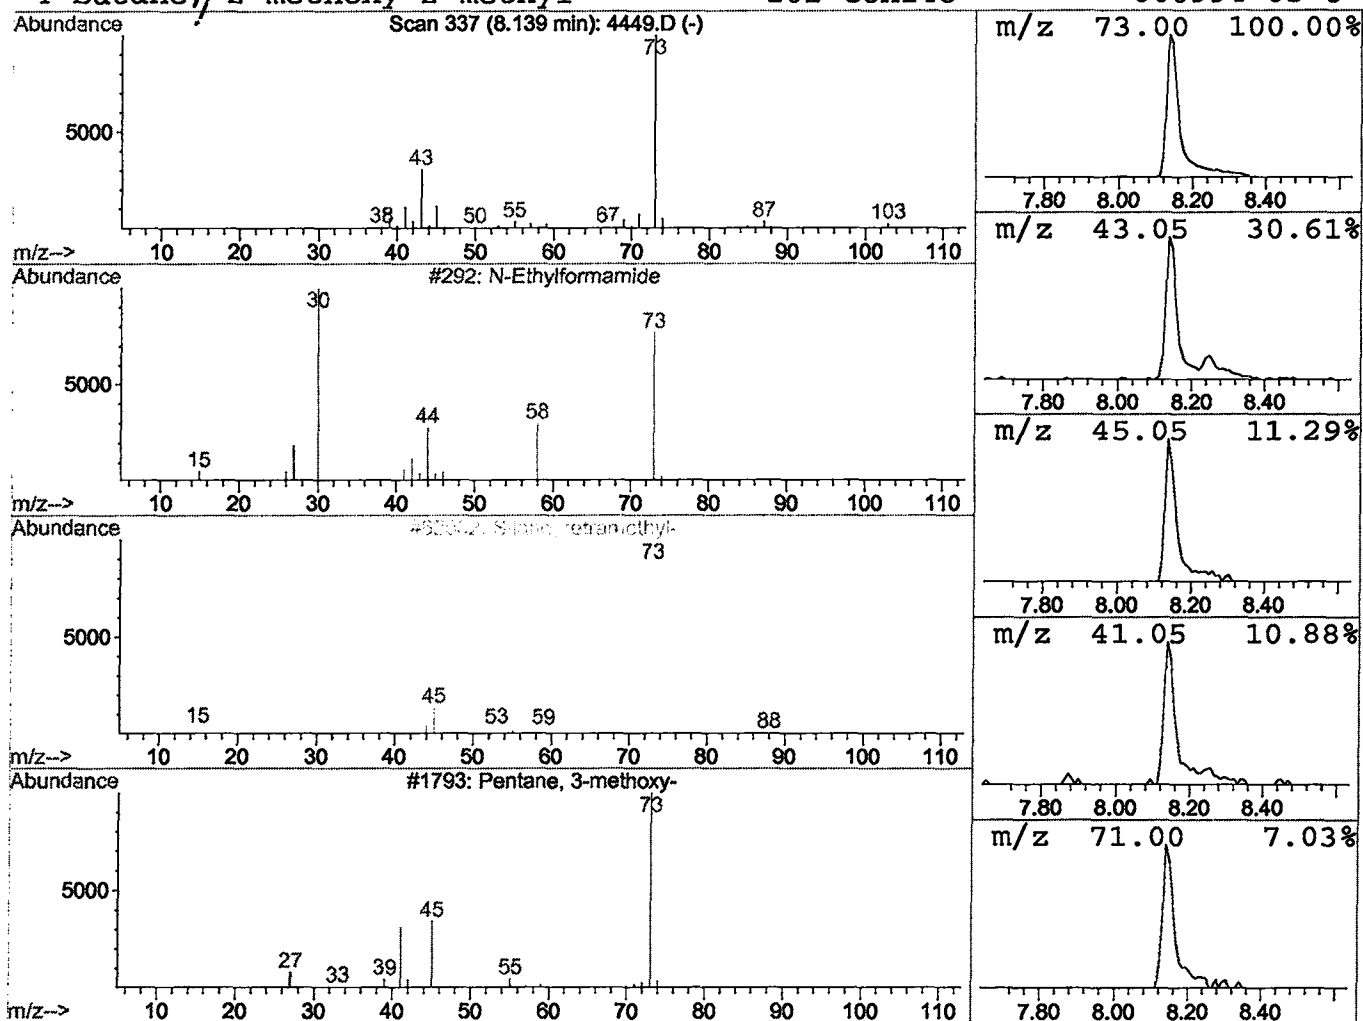

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 21 Mar 2002 10:08 pm
Data File: C:\HPCHEM\1\DATA\MAR2102\4449.D
Name: gc/ms scan 3/1
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc Units	Area	IntStd	ISRT	ISArea	ISConc
<u>N-Ethylformamide</u>	8.14	1.5 ug/l	239324	ISTD01	12.26	3201250	20.0
4449.D GCMS0308.M	Fri Mar 22 09:43:39 2002						