

Method 508 MOD.Date Extracted 3-1-02Page 116

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
L.B.		500ml		1ml			1ml		7			
Ref 1					1ml							
Ref 2					1ml							
4336												
4337	F.B.											
4377												
4378												
4379												
4380	F.B.											
4381												
4382												
4383												
4384	F.B.											
* No sample 4336 Extract on Tray Reext on 3/28/02												
Remarks 4377 WAS ACIDIC AND NaOH WAS ADDED TO bring pH TO SEVEN OR NEUTRAL												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - SEP. FUN. Solv. lot# <u>TD 1252</u> NaCl lot# <u>V39618</u> Na2SO4 lot# <u>V46623</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF SPIKE	2193											
MDL/MDRF												
Q. CHECK												
INT. STD.	2203d											
SURROGATE	2160 R											
LPC												
ENDRIN/DDT												

Analyst A.D.
revision 4/12/01

Verified by _____

Reviewed by DN
Date 4/2/02

Sequence Name: C:\MSDCHEM\1\SEQUENCE\032502.S

Comment:

Operator: McLean

Data Path: C:\MSDCHEM\1\DATA\032602\

Pre-Seq Cmd:

Post-Seq Cmd:


Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	14	DFTPP	508SCAN	DFTPP 3/25
2	Sample	15	CAL40X	508SCAN	CAL 40 A
3	Sample	3	MCDD0322	508SCAN	MC
4	Sample	17	CAL10X	508SCAN	CAL 10 A
5	Sample	19	MCIS	508SCAN	MC WITH IS
6	Sample	18	SURRXX	508SCAN	SURROGATE
7	Sample	1	228LB	508SCAN	2/28/02
8	Sample	2	228REF1	508SCAN	2/28/02
9	Sample	3	228REF2	508SCAN	2/28/02
10	Sample	4	4247	508SCAN	2/28/02
11	Sample	5	4334B	508SCAN	2/28/02
12	Sample	6	4330	508SCAN	2/28/02
13	Sample	7	4331	508SCAN	2/28/02
14	Sample	8	4246	508SCAN	2/28/02
15	Sample	9	4335	508SCAN	2/28/02
16	Sample	10	4245	508SCAN	2/28/02
17	Sample	11	4333	508SCAN	2/28/02
18	Sample	12	4248	508SCAN	2/28/02
19	Sample	13	4332	508SCAN	2/28/02
20	Sample	14	DFTB0326	508SCAN	DFTPP
21	Sample	17	C10B326	508SCAN	CAL 10
22	Sample	23	C10M326	508SCAN	CAL 10M
23	Sample	24	C25M326	508SCAN	CAL 25M
24	Sample	18	SURRB	508SCAN	SURROGATE
25	Sample	26	LBB326	508SCAN	LB 3/1/02
26	Sample	27	REF1B326	508SCAN	REF 1 3/1/02
27	Sample	28	REF2B326	508SCAN	REF 2 3/1/02
28	Sample	29	4337FB	508SCAN	SAMPLE 4337 3/1/02
29	Sample	30	4377	508SCAN	SAMPLE 4377
30	Sample	31	4378	508SCAN	SAMPLE 4378
31	Sample	32	4379	508SCAN	SAMPLE 4379
32	Sample	33	4380FB	508SCAN	SAMPLE 4380
33	Sample	34	4381	508SCAN	SAMPLE 4381
34	Sample	35	4382	508SCAN	SAMPLE 4382
35	Sample	36	4383	508SCAN	SAMPLE 4383
36	Sample	37	4384FB	508SCAN	SAMPLE 4384
37	Sample	14	DFTC326	508SCAN	DFTPP
38	Sample	17	C10C326	508SCAN	CAL 10
39	Sample	22	C100C326	508SCAN	CAL 100
40	Sample	18	SURRC	508SCAN	SURROGATE
41	Sample	51	LBC326	508SCAN	LB 3/2/02
42	Sample	52	REF1C326	508SCAN	REF 1 3/2/02
43	Sample	53	REF2C326	508SCAN	REF 2 3/2/02

Sequence Name: C:\MSDCHEM\1\SEQUENCE\032502.S

Line	Type	Vial	DataFile	Method	Sample Name
44	Sample	54 4509	508SCAN	SAMPLE 4509	3/2/02
45	Sample	55 4510	508SCAN	SAMPLE 4510	3/2/02
46	Sample	56 4511	508SCAN	SAMPLE 4511	3/2/02
47	Sample	57 4512	508SCAN	SAMPLE 4512	3/2/02
48	Sample	58 4513	508SCAN	SAMPLE 4513	3/2/02
49	Sample	59 4514	508SCAN	SAMPLE 4514	3/2/02
50	Sample	60 4515	508SCAN	SAMPLE 4515	3/2/02

File : C:\MSDCHEM\1\DATA\032602\DFTB0326.D
Operator : McLean
Acquired : 26 Mar 2002 9:49 pm using AcqMethod 508SCAN
Instrument : Instrumen
Sample Name: DFTPP
Misc Info :
Vial Number: 14

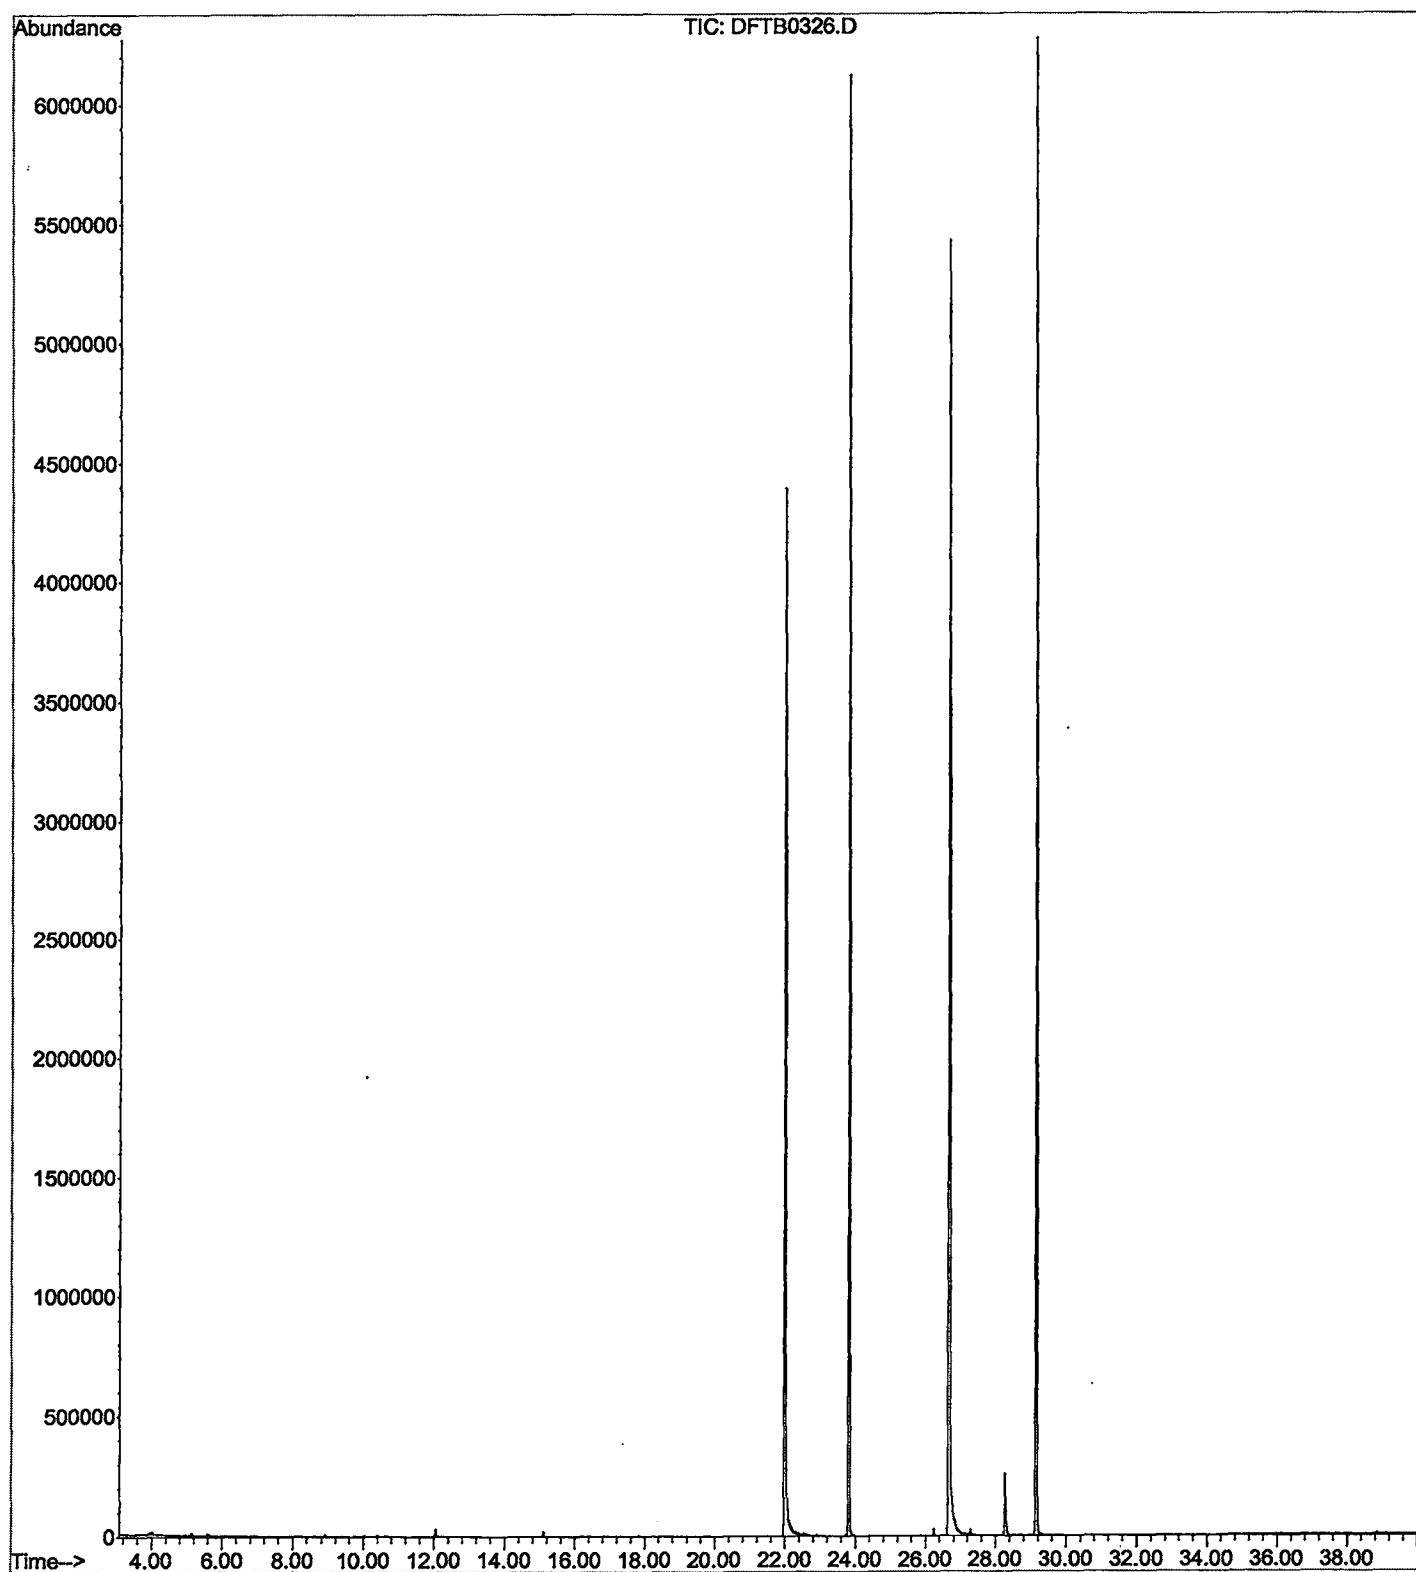

DFTPP

Data File : C:\MSDCHEM\1\DATA\032602\DFTB0326.D

Acq On : 26 Mar 2002 9:49 pm

Sample : DFTPP

Misc :

MS Integration Params: BENZO.P

Vial: 14

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Spectrum Information: Scan 3531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.5	391488	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.5	330304	PASS
70	69	0.00	2	0.3	1124	PASS
127	198	10	80	49.9	339520	PASS
197	198	0.00	2	0.0	0	PASS
198	198	50	100	100.0	680896	PASS
199	198	5	9	6.6	44920	PASS
275	198	10	60	21.6	146880	PASS
365	198	1	100	2.7	18512	PASS
441	443	0.01	100	84.3	91752	PASS
442	198	50	100	88.0	599104	PASS
443	442	15	24	18.2	108904	PASS

DFTB0326.D 5080302.M

Wed Mar 27 08:54:23 2002