


User: Bohlk, Ted
Westchester Dept. of Labs & Research
Date: 06/04/2002 Time: 12:29:54

Sample: AE11555
Analysis: SLP525 Organic Extractables
Units: ug
Started: 5/29/02 12:27 Ended: 5/29/02 12:27 Analyst: TB
Result source: manual entry
Page: 1

	Component Name	Vial	Result
1	DFTPP		PASSED
2	ENDRIN		2.8
3	DDT		0

File : C:\MSDCHEM\1\DATA\052902\DFTB0529.D
 Operator : Bohlk / Inst 213
 Acquired : 29 May 2002 10:48 am using AcqMethod 052802
 Instrument : Instrumen
 Sample Name: DFTPP/ENDRIN
 Misc Info :
 Vial Number: 1

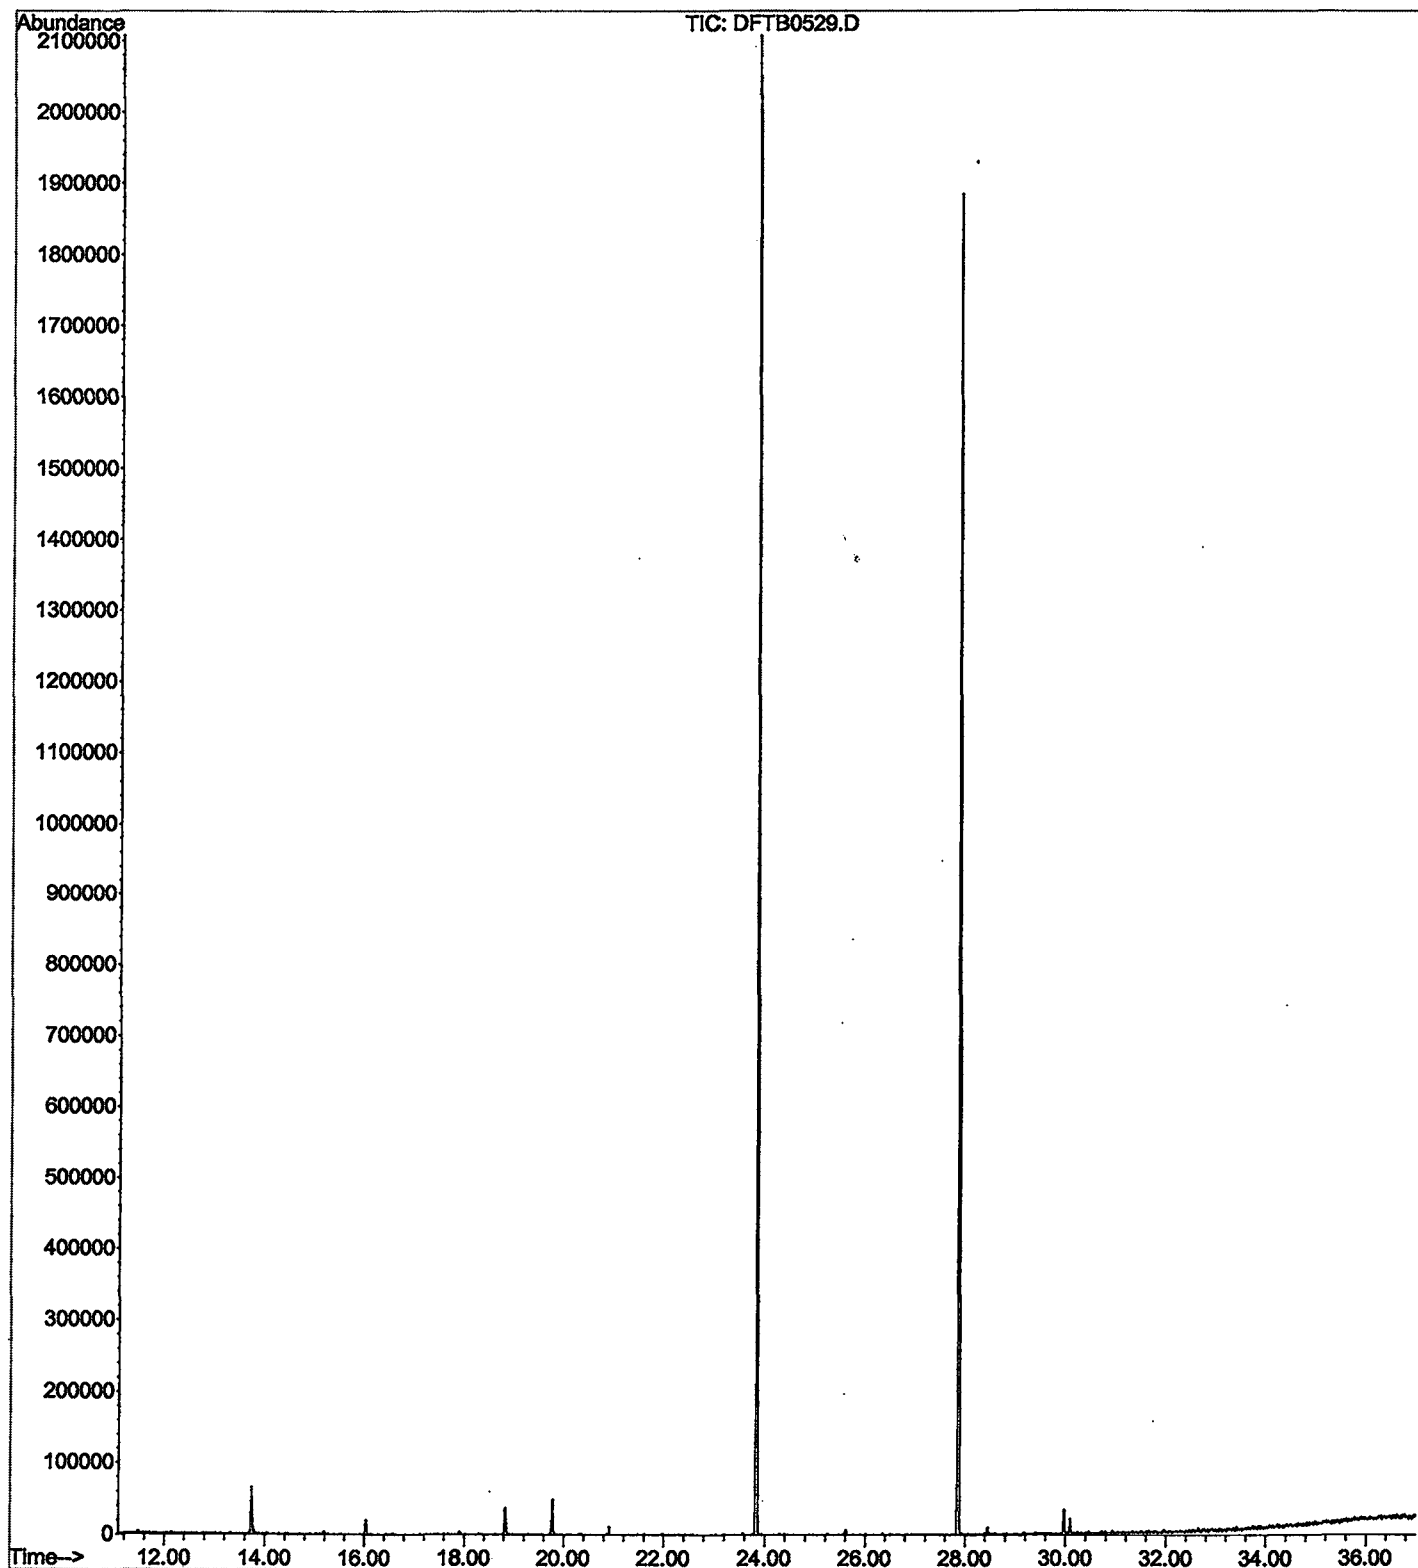

DRIFT

Data File : C:\MSDCHEM\1\DATA\052902\DFTB0529.D

Acq On : 29 May 2002 10:48 am

Sample : DFTPP/ENDRIN

Misc :

MS Integration Params: rteint.p

Vial: 1

Operator: Bohlk / Inst 213

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\052802.M (RTE Integrator)

Title : Quantitation For Method 525.2

Spectrum Information: Average of 23.793 to 23.874 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	27918	PASS
68	69	0.00	2	0.2	57	PASS
69	198	0.00	100	38.4	32343	PASS
70	69	0.00	2	0.2	54	PASS
127	198	10	80	53.6	45163	PASS
197	198	0.00	2	0.3	244	PASS
198	198	50	100	100.0	84214	PASS
199	198	5	9	6.0	5056	PASS
275	198	10	60	18.0	15121	PASS
365	198	1	100	1.9	1625	PASS
441	443	0.01	100	73.9	8345	PASS
442	198	50	100	67.6	56892	PASS
443	442	15	24	19.8	11289	PASS

DFTB0529.D 052802.M

Wed May 29 11:33:18 2002

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\052902\DFTB0529.D

Vial: 1

Acq On : 29 May 2002 10:48 am

Operator: Bohlk / Inst 213

Sample : DFTPP/ENDRIN

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: rteint.p

Method : C:\MSDCHEM\1\5973N\052802.M (RTE Integrator)

Title : Quantitation For Method 525.2

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 5000 Area counts

Start Thrs: 0.2

Max Peaks: 10

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5


Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	27.856	1846	1850	1855	rM 2	1885789	3265780	100.00%	97.234%
2	28.455	1912	1916	1918	rM	8889	10997	0.34%	0.327%
3	29.979	2080	2084	2087	rM 2	33210	54305	1.66%	1.617%
4	30.087	2092	2096	2100	rM 4	20422	27614	0.85%	0.822%

Sum of corrected areas: 3358696

2.8 %
Endrin
Breakdown

File : C:\MSDCHEM\1\DATA\052902\DDTB0529.D
Operator : Bohlk / Inst 213
Acquired : 29 May 2002 11:34 am using AcqMethod 052802
Instrument : Instrumen
Sample Name: DDT
Misc Info :
Vial Number: 2

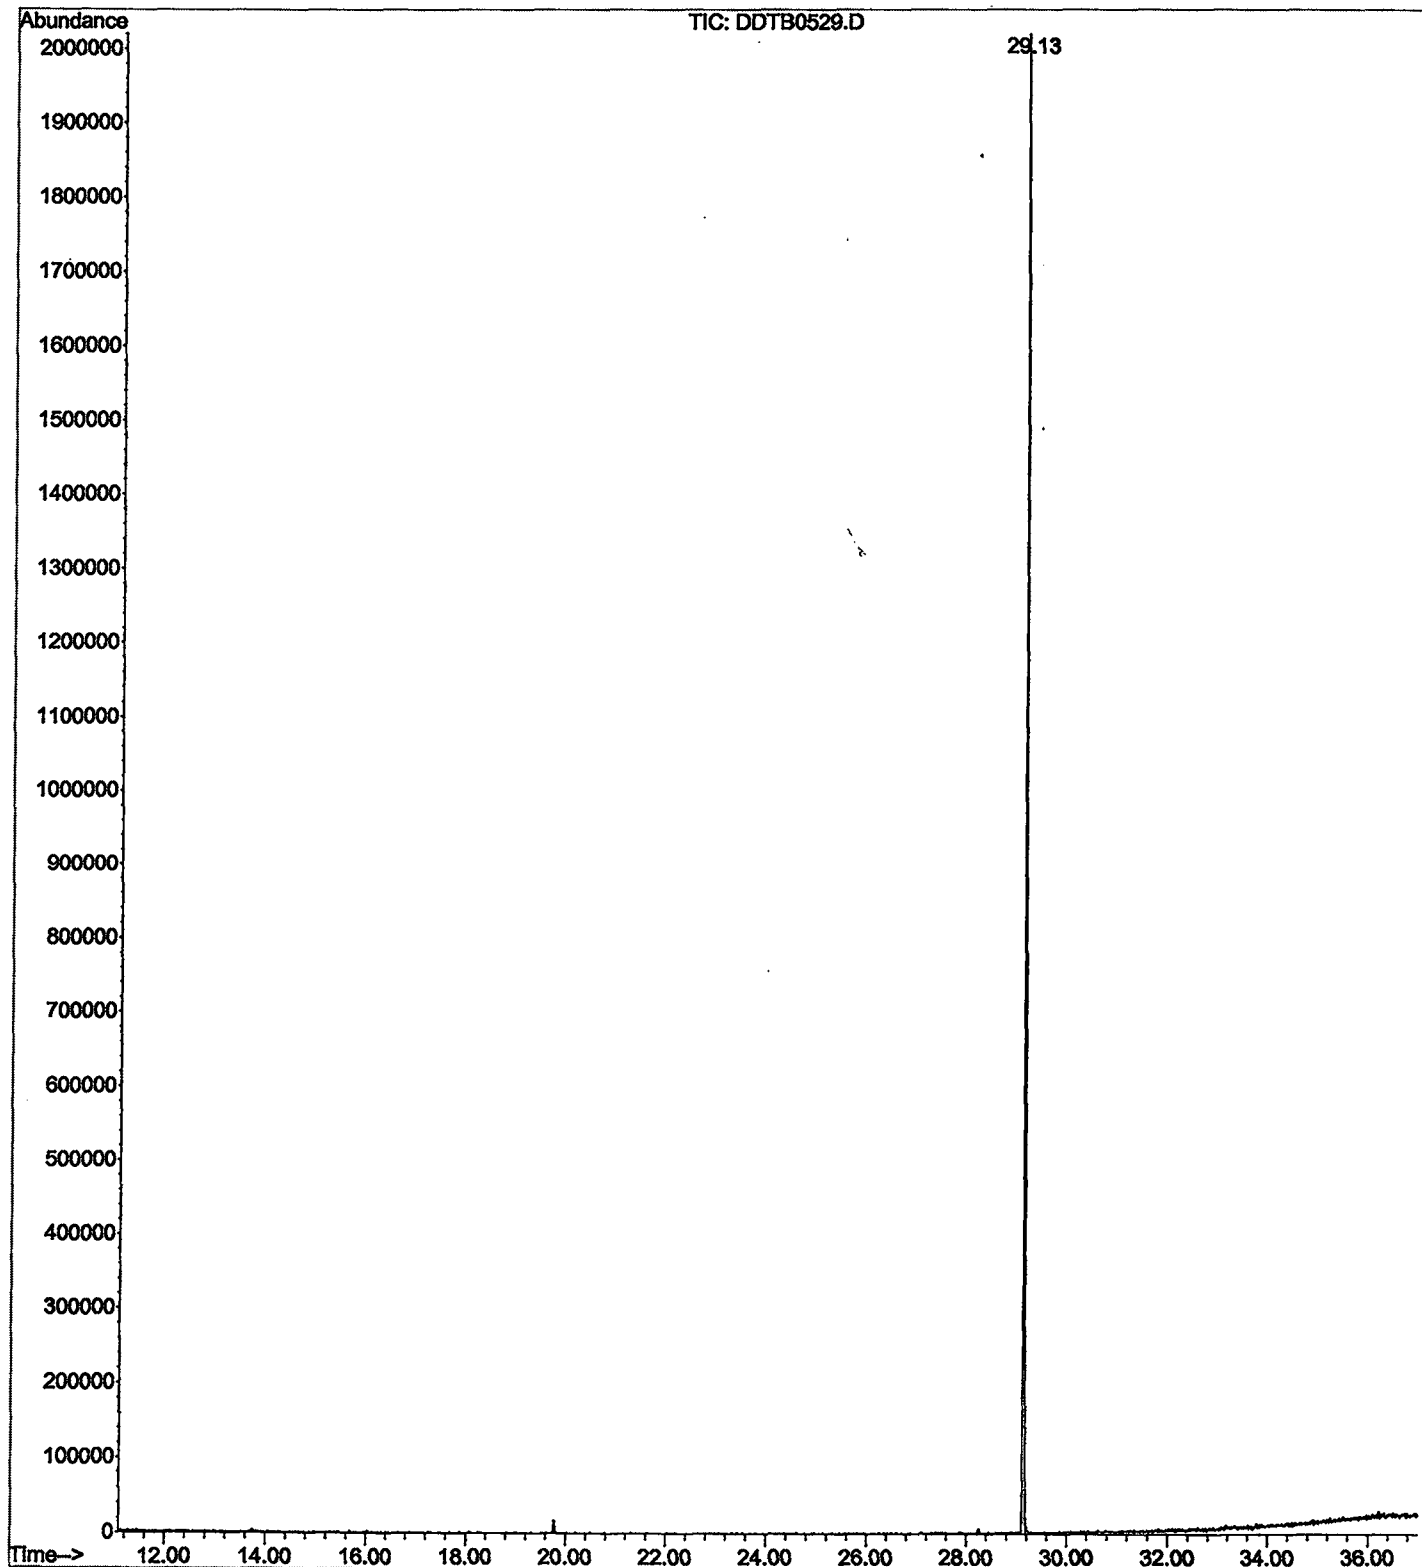

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\052902\DDTB0529.D
 Acq On : 29 May 2002 11:34 am
 Sample : DDT
 Misc :
 MS Integration Params: rteint.p

Vial: 2
 Operator: Bohlk / Inst 213
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\052802.M (RTE Integrator)
 Title : Quantitation For Method 525.2
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 5000 Area counts
 Start Thrs: 0.2 Max Peaks: 10
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5


Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	29.126	1986	1990	1996	rM	2020064	3408129	100.00%	100.000%

Sum of corrected areas: 3408129

0.1 DDT
 Breakdown

File : C:\MSDCHEM\1\DATA\053002\DFTB0530.D
 Operator : Bohlk / Inst 213
 Acquired : 30 May 2002 9:02 am using AcqMethod 052802
 Instrument : Instrumen
 Sample Name: DFTPP/ENDRIN
 Misc Info :
 Vial Number: 1

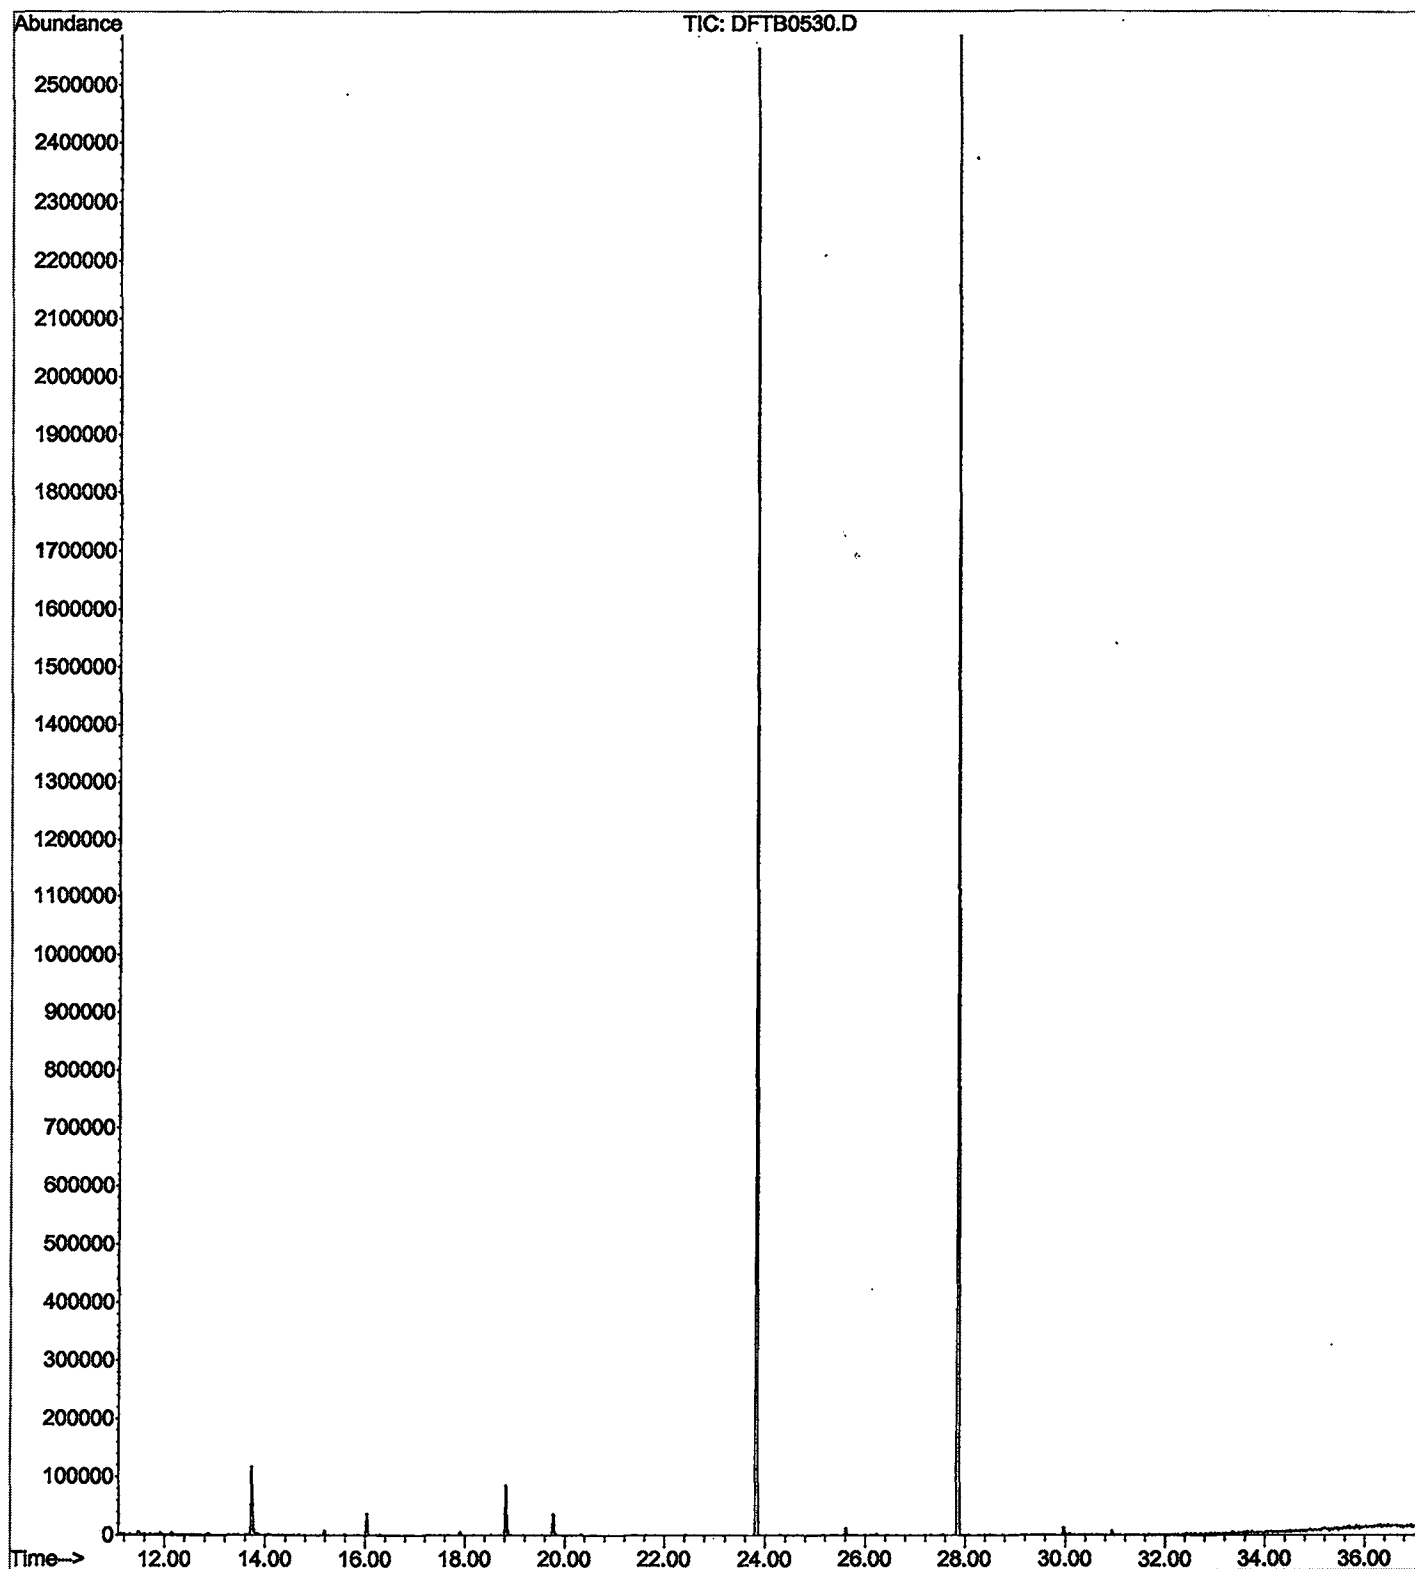

DFTPP

Data File : C:\MSDCHEM\1\DATA\053002\DFTB0530.D

Acq On : 30 May 2002 9:02 am

Sample : DFTPP/ENDRIN

Misc :

MS Integration Params: rteint.p

Vial: 1

Operator: Bohlk / Inst 213

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\052802.M (RTE Integrator)

Title : Quantitation For Method 525.2

Spectrum Information: Average of 23.784 to 23.874 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	30627	PASS
68	69	0.00	2	0.6	225	PASS
69	198	0.00	100	38.6	36304	PASS
70	69	0.00	2	0.3	120	PASS
127	198	10	80	54.2	51004	PASS
197	198	0.00	2	0.1	100	PASS
198	198	50	100	100.0	94117	PASS
199	198	5	9	6.4	6035	PASS
275	198	10	60	18.7	17631	PASS
365	198	1	100	1.8	1722	PASS
441	443	0.01	100	78.4	9717	PASS
442	198	50	100	72.2	67912	PASS
443	442	15	24	18.3	12394	PASS

DFTB0530.D 052802.M

Thu May 30 16:21:07 2002

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\053002\DFTB0530.D
Acq On : 30 May 2002 9:02 am
Sample : DFTPP/ENDRIN
Misc :
MS Integration Params: rteint.p

Vial: 1
Operator: Bohlk / Inst 213
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\052802.M (RTE Integrator)
Title : Quantitation For Method 525.2
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 5000 Area counts
Start Thrs: 0.2 Max Peaks: 10
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5


Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	27.856	1846	1850	1855	rM	2585297	4753205	100.00%	99.393%
2	29.969	2080	2083	2087	rM 2	13001	21439	0.45%	0.448%
3	30.096	2093	2097	2100	rM 2	3484	7573	0.16%	0.158%

Sum of corrected areas: 4782217

0.61 %
Endrin
Breakdown

File : C:\MSDCHEM\1\DATA\053002\DDTB0530.D
 Operator : Bohlk / Inst 213
 Acquired : 30 May 2002 9:47 am using AcqMethod 052802
 Instrument : Instrumen
 Sample Name: DDT
 Misc Info :
 Vial Number: 2

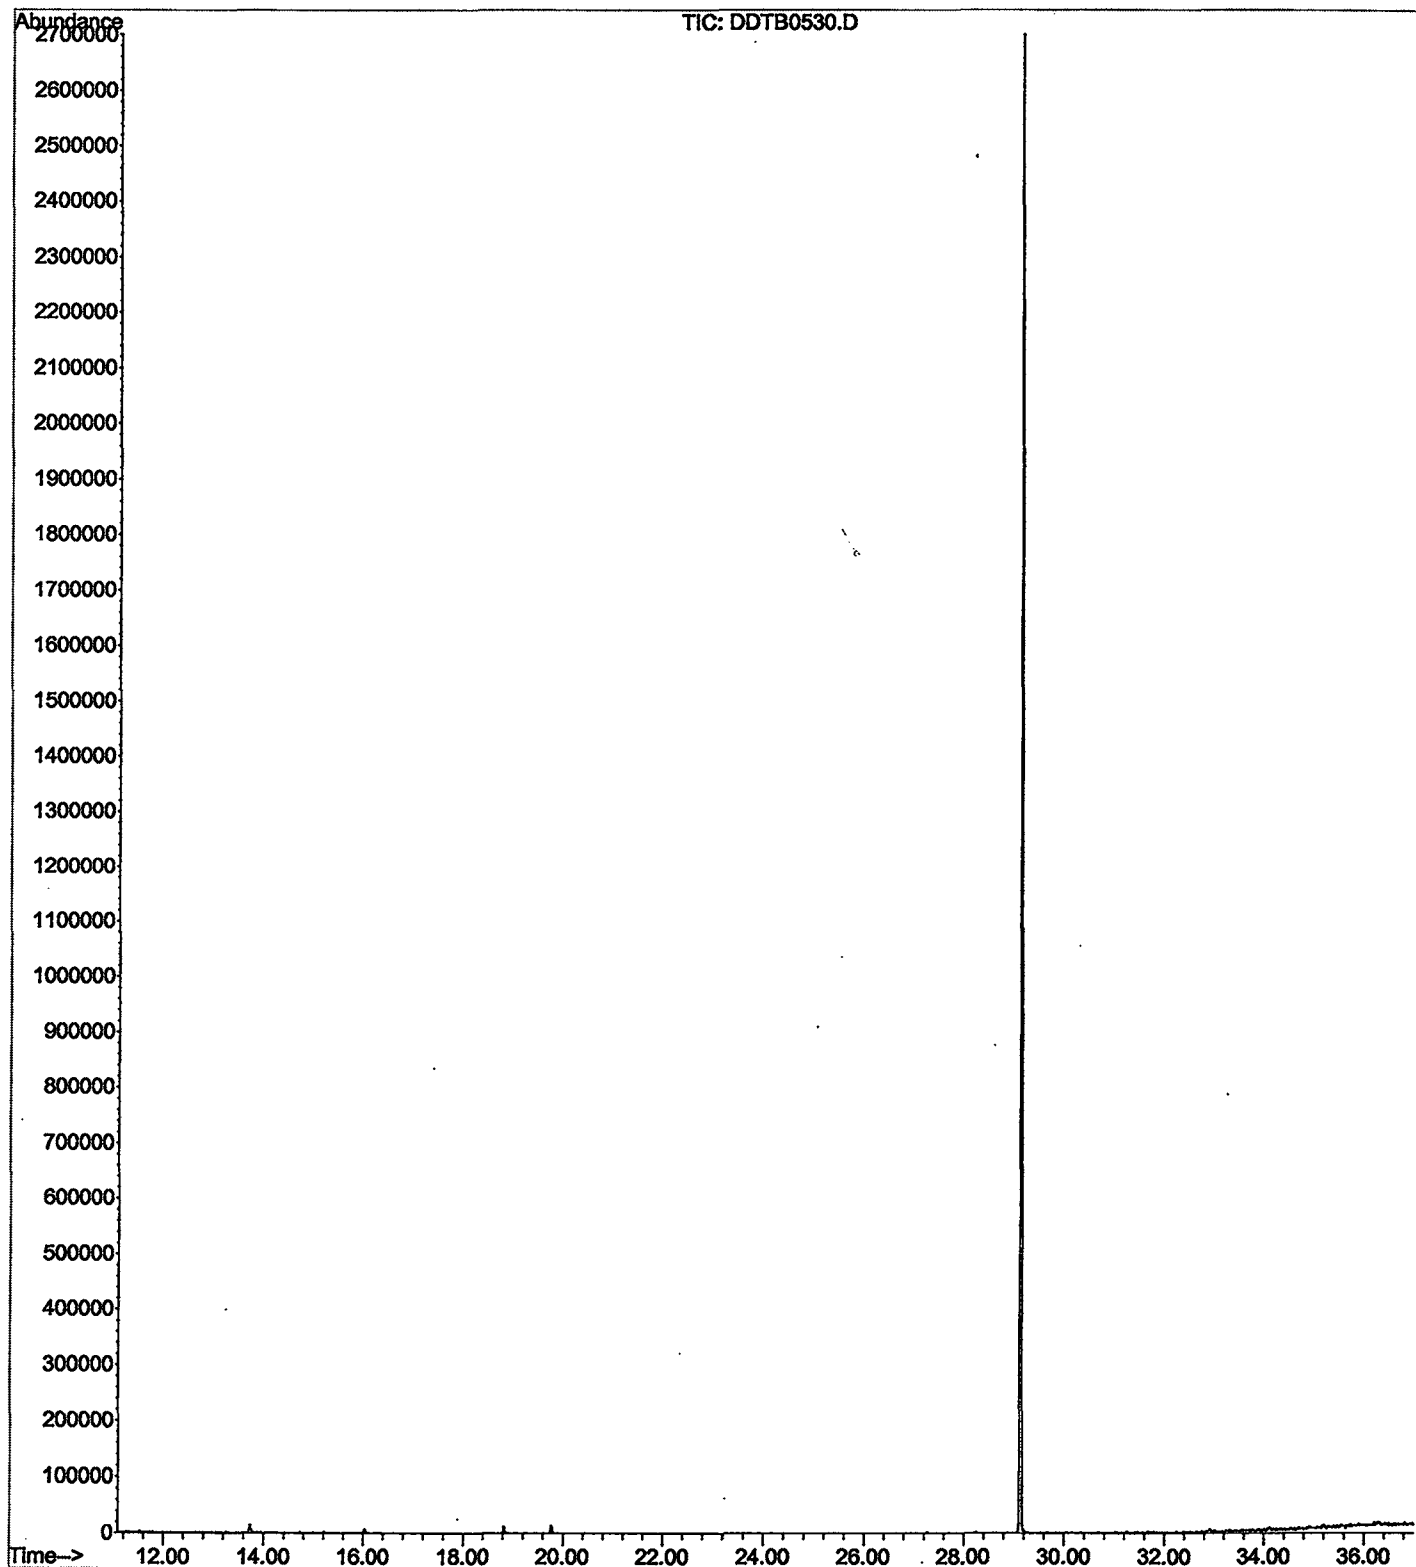

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\053002\DDTB0530.D

Vial: 2

Acq On : 30 May 2002 9:47 am

Operator: Bohlk / Inst 213

Sample : DDT

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: rteint.p

Method : C:\MSDCHEM\1\5973N\052802.M (RTE Integrator)

Title : Quantitation For Method 525.2

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 5000 Area counts

Start Thrs: 0.2

Max Peaks: 10

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	29.126	1984	1990	1999	rM	2700744	4631703	100.00%	100.000%

Sum of corrected areas: 4631703

0 % DDT

Breakdown