


DFTPP

Data File : C:\HPCHEM\1\DATA\MAY2102\DFTPP1.D
 Acq On : 21 May 2002 2:35 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

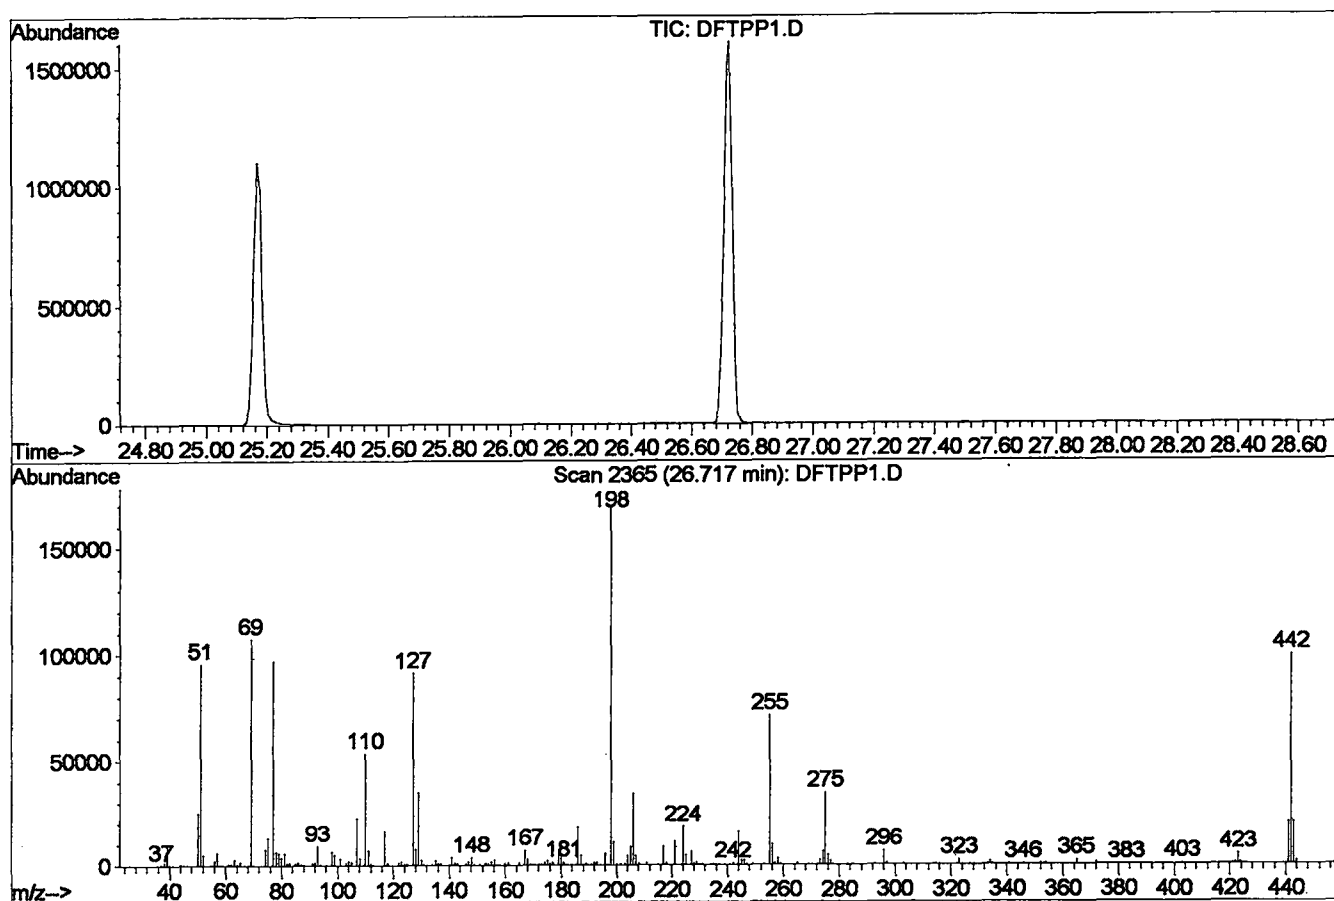

Spectrum Information: Scan 2365

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	56.5	96032	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	63.3	107656	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	53.9	91688	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	170112	PASS
199	198	5	9	6.7	11437	PASS
275	198	10	30	20.5	34864	PASS
365	198	1	100	1.3	2285	PASS
441	443	0.01	100	99.3	20208	PASS
442	198	40	110	58.5	99456	PASS
443	442	17	23	20.5	20352	PASS