

Quantitation Report


(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0602\9677.D
 Acq On : 7 May 2002 10:54 am
 Sample : GC/MS SCAN 4/25
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 9 8:53 2002

Vial: 20
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0501



Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.19	152	653872	40.00	ug/l	-0.02
10) Naphthalene-d8	15.83	136	2412396	40.00	ug/l	-0.02
17) Acenaphthene-d10	21.13	164	1320925	40.00	ug/l	-0.01
30) Phenanthrene-d10	25.58	188	1836311	40.00	ug/l	-0.01
38) Chrysene-d12	33.63	240	1014546	40.00	ug/l	-0.03
44) Perylene-d12	37.87	264	611819	40.00	ug/l	-0.01

System Monitoring Compounds

28) TCMX	23.27	209	39174	6.09	ug/L	-0.02
Spiked Amount	10.000		Recovery	=	60.90%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.		
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	15.88	128	837	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-Chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	21.46	165	264	N.D.		
25) Diethylphthalate	22.62	149	883	N.D.		
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.63	178	206	N.D.		

(#) = qualifier out of range (m) = manual integration

9677.D GCMS0501.M Thu May 09 08:53:55 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0602\9677.D

Vial: 20

Acq On : 7 May 2002 10:54 am

Operator:

Sample : GC/MS SCAN 4/25

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 9 8:53 2002

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed May 01 10:40:31 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0501

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.64	178	206	N.D.		
36) Di-n-butylphthalate	27.54	149	2167	N.D.		
37) Fluoranthene	29.26	202	187	N.D.		
39) Pyrene	29.94	202	323	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.63	228	3084	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.86	149	3894	N.D.		
43) Chrysene	33.71	228	482	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	36.69	252	1262	N.D.		
47) Benzo(k)fluoranthene	36.69	252	1262	N.D.		
48) Benzo(a)pyrene	37.87	252	2501	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

9677.D GCMS0501.M

Thu May 09 08:53:56 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY0602\9677.D
 Acq On : 7 May 2002 10:54 am
 Sample : GC/MS SCAN 4/25
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 9 8:53 2002

Vial: 20
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration

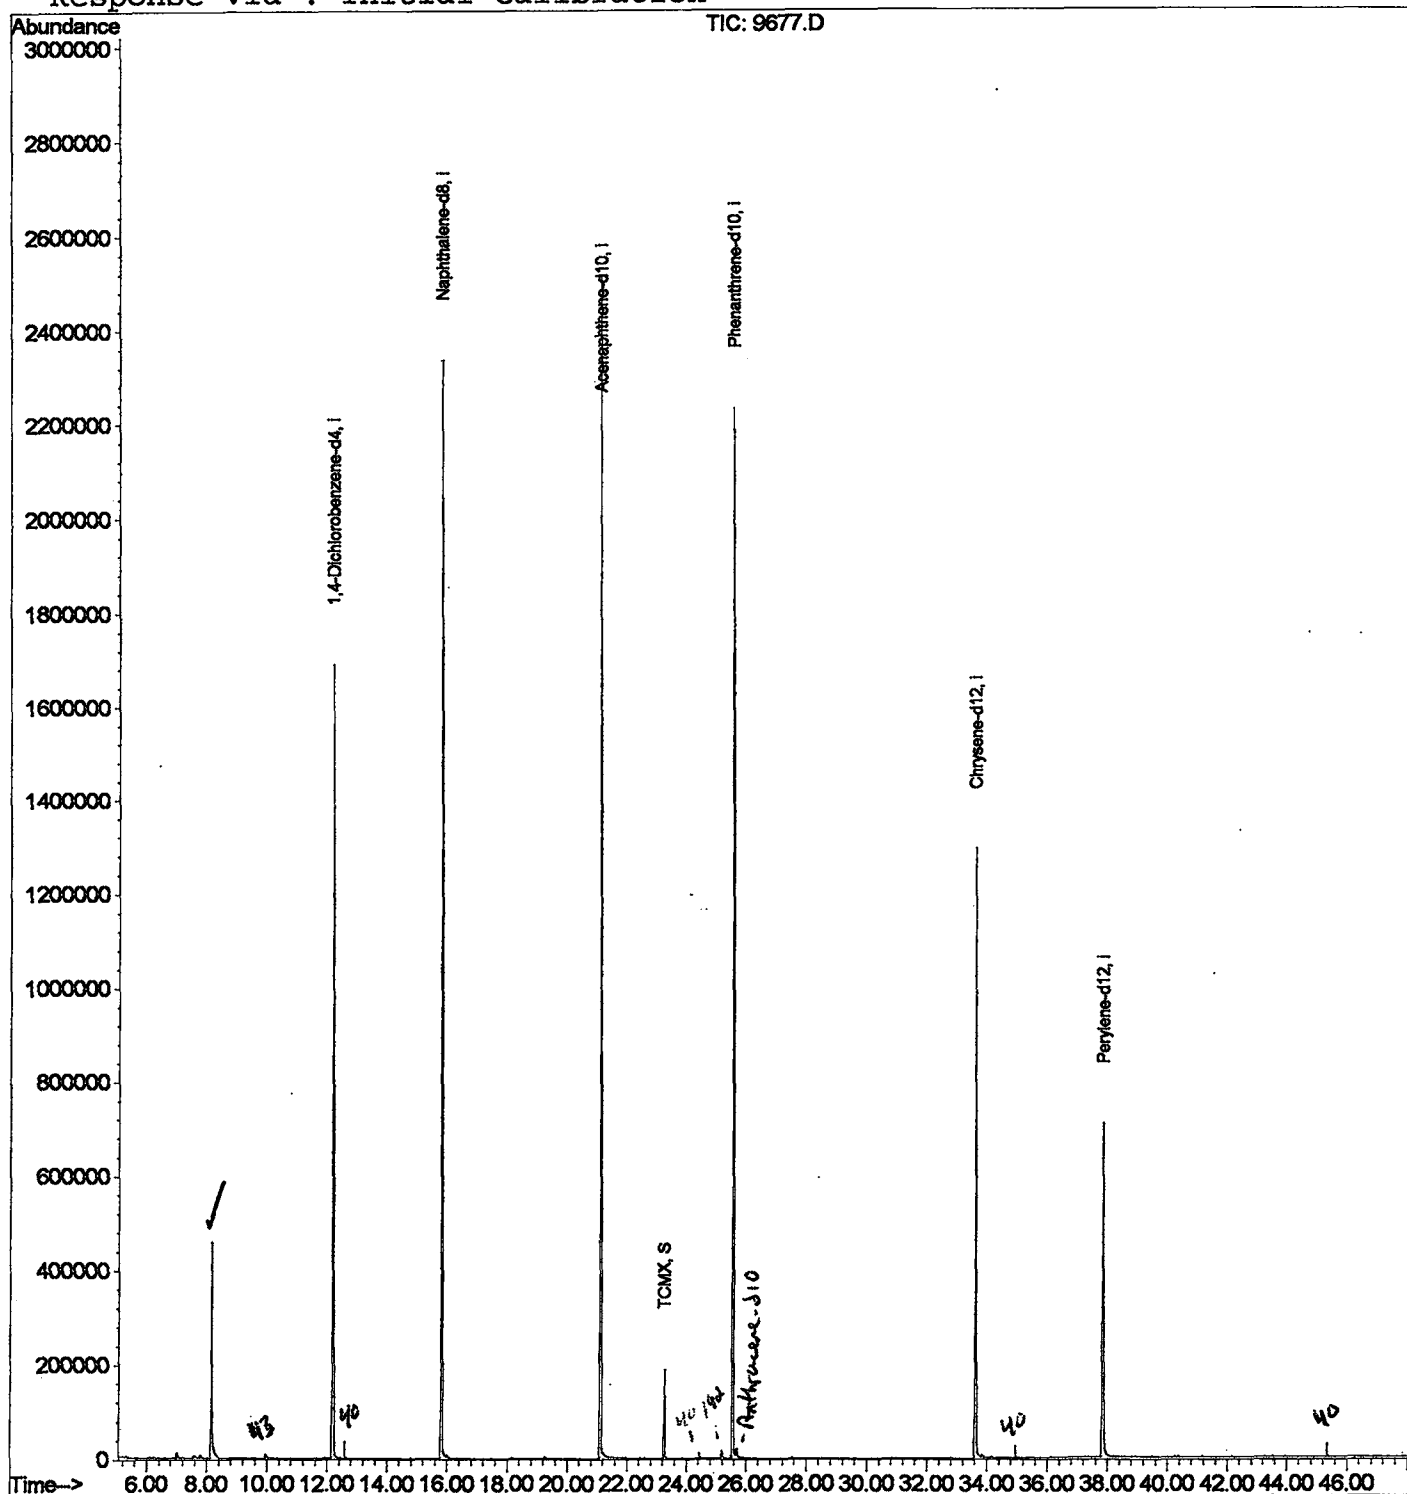

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY0602\9677.D

Vial: 20

Acq On : 7 May 2002 10:54 am

Operator:

Sample : GC/MS SCAN 4/25

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.159	336	340	371	rVB	457770	1004028	18.97%	3.991%
2	12.191	775	780	797	rBV	1688038	3718093	70.23%	14.780%
3	15.829	1170	1177	1193	rBV	2336611	4755336	89.82%	18.903%
4	21.135	1749	1756	1775	rBV	2516631	5294038	100.00%	21.045%
5	23.270	1982	1989	1996	rBV	189574	372570	7.04%	1.481%
6	25.579	2233	2241	2250	rBV2	2232386	4873158	92.05%	19.372%
7	33.634	3113	3120	3136	rBV2	1291085	3015754	56.97%	11.988%
8	37.868	3573	3582	3600	rBV2	703996	2122883	40.10%	8.439%




Sum of corrected areas: 25155860

9677.D GCMS0501.M

Thu May 09 11:25:17 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0602\9677.D
 Operator :
 Acquired : 7 May 2002 10:54 am using AcqMethod GCMS0501
 Instrument : 209
 Sample Name: GC/MS SCAN 4/25
 Misc Info :
 Vial Number: 20
 Quant File : GCMS0501.RES (RTE Integrator)

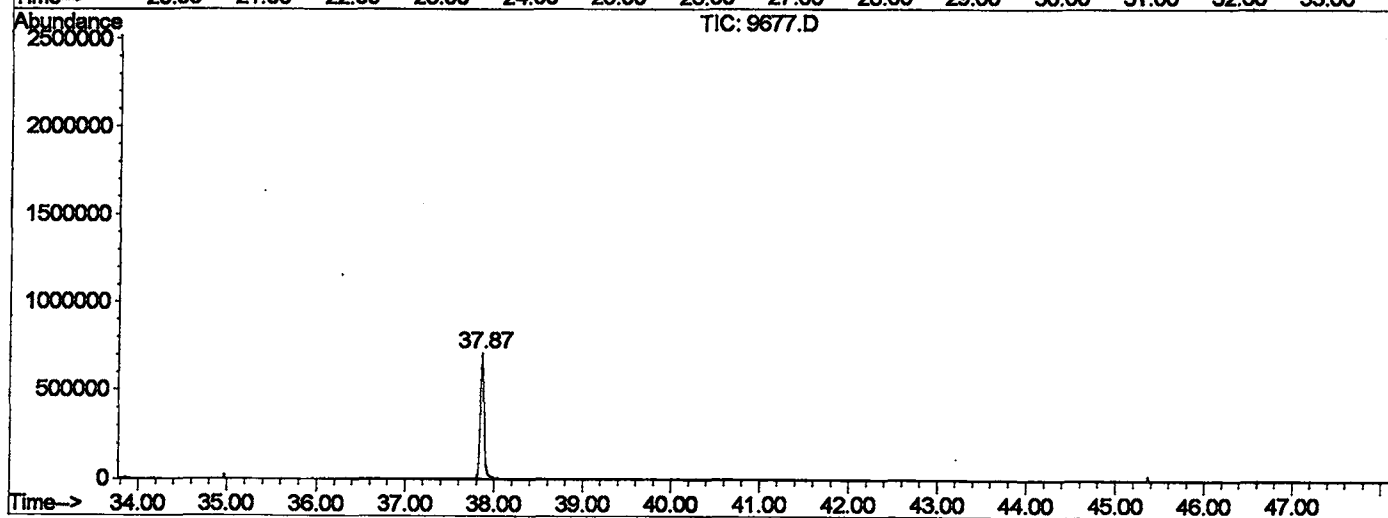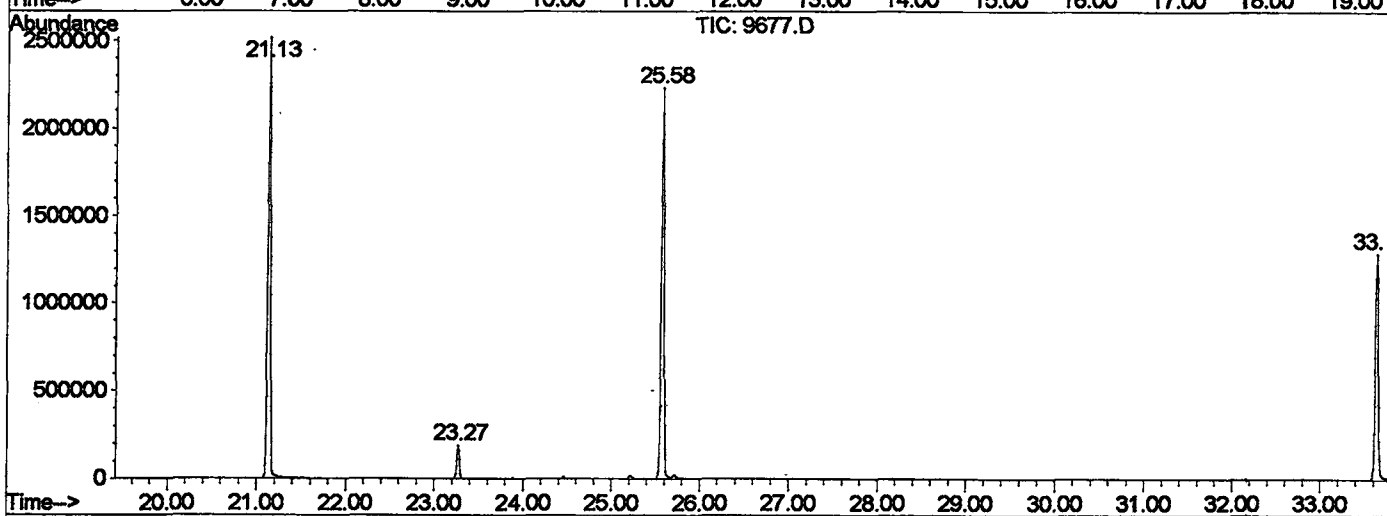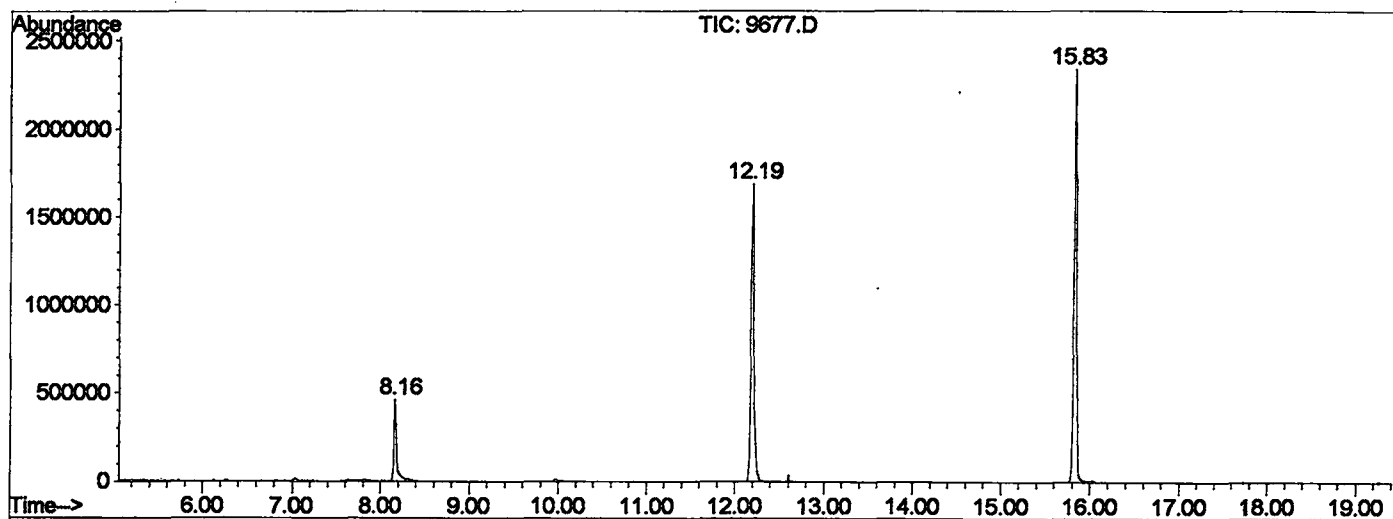

9677.D GCMS0501.M Thu May 09 11:25:17 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY0602\9677.D
Acq On : 7 May 2002 10:54 am
Sample : GC/MS SCAN 4/25
Misc :
MS Integration Params: LSCINT.P










Vial: 20
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.16	10.80 ug/l	1004030	1,4-Dichlorobenzene-d4	12.19

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78	
2	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9	
3	Acetone	58	C3H6O	000067-64-1	7	
4	Butane	58	C4H10	000106-97-8	5	

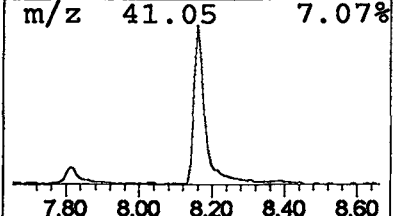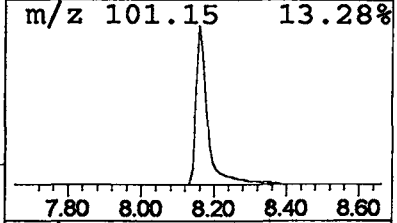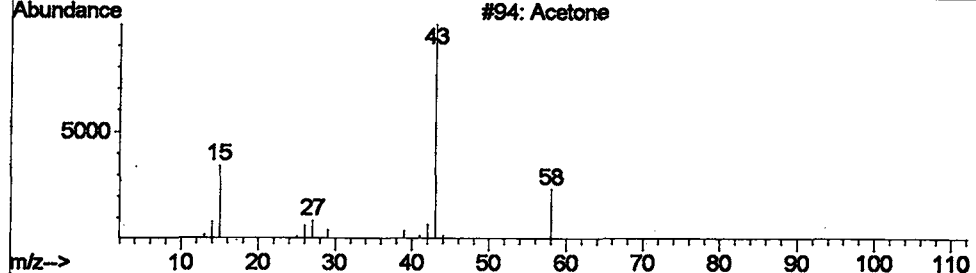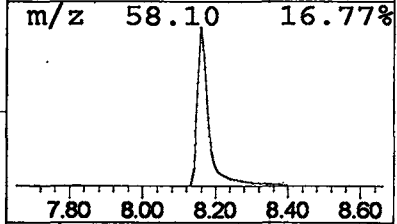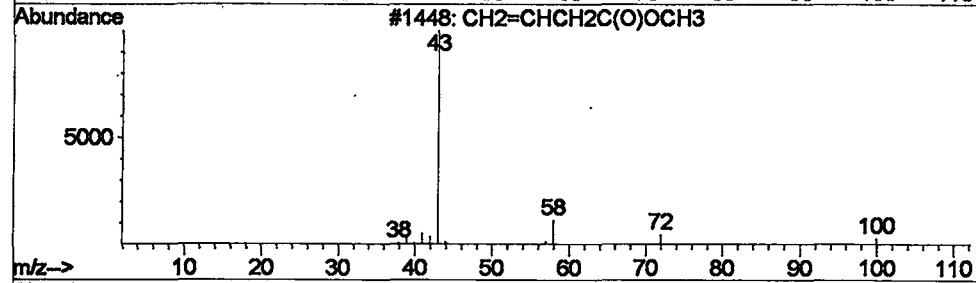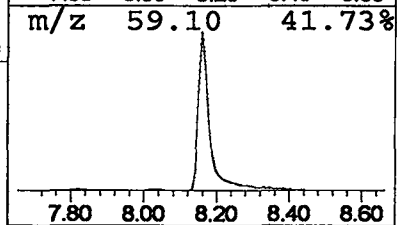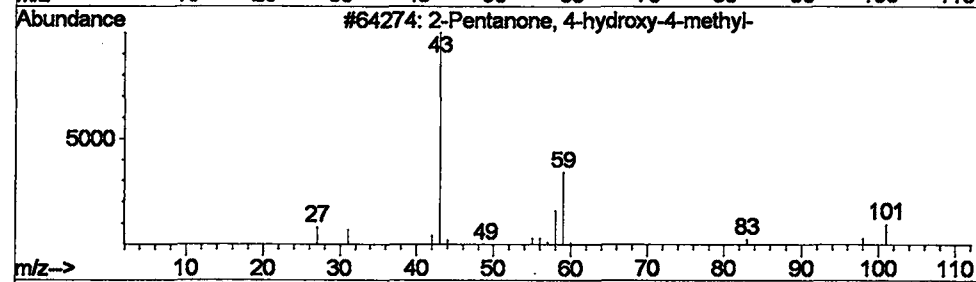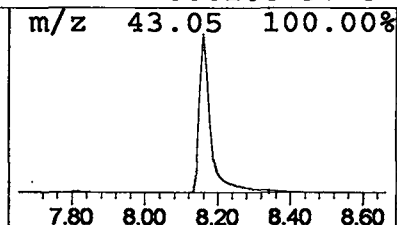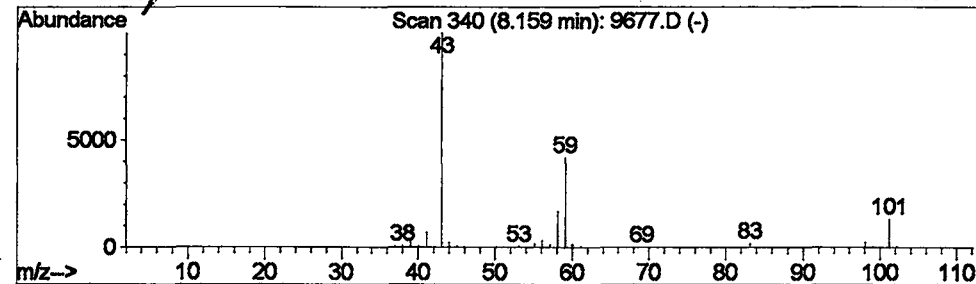

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 7 May 2002 10:54 am
 Data File: C:\HPCHEM\1\DATA\MAY0602\9677.D
 Name: GC/MS SCAN 4/25
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.16	10.8	ug/l	1004030	ISTD01	12.19	3718090	40.0
9677.D GCMS0501.M	Thu May 09 11:25:19 2002							