

Method 508 mod

Date Extracted 5/22/02

Page 139

~~#~~GCM5-18705

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500 mL		1 mL			1 mL	8A	7			
Ref 1					1 mL			8B				
Ref 2					1 mL			7A				
12152								6A				
12153								6B				
12154	FB							4B				
12155								7B				
12156								4A				
12157								2A				
12158								3A				
12159								3B				
12160								2B				
Remarks												
Reviewed by: <i>CB</i> 8/23/02												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type - SEP. Fun.		Solv. lot#	X07E07		NaCl lot#		V39614		Na2SO4 lot#		V46648	
STANDARD	INT STD LOG#											
CALIBRATION	04300											
REF SPIKE	2297E											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	2284C (5/17/02)											
LPC												
ENDRIN/DDT												

Analyst AD / DM
revision 4/12/01

Verified by ly

Reviewed by _____
Date _____

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAY2402.S

Comment:

Operator: Morgan

Data Path: C:\HPCHEM\1\DATA\MAY2402\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

(X) Full Method

(X) Inject Anyway

() Reprocessing Only

() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------


1	Sample	1	DFTPP	GCMS0520	
2	Sample	2	CAL20	GCMS0520	
3	Sample	3	LB	GCMS0520	gc/ms scan 5/22
4	Sample	4	REF1	GCMS0520	gc/ms scan 5/22
5	Sample	5	REF2	GCMS0520	gc/ms scan 5/22
6	Sample	6	12152	GCMS0520	gc/ms scan 5/22
7	Sample	7	12153	GCMS0520	gc/ms scan 5/22
8	Sample	8	12154	GCMS0520	gc/ms scan 5/22
9	Sample	9	12155	GCMS0520	gc/ms scan 5/22
10	Sample	10	12156	GCMS0520	gc/ms scan 5/22
11	Sample	11	12157	GCMS0520	gc/ms scan 5/22
12	Sample	12	12158	GCMS0520	gc/ms scan 5/22
13	Sample	13	12159	GCMS0520	gc/ms scan 5/22
14	Sample	14	12160	GCMS0520	gc/ms scan 5/22
15	Sample	15	LBA	GCMS0520	gc/ms scan 5/21
16	Sample	16	REFA1	GCMS0520	gc/ms scan 5/21
17	Sample	17	REFA2	GCMS0520	gc/ms scan 5/21
18	Sample	18	12093	GCMS0520	gc/ms scan 5/21
19	Sample	19	12094	GCMS0520	gc/ms scan 5/21
20	Sample	20	12095	GCMS0520	gc/ms scan 5/21
21	Sample	21	12096	GCMS0520	gc/ms scan 5/21
22	Sample	22	12097	GCMS0520	gc/ms scan 5/21
23	Sample	23	12098	GCMS0520	gc/ms scan 5/21
24	Sample	24	12099	GCMS0520	gc/ms scan 5/21
25	Sample	25	12151	GCMS0520	gc/ms scan 5/21

fb

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY2402\DFTPP.D
 Acq On : 24 May 2002 3:32 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: Morgan
 Inst : 209
 Multiplr: 1.00

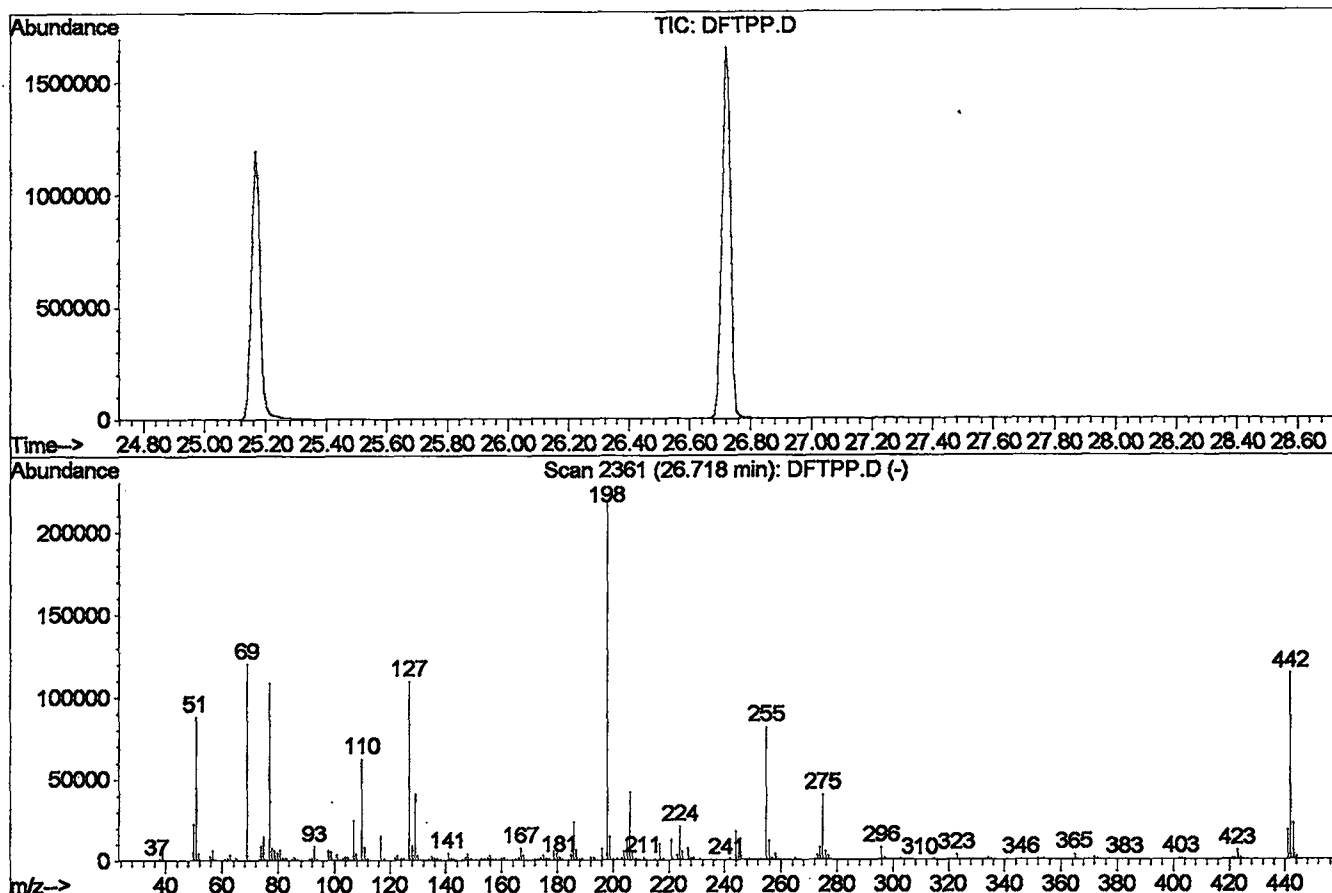

Spectrum Information: Scan 2361

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	40.3	88128	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	55.1	120584	PASS
70	69	0.00	2	0.4	492	PASS
127	198	40	60	50.1	109656	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	218816	PASS
199	198	5	9	6.8	14820	PASS
275	198	10	30	18.5	40496	PASS
365	198	1	100	1.6	3457	PASS
441	443	0.01	100	83.0	18528	PASS
442	198	40	110	52.1	114088	PASS
443	442	17	23	19.6	22336	PASS