

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 06/07/2002 Time: 09:16:02

Sample: AE12158
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 6/7/02 09:15 Ended: 6/7/02 09:15 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		89		10.0

Comments for Sample AE12158 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 06-07-2002 Time: 09:16:36

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 1 of the 43 compounds in the LCS Standard was low.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY2402\12158.D

Vial: 12

Acq On : 25 May 2002 2:23 am

Operator: Morgan

Sample : gc/ms scan 5/22

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 28 12:00 2002

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Tue May 28 11:39:13 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0520

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.14	152	499197	40.00	ug/l	0.00
10) Naphthalene-d8	15.77	136	1970064	40.00	ug/l	-0.02
17) Acenaphthene-d10	21.08	164	936738	40.00	ug/l	0.00
30) Phenanthrene-d10	25.51	188	1332302	40.00	ug/l	-0.02
38) Chrysene-d12	33.58	240	717355	40.00	ug/l	-0.03
44) Perylene-d12	37.78	264	474574	40.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.22	209	167154	35.50	ug/L	-0.01
Spiked Amount	40.000		Recovery	=	88.75%	

Target Compounds

					Qvalue
2) N-nitrosodimethylamine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	12.13	146	333	N.D.	
5) 1,4-Dichlorobenzene	12.13	146	333	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.58	149	431	N.D.	
26) 4-Chlorophenylphenylether	23.22	204	1174	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	23.22	168	397	N.D.	
32) 4-Bromophenylphenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.52	178	513	N.D.	

(#) = qualifier out of range (m) = manual integration

12158.D GCMS0520.M Tue May 28 12:01:21 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY2402\12158.D
Acq On : 25 May 2002 2:23 am
Sample : gc/ms scan 5/22
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 28 12:00 2002

Vial: 12
Operator: Morgan
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Tue May 28 11:39:13 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0520

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.52	178	513		N.D.	
36) Di-n-butylphthalate	27.50	149	2078		N.D.	
37) Fluoranthene	0.00	202	0		N.D.	
39) Pyrene	0.00	202	0		N.D.	
40) Butylbenzylphthalate	0.00	149	0		N.D.	
41) Benzo(a)anthracene	33.58	228	1564		N.D.	
42) Bis(2-ethylhexyl)phthalate	33.80	149	540		N.D.	
43) Chrysene	33.58	228	1564		N.D.	
45) Di-n-Octylphthalate	0.00	149	0		N.D.	
46) Benzo(b)fluoranthene	0.00	252	0		N.D.	
47) Benzo(k)fluoranthene	0.00	252	0		N.D.	
48) Benzo(a)pyrene	37.80	252	1766		N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0		N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0		N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0		N.D.	

(#) = qualifier out of range (m) = manual integration

12158.D GCMS0520.M Tue May 28 12:01:22 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY2402\12158.D
 Acq On : 25 May 2002 2:23 am
 Sample : gc/ms scan 5/22
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 28 12:00 2002

Vial: 12
 Operator: Morgan
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0520.RES

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue May 28 11:39:13 2002
 Response via : Initial Calibration

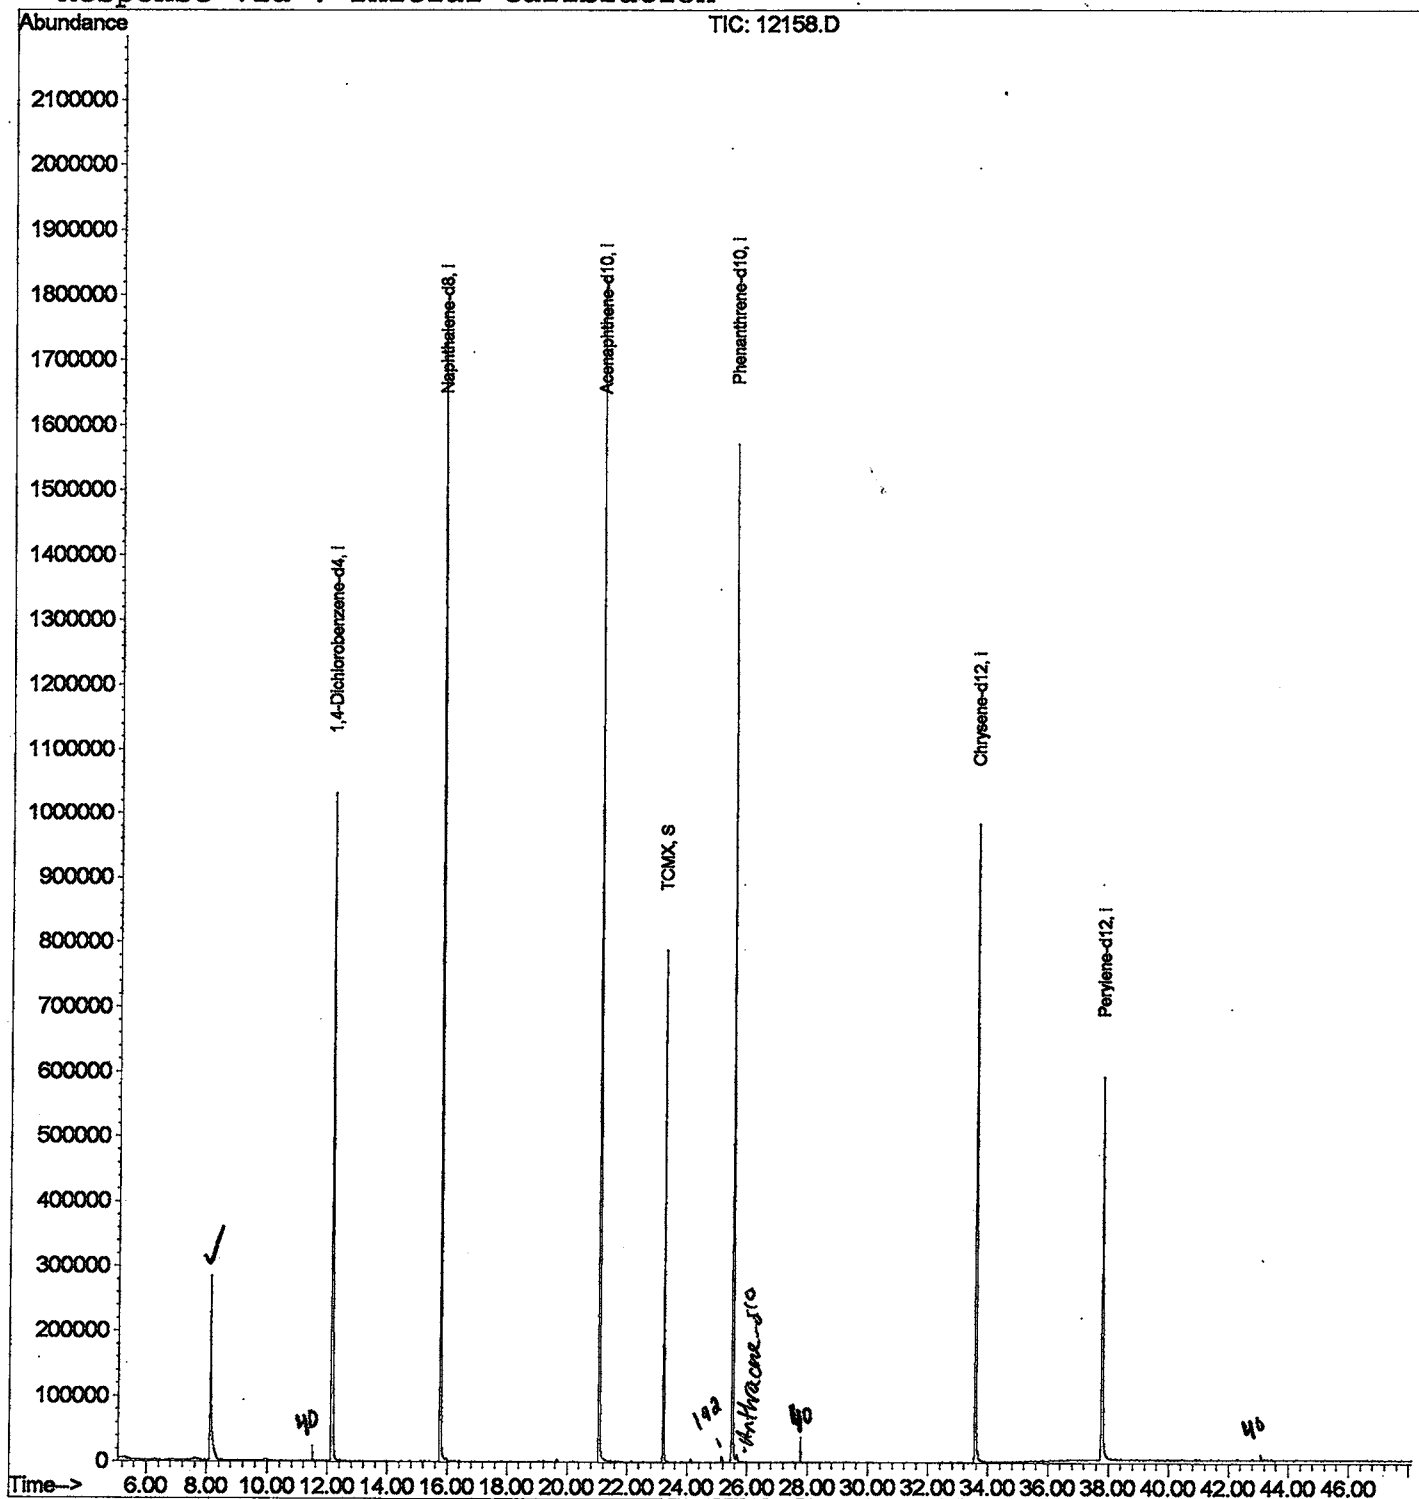

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY2402\12158.D
Acq On : 25 May 2002 2:23 am
Sample : gc/ms scan 5/22
Misc :
MS Integration Params: LSCINT.P

Vial: 12
Operator: Morgan
Inst : 209
Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.118	331	335	367	rVB	283060	797607	21.45%	4.003%
2	12.139	767	773	788	rBV	1031575	2716338	73.04%	13.632%
3	15.774	1163	1169	1187	rBV	1779594	3652354	98.21%	18.329%
4	21.081	1741	1747	1761	rBV	1830801	3718814	100.00%	18.662%
5	23.220	1972	1980	1988	rBV	787353	1601302	43.06%	8.036%
6	25.515	2224	2230	2242	rBV2	1569410	3412482	91.76%	17.125%
7	33.575	3101	3108	3123	rBV2	982219	2257676	60.71%	11.330%
8	37.789	3559	3567	3582	rBV2	588452	1770193	47.60%	8.883%




Sum of corrected areas: 19926766

12158.D GCMS0520.M

Tue May 28 12:05:00 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY2402\12158.D
 Operator : Morgan
 Acquired : 25 May 2002 2:23 am using AcqMethod GCMS0520
 Instrument : 209
 Sample Name: gc/ms scan 5/22
 Misc Info :
 Vial Number: 12
 Quant File :GCMS0520.RES (RTE Integrator)

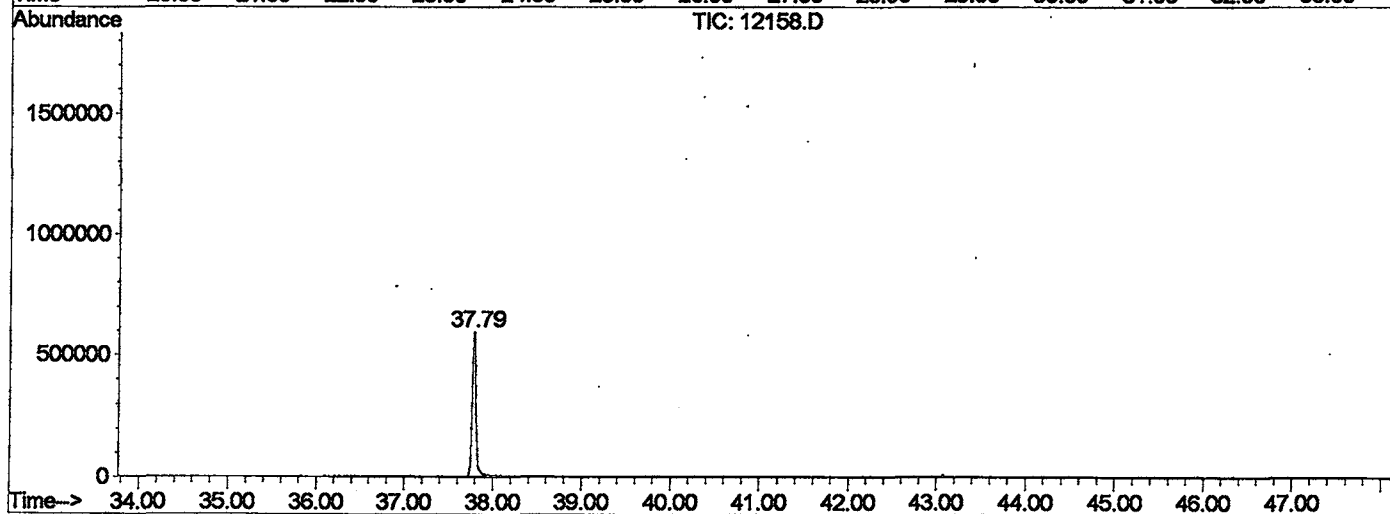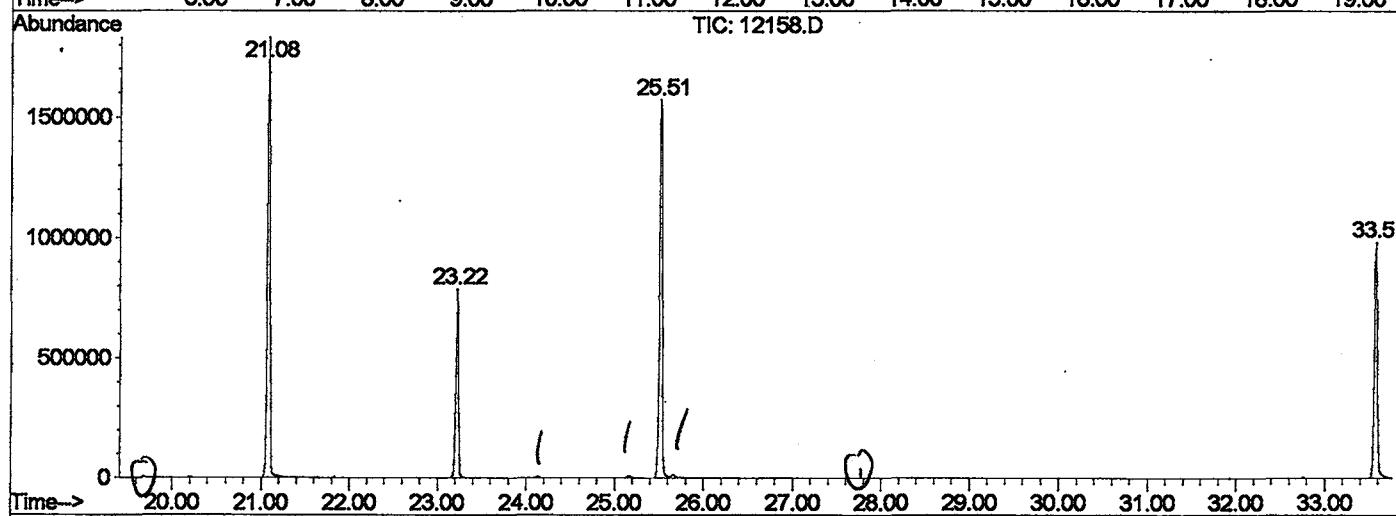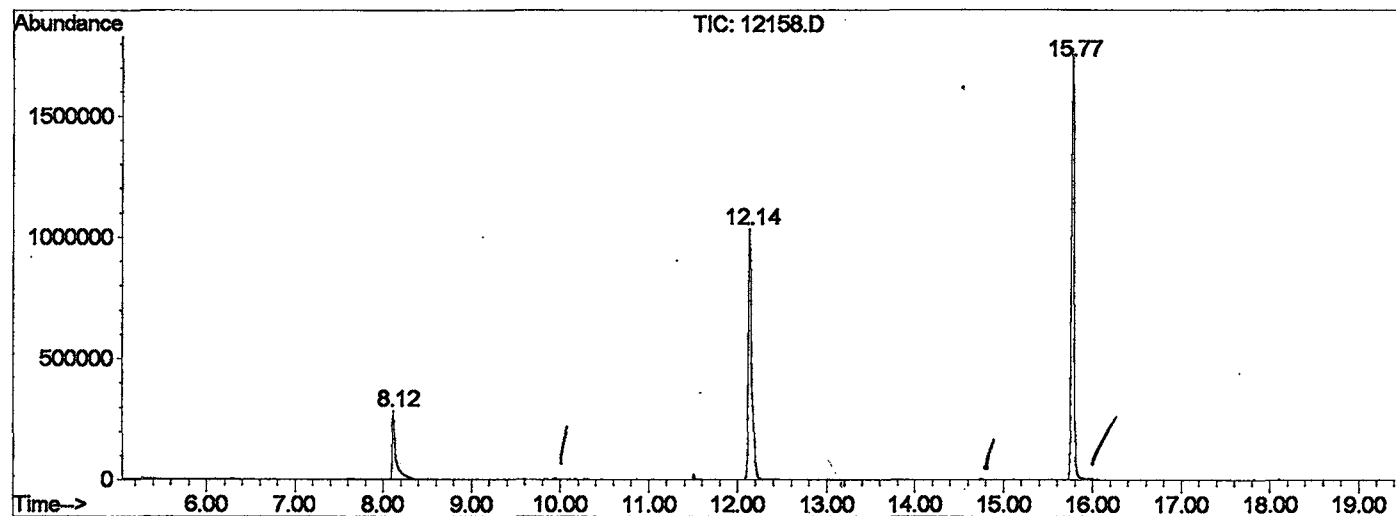

12158.D GCMS0520.M Tue May 28 12:05:00 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY2402\12158.D
 Acq On : 25 May 2002 2:23 am
 Sample : gc/ms scan 5/22
 Misc :
 MS Integration Params: LSCINT.P










Vial: 12
 Operator: Morgan
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.12	11.75 ug/l	797607	1,4-Dichlorobenzene-d4	12.14

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78
2		Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	25
3		Acetone	58	C3H6O	000067-64-1	16
4		Formamide, N,N-diethyl-	101	C5H11NO	000617-84-5	12

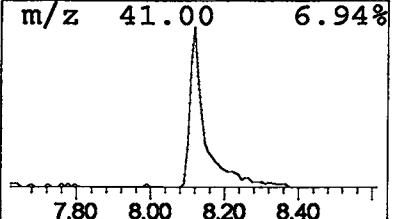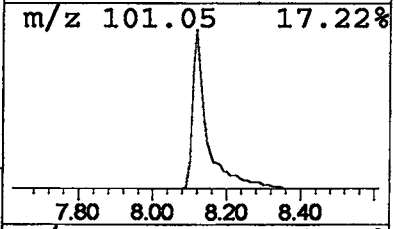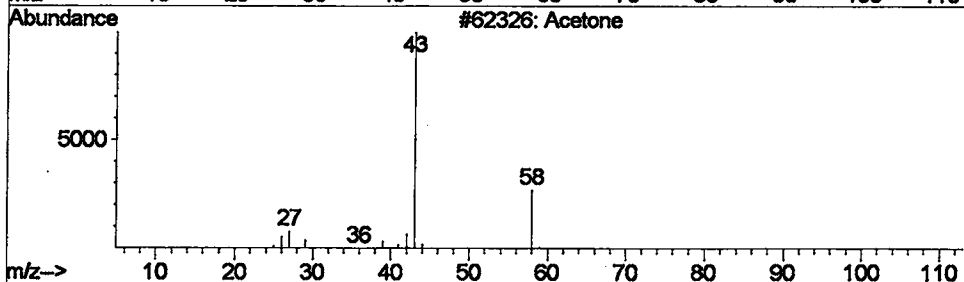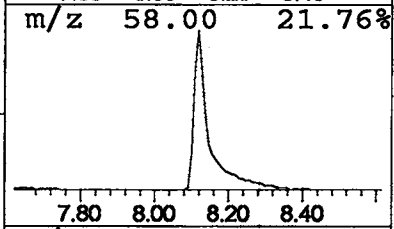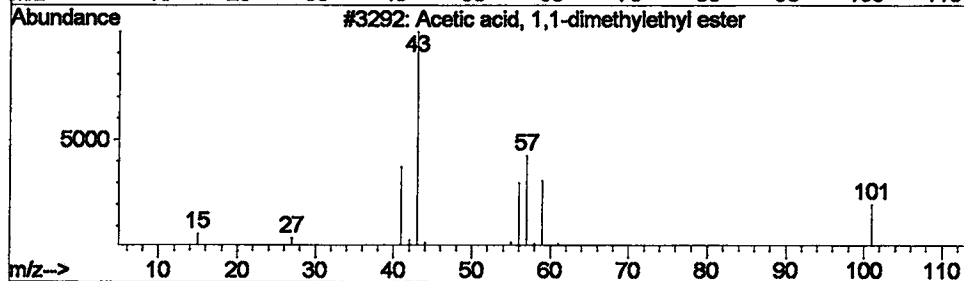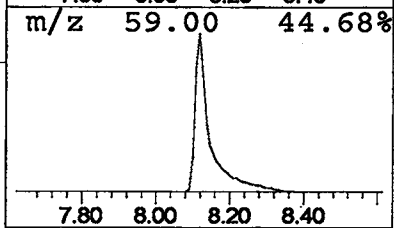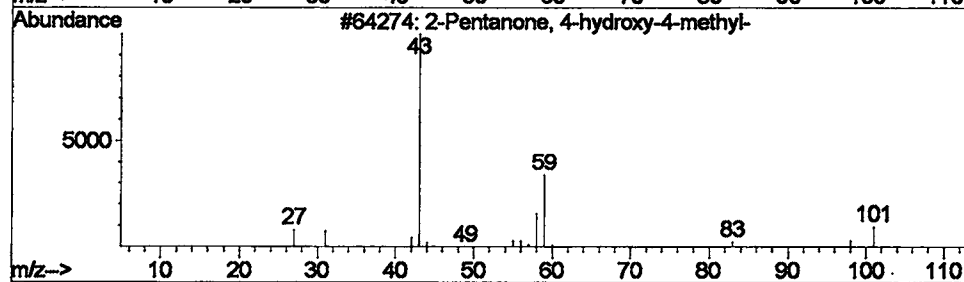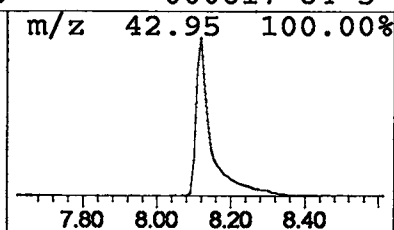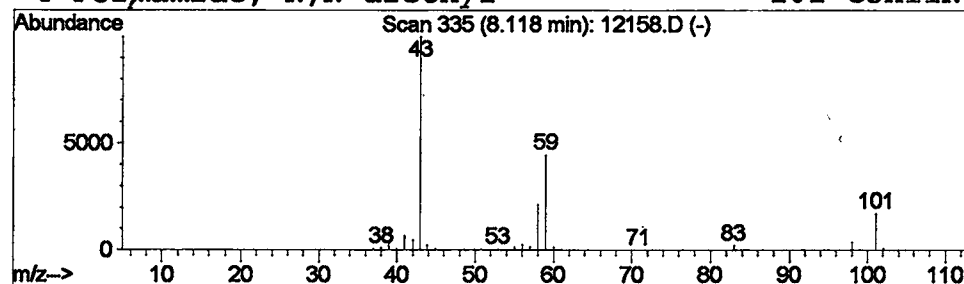

Tentatively Identified Compound (LSC) summary

Operator ID: Morgan Date Acquired: 25 May 2002 2:23 am
Data File: C:\HPCHEM\1\DATA\MAY2402\12158.D
Name: gc/ms scan 5/22
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.12	11.7	ug/l	797607	ISTD01	12.14	2716340	40.0

12158.D GCMS0520.M Tue May 28 12:05:01 2002