

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 06/07/2002 Time: 09:17:43

Sample: AE12159
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 6/7/02 09:16 Ended: 6/7/02 09:16 Analyst: DLV
 Page: 1

	Component Name	Vol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		86		10.0

Comments for Sample AE12159 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 06-07-2002 Time: 09:18:12

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 1 of the 43 compounds in the LCS Standard was low.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY2402\12159.D
 Acq On : 25 May 2002 3:22 am
 Sample : gc/ms scan 5/22
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 28 12:01 2002

Vial: 13
 Operator: Morgan
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue May 28 11:39:13 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0520

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.14	152	550091	40.00	ug/l	0.00
10) Naphthalene-d8	15.77	136	2197236	40.00	ug/l	-0.02
17) Acenaphthene-d10	21.09	164	1057511	40.00	ug/l	0.00
30) Phenanthrene-d10	25.53	188	1505967	40.00	ug/l	0.00
38) Chrysene-d12	33.60	240	784306	40.00	ug/l	0.00
44) Perylene-d12	37.82	264	522437	40.00	ug/l	0.02

System Monitoring Compounds

28) TCMX	23.23	209	182993	34.43	ug/L	0.00
Spiked Amount	40.000		Recovery	=	86.08%	

Target Compounds

					Qvalue
2) N-nitrosodimethylamine	5.42	74	467	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	12.14	146	437	N.D.	
5) 1,4-Dichlorobenzene	12.14	146	437	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.83	128	380	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.56	149	410	N.D.	
26) 4-Chlorophenylphenylether	23.23	204	1267	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	23.23	168	429	N.D.	
32) 4-Bromophenylphenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.53	178	639	N.D.	

(#) = qualifier out of range (m) = manual integration

12159.D GCMS0520.M Tue May 28 12:02:12 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY2402\12159.D

Vial: 13

Acq On : 25 May 2002 3:22 am

Operator: Morgan

Sample : gc/ms scan 5/22

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 28 12:01 2002

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Tue May 28 11:39:13 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0520

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.53	178	639		N.D.	
36) Di-n-butylphthalate	27.51	149	1672		N.D.	
37) Fluoranthene	0.00	202	0		N.D.	
39) Pyrene	0.00	202	0		N.D.	
40) Butylbenzylphthalate	0.00	149	0		N.D.	
41) Benzo(a)anthracene	33.60	228	1850		N.D.	
42) Bis(2-ethylhexyl)phthalate	33.83	149	1207		N.D.	
43) Chrysene	33.60	228	1850		N.D.	
45) Di-n-Octylphthalate	0.00	149	0		N.D.	
46) Benzo(b)fluoranthene	0.00	252	0		N.D.	
47) Benzo(k)fluoranthene	0.00	252	0		N.D.	
48) Benzo(a)pyrene	37.82	252	1965		N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0		N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0		N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0		N.D.	

 (#) = qualifier out of range (m) = manual integration

12159.D GCMS0520.M

Tue May 28 12:02:13 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY2402\12159.D
Acq On : 25 May 2002 3:22 am
Sample : gc/ms scan 5/22
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 28 12:01 2002

Vial: 13
Operator: Morgan
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0520.RES

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Tue May 28 11:39:13 2002
Response via : Initial Calibration

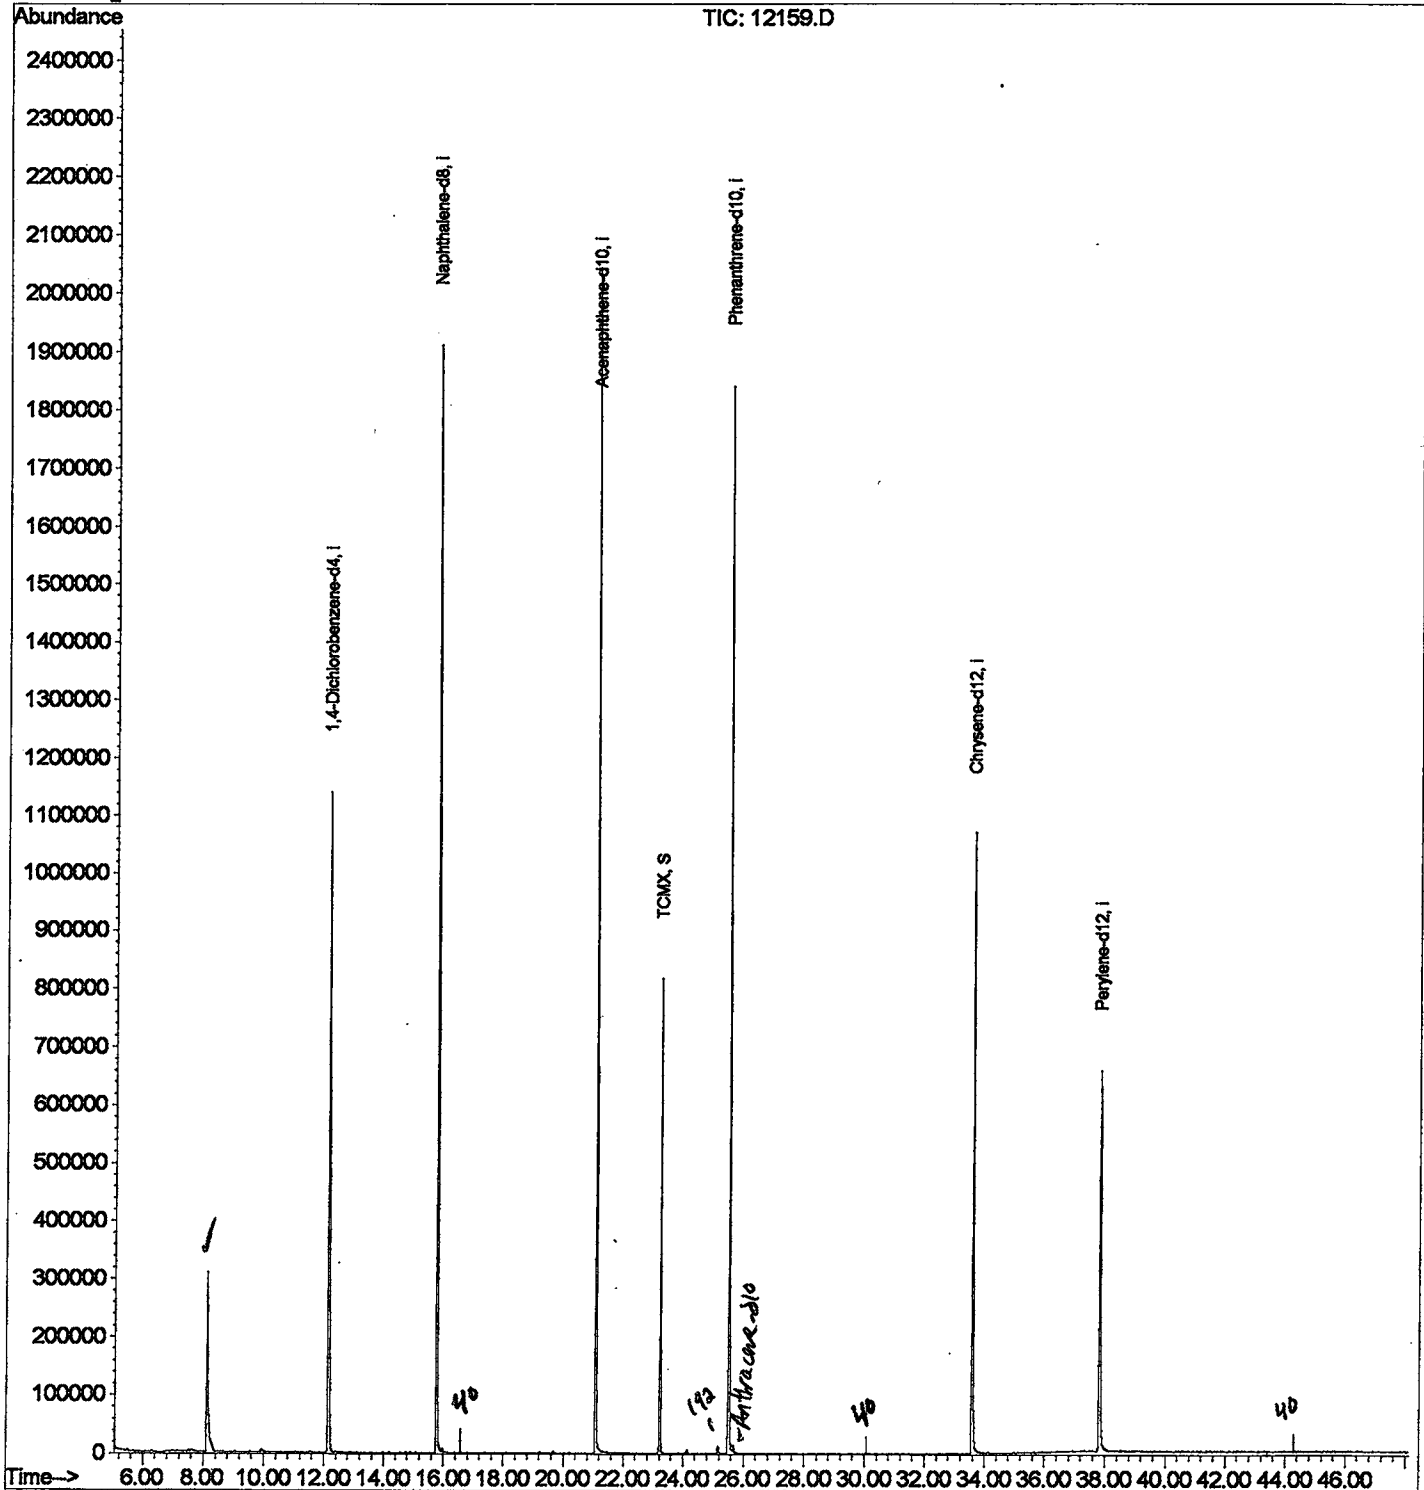

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY2402\12159.D
 Acq On : 25 May 2002 3:22 am
 Sample : gc/ms scan 5/22
 Misc :
 MS Integration Params: LSCINT.P

Vial: 13
 Operator: Morgan
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.115	330	334	365	rVB	309160	879752	21.05%	3.978%
2	12.136	767	772	787	rBV	1139077	3018025	72.22%	13.646%
3	15.771	1163	1168	1182	rBV	1909454	4049328	96.89%	18.309%
4	21.086	1741	1747	1767	rBV	2041376	4179136	100.00%	18.896%
5	23.235	1973	1981	1986	rBV	817067	1715156	41.04%	7.755%
6	25.530	2220	2231	2243	rBV2	1841390	3853976	92.22%	17.425%
7	33.599	3103	3110	3123	rBV2	1069671	2465537	59.00%	11.148%
8	37.822	3562	3570	3590	rBV2	655110	1956041	46.80%	8.844%




Sum of corrected areas: 22116951

12159.D GCMS0520.M

Tue May 28 12:05:09 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY2402\12159.D
 Operator : Morgan
 Acquired : 25 May 2002 3:22 am using AcqMethod GCMS0520
 Instrument : 209
 Sample Name: gc/ms scan 5/22
 Misc Info :
 Vial Number: 13
 Quant File : GCMS0520.RES (RTE Integrator)

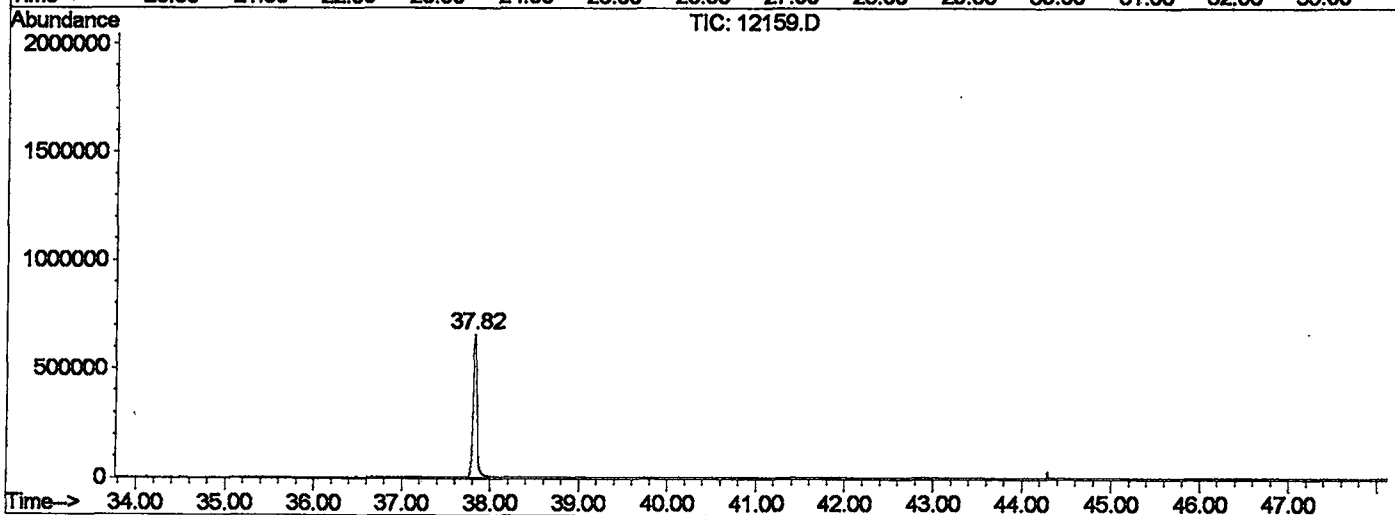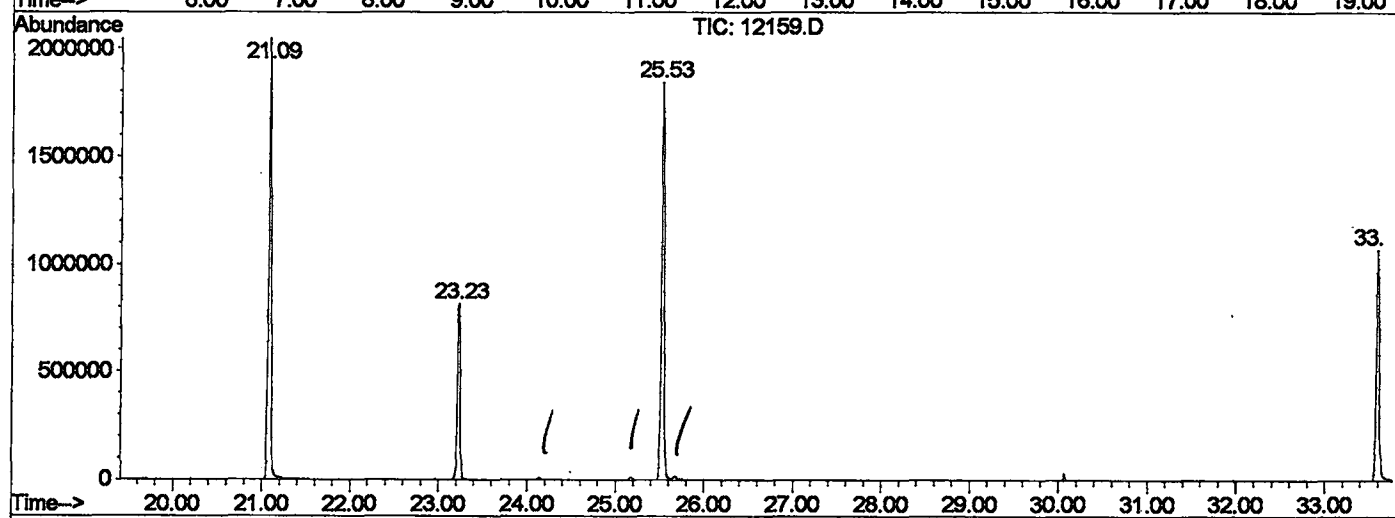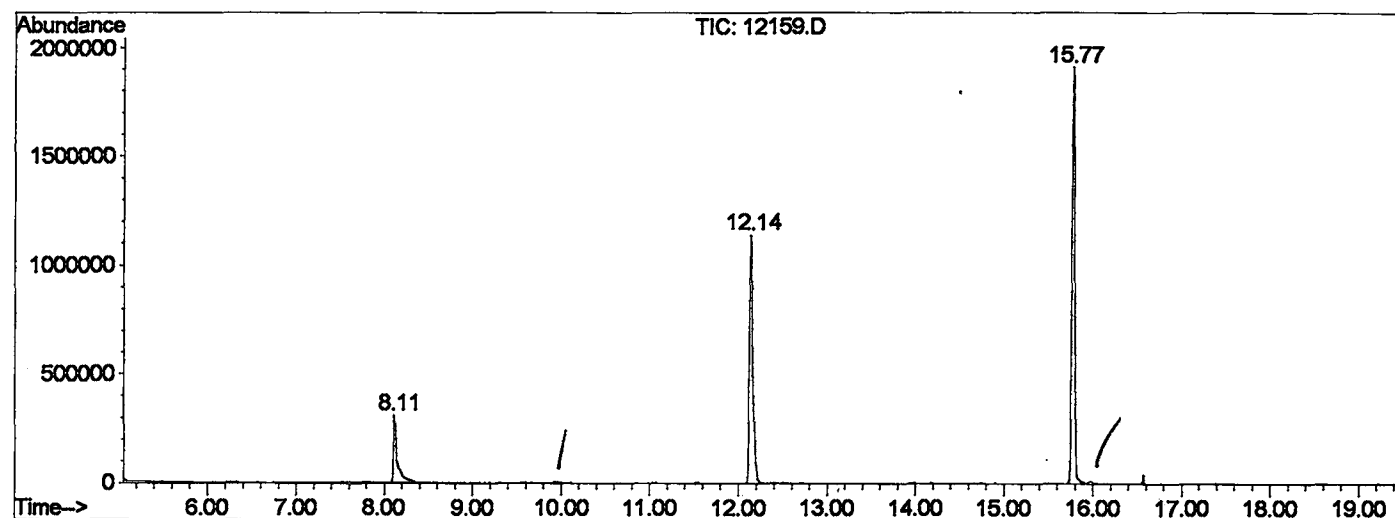

12159.D GCMS0520.M Tue May 28 12:05:10 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY2402\12159.D
Acq On : 25 May 2002 3:22 am
Sample : gc/ms scan 5/22
Misc :
MS Integration Params: LSCINT.P

Vial: 13
Operator: Morgan
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)









Title : 209 625/TCLP calibration table

Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.11	11.66 ug/l	879752	1,4-Dichlorobenzene-d4	12.14

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78	
2	Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	25	
3	Acetone	58	C3H6O	000067-64-1	16	
4	Formamide, N,N-diethyl-	101	C5H11NO	000617-84-5	12	

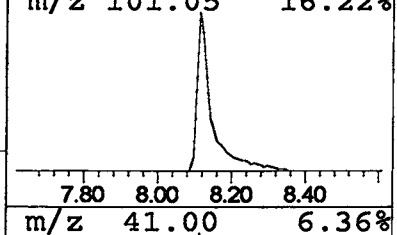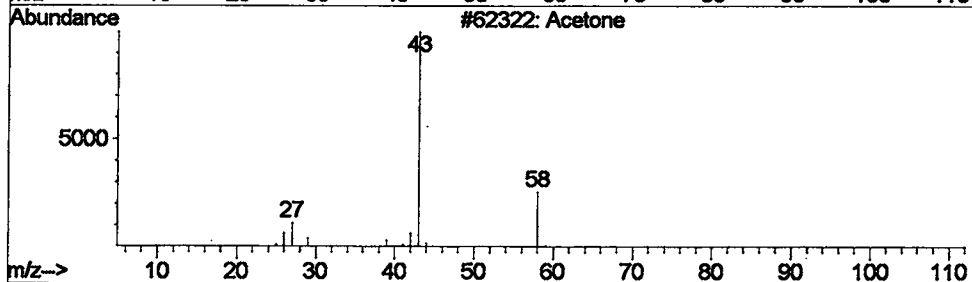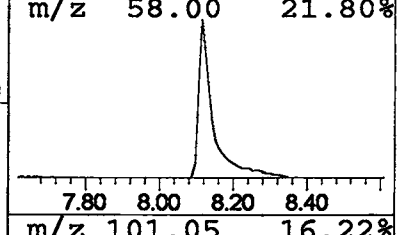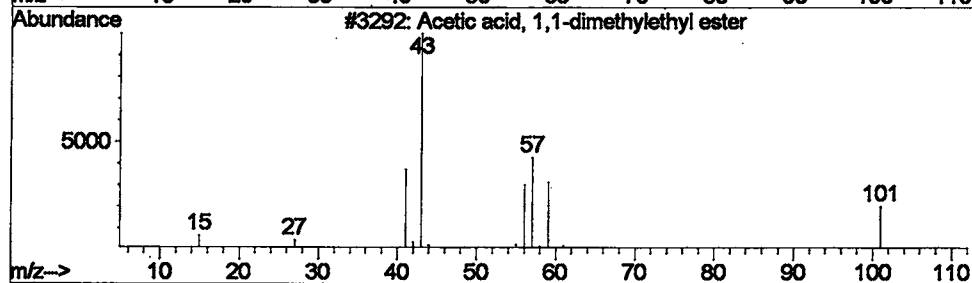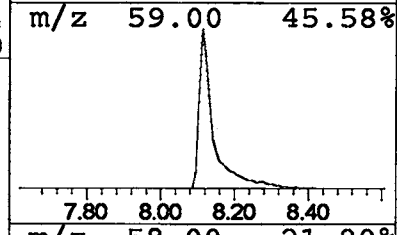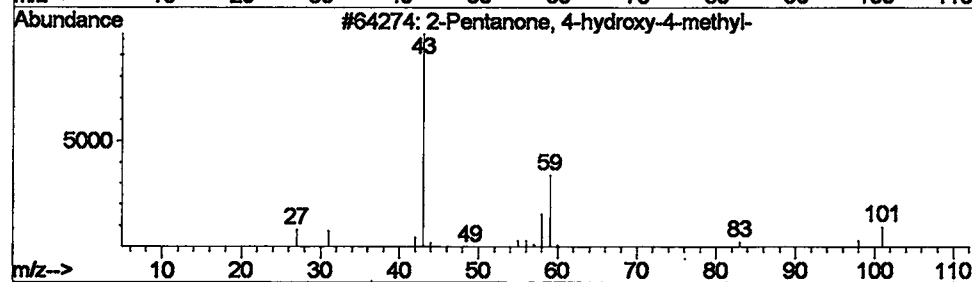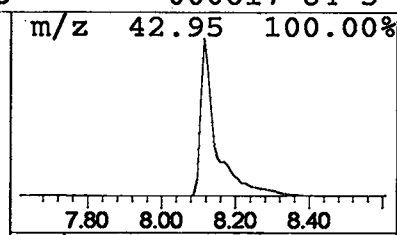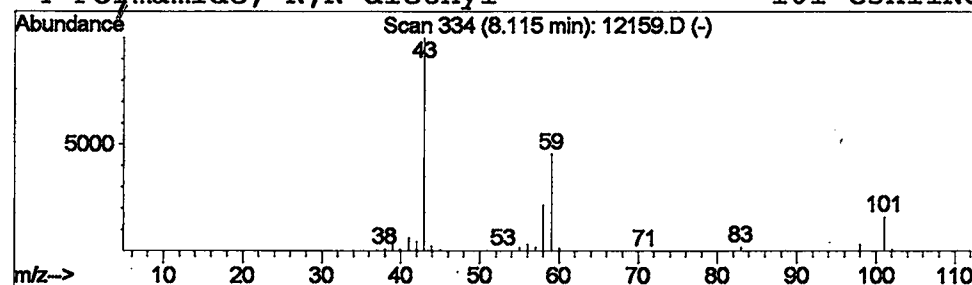

Tentatively Identified Compound (LSC) summary

Operator ID: Morgan Date Acquired: 25 May 2002 3:22 am
Data File: C:\HPCHEM\1\DATA\MAY2402\12159.D
Name: gc/ms scan 5/22
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.11	11.7	ug/l	879752	ISTD01	12.14	3018030	40.0

12159.D GCMS0520.M Tue May 28 12:05:11 2002