

Method 508 mod

Date Extracted 5-23-02

Page 141

NY

#GCM5-13729

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500 ml		1M			1M	8A	7			
12163					1M			8B				
12164								7A				
12165								2B				
12166	FB							4A				
12168								6B				
12169								7B				
12170	FB							2A				
12223								6A				
12224	see 5/31							1A				
12225								3A				
								4B				
								3B				
Remarks												
Reviewed by <u>C/B 8/23/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type <u>SEP Fun</u>		Solv. lot# <u>X07E07</u>		NaCl lot# <u>V39614</u>		Na2SO4 lot# <u>V46648</u>						
STANDARD	INT STD LOG#											
CALIBRATION	<u>043002</u>											
REF/SPIKE	<u>2297E</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>052802</u>											
SURROGATE	<u>TCMX 2284E 5/22/02</u>											
LPC												
ENDRIN/DDT												

Analyst
revision 4/12/01


Verified by ny

Reviewed by DN 6/3/02

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY2902\DFTPP1.D
 Acq On : 29 May 2002 11:19 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0528.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: Morgan
 Inst : 209
 Multiplr: 1.00

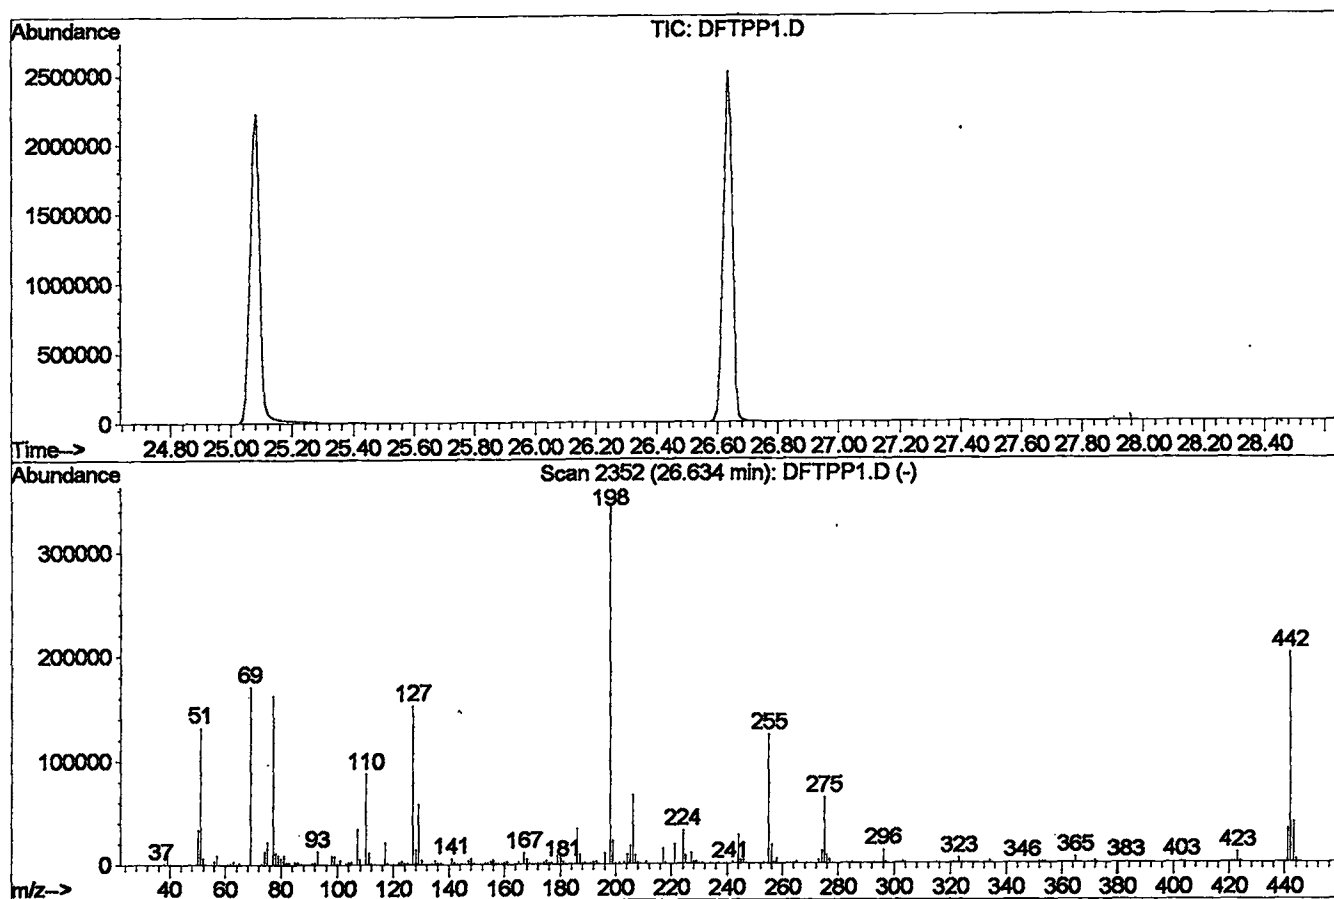

Spectrum Information: Scan 2352

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	38.2	132160	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.5	171392	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	44.4	153664	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	346368	PASS
199	198	5	9	6.8	23448	PASS
275	198	10	30	18.7	64624	PASS
365	198	1	100	1.7	5846	PASS
441	443	0.01	100	83.7	33312	PASS
442	198	40	110	58.4	202368	PASS
443	442	17	23	19.7	39784	PASS

DFTPP1.D GCMS0528.M Thu May 30 08:52:30 2002