

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 06/07/2002 Time: 14:10:24

Sample: AE12538
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 6/7/02 14:09 Ended: 6/7/02 14:09 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		78		10.0

Comments for Sample AE12538 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 06-07-2002 Time: 14:10:49

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JUN0302\12538.D
 Acq On : 4 Jun 2002 2:57 am
 Sample : gc/ms scan 5/28
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Jun 4 11:44 2002

Vial: 19
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0531.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri May 31 09:43:55 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0531

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.07	152	442698	40.00	ug/l	0.00
10) Naphthalene-d8	15.70	136	1787159	40.00	ug/l	-0.02
17) Acenaphthene-d10	20.99	164	856487	40.00	ug/l	0.00
30) Phenanthrene-d10	25.43	188	1321350	40.00	ug/l	0.00
38) Chrysene-d12	33.47	240	756761	40.00	ug/l	-0.03
44) Perylene-d12	37.65	264	449179	40.00	ug/l	-0.03

System Monitoring Compounds

28) TCMX	23.13	209	184969	31.21	ug/L	-0.02
Spiked Amount	40.000		Recovery	=	78.03%	

Target Compounds

					Qvalue
2) N-nitrosodimethylamine	5.38	74	379	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.75	128	274	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.49	149	964	N.D.	
26) 4-Chlorophenylphenylether	23.13	204	1191	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	23.13	168	509	N.D.	
32) 4-Bromophenylphenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.43	178	425	N.D.	

(#) = qualifier out of range (m) = manual integration

12538.D GCMS0531.M Tue Jun 04 11:45:18 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JUN0302\12538.D
Acq On : 4 Jun 2002 2:57 am
Sample : gc/ms scan 5/28
Misc :
MS Integration Params: GOOFY.P
Quant Time: Jun 4 11:44 2002

Vial: 19
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0531.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri May 31 09:43:55 2002
Response via : Initial Calibration.
DataAcq Meth : GCMS0531

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
35) Anthracene	25.43	178	425	N.D.	
36) Di-n-butylphthalate	27.41	149	17836	0.37 ug/l #	98
37) Fluoranthene	29.13	202	267	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo(a)anthracene	33.47	228	1871	N.D.	
42) Bis(2-ethylhexyl)phthalate	33.71	149	1592	N.D.	
43) Chrysene	33.47	228	1871	N.D.	
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo(b)fluoranthene	0.00	252	0	N.D.	
47) Benzo(k)fluoranthene	0.00	252	0	N.D.	
48) Benzo(a)pyrene	37.64	252	1714	N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

12538.D GCMS0531.M

Tue Jun 04 11:45:19 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\JUN0302\12538.D
Acq On : 4 Jun 2002 2:57 am
Sample : gc/ms scan 5/28
Misc :
MS Integration Params: GOOFY.P
Quant Time: Jun 4 11:44 2002

Vial: 19
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0531.RES

Method : C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri May 31 09:43:55 2002
Response via : Initial Calibration

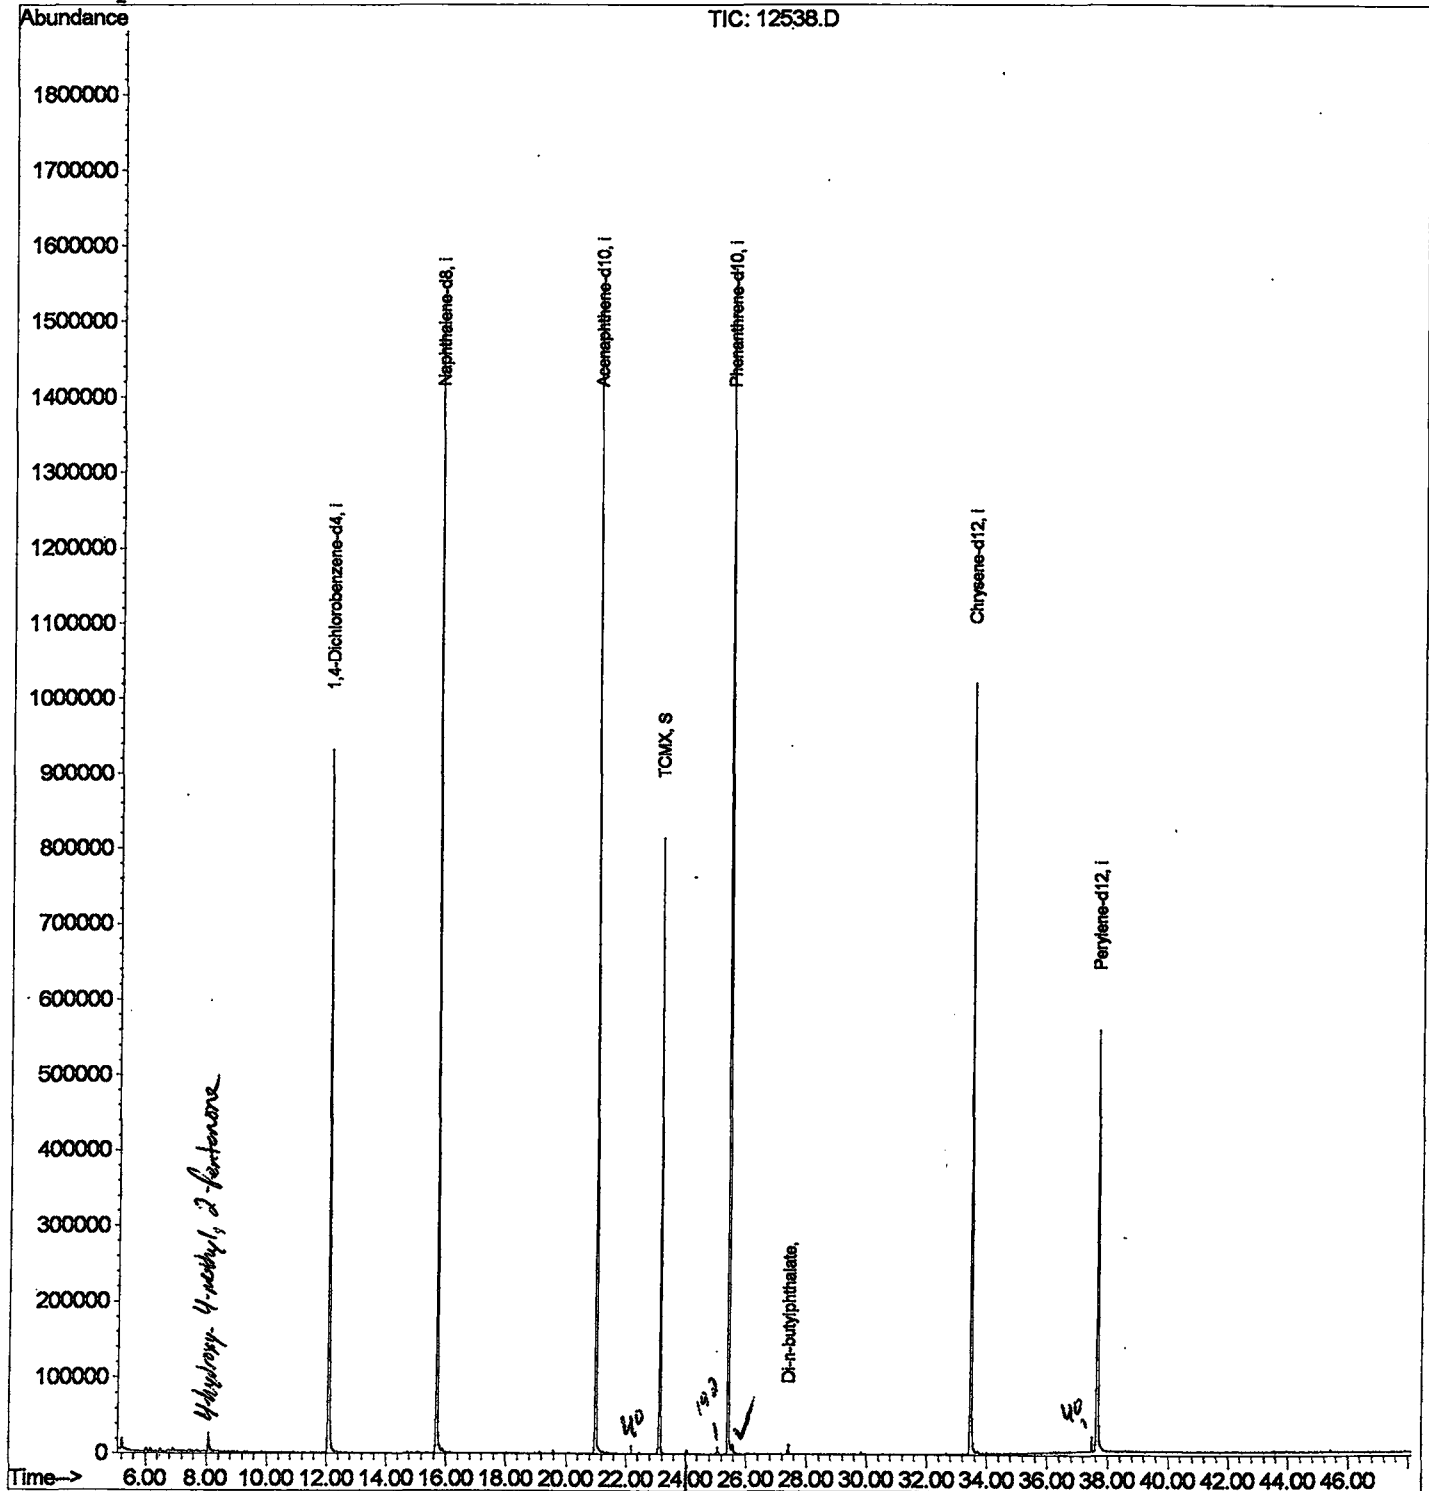

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\JUN0302\12538.D

Vial: 19

Acq On : 4 Jun 2002 2:57 am

Operator:

Sample : gc/ms scan 5/28

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.068	326	329	342	rBV	25333	67894	1.99%	0.370%
2	12.062	759	764	785	rBV	931386	2421307	70.89%	13.201%
3	15.697	1154	1160	1176	rBV	1518612	3300653	96.64%	17.995%
4	20.985	1730	1736	1757	rBV	1545997	3389457	99.24%	18.479%
5	23.133	1962	1970	1978	rBV	814652	1687685	49.41%	9.201%
6	25.428	2213	2220	2231	rBV2	1570057	3415424	100.00%	18.621%
7	25.566	2231	2235	2251	rVB2	12916	47127	1.38%	0.257%
8	33.470	3090	3096	3112	rBV2	1021454	2377288	69.60%	12.961%
9	37.647	3544	3551	3562	rBV2	555990	1635278	47.88%	8.915%




Sum of corrected areas: 18342113

12538.D GCMS0531.M

Tue Jun 04 11:52:05 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\JUN0302\12538.D
Operator :
Acquired : 4 Jun 2002 2:57 am using AcqMethod GCMS0531
Instrument : 209
Sample Name: gc/ms scan 5/28
Misc Info :
Vial Number: 19
Quant File : GCMS0531.RES (RTE Integrator)

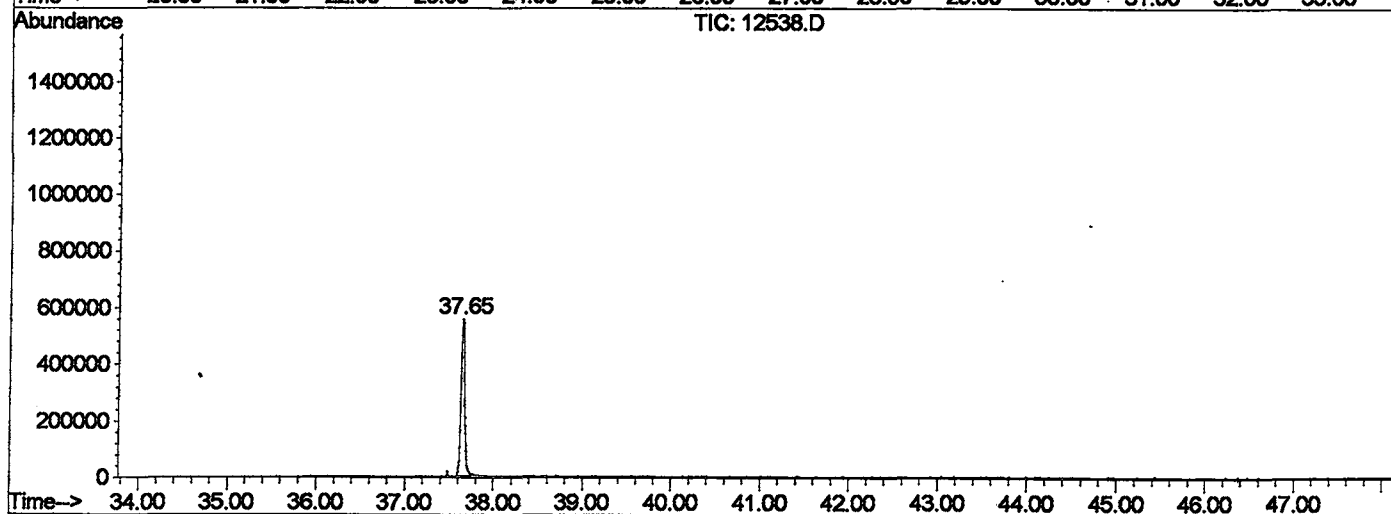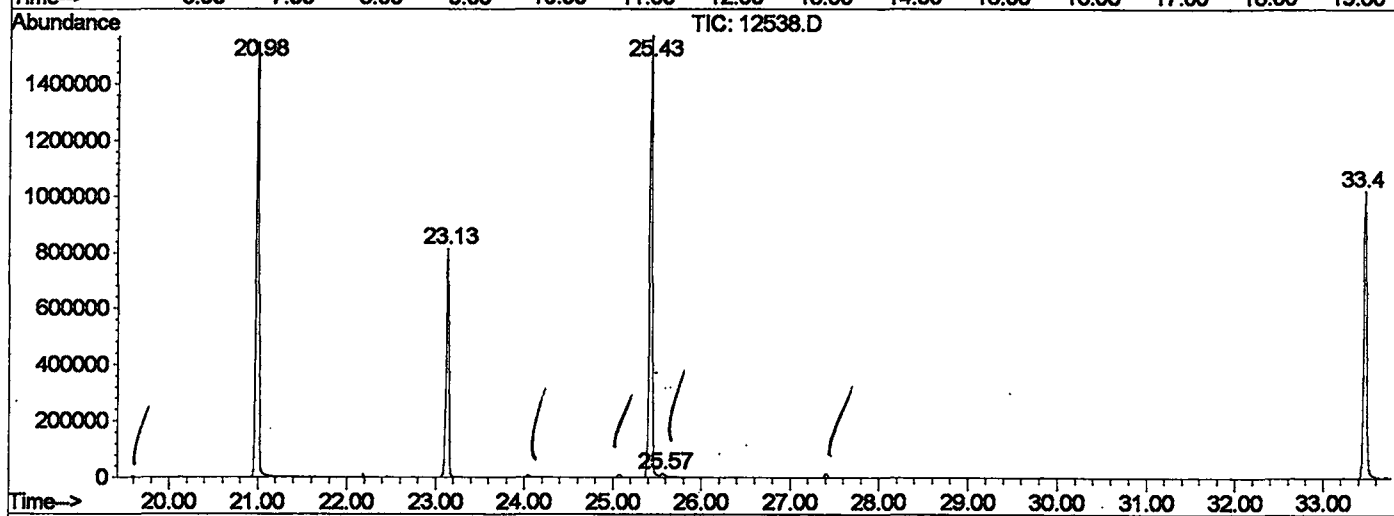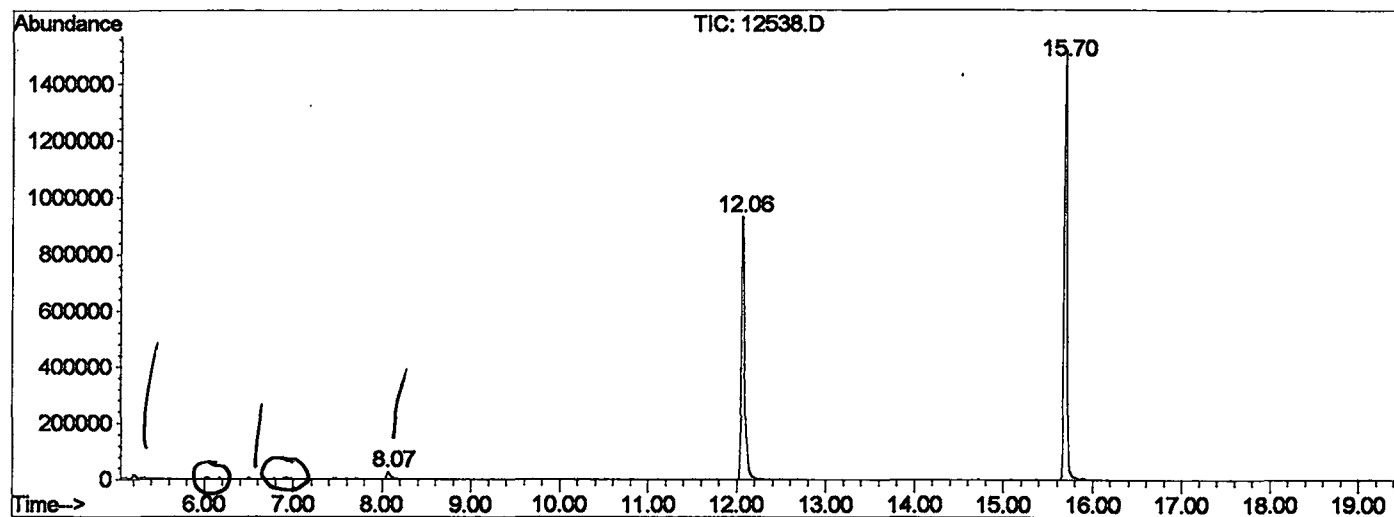

12538.D GCMS0531.M Tue Jun 04 11:52:05 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JUN0302\12538.D
Acq On : 4 Jun 2002 2:57 am
Sample : gc/ms scan 5/28
Misc :
MS Integration Params: LSCINT.P







Vial: 19
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.07	1.12 ug/l	67894	1,4-Dichlorobenzene-d4	12.07

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	83	
2	5-Hexen-2-one	98	C6H10O	000109-49-9	9	
3	Acetone	58	C3H6O	000067-64-1	9	
4	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9	

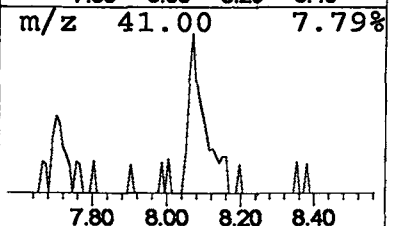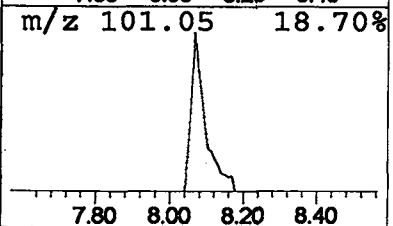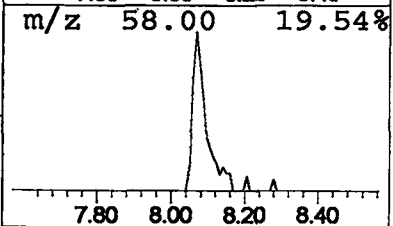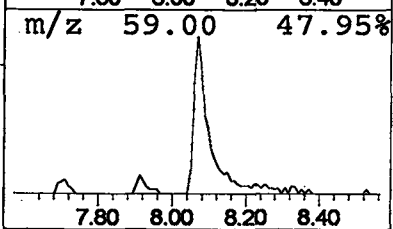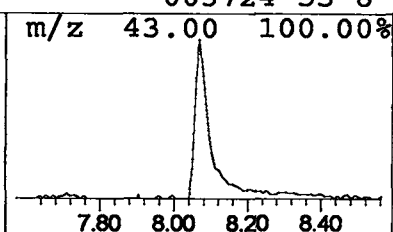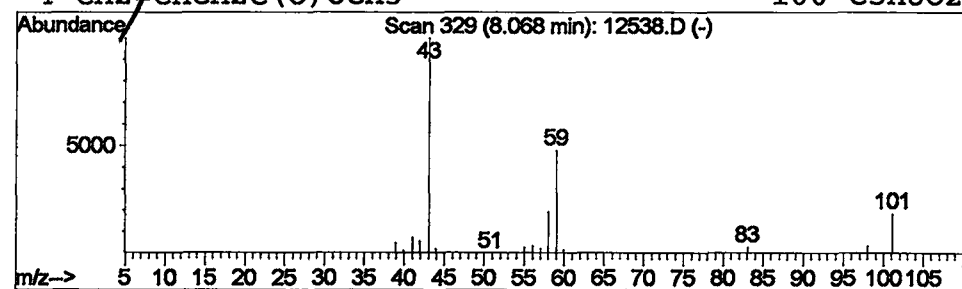

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JUN0302\12538.D
 Acq On : 4 Jun 2002 2:57 am
 Sample : gc/ms scan 5/28
 Misc :
 MS Integration Params: LSCINT.P


Vial: 19
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Phenanthrene-d10 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.57	0.55 ug/l	47127	Phenanthrene-d10	25.43

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Phenanthrene-d10	188	C14D10	001517-22-2	83
2		2-Quinolinecarboxaldehyde, 8-hydrox	188	C10H8N2O2	005603-22-5	42
3		4H-Pyrido[1,2-a]pyrimidin-4-one, 3-	188	C11H12N2O	057773-19-0	42
4		Naphthalene, 1,7-dimethoxy-	188	C12H12O2	005309-18-2	40

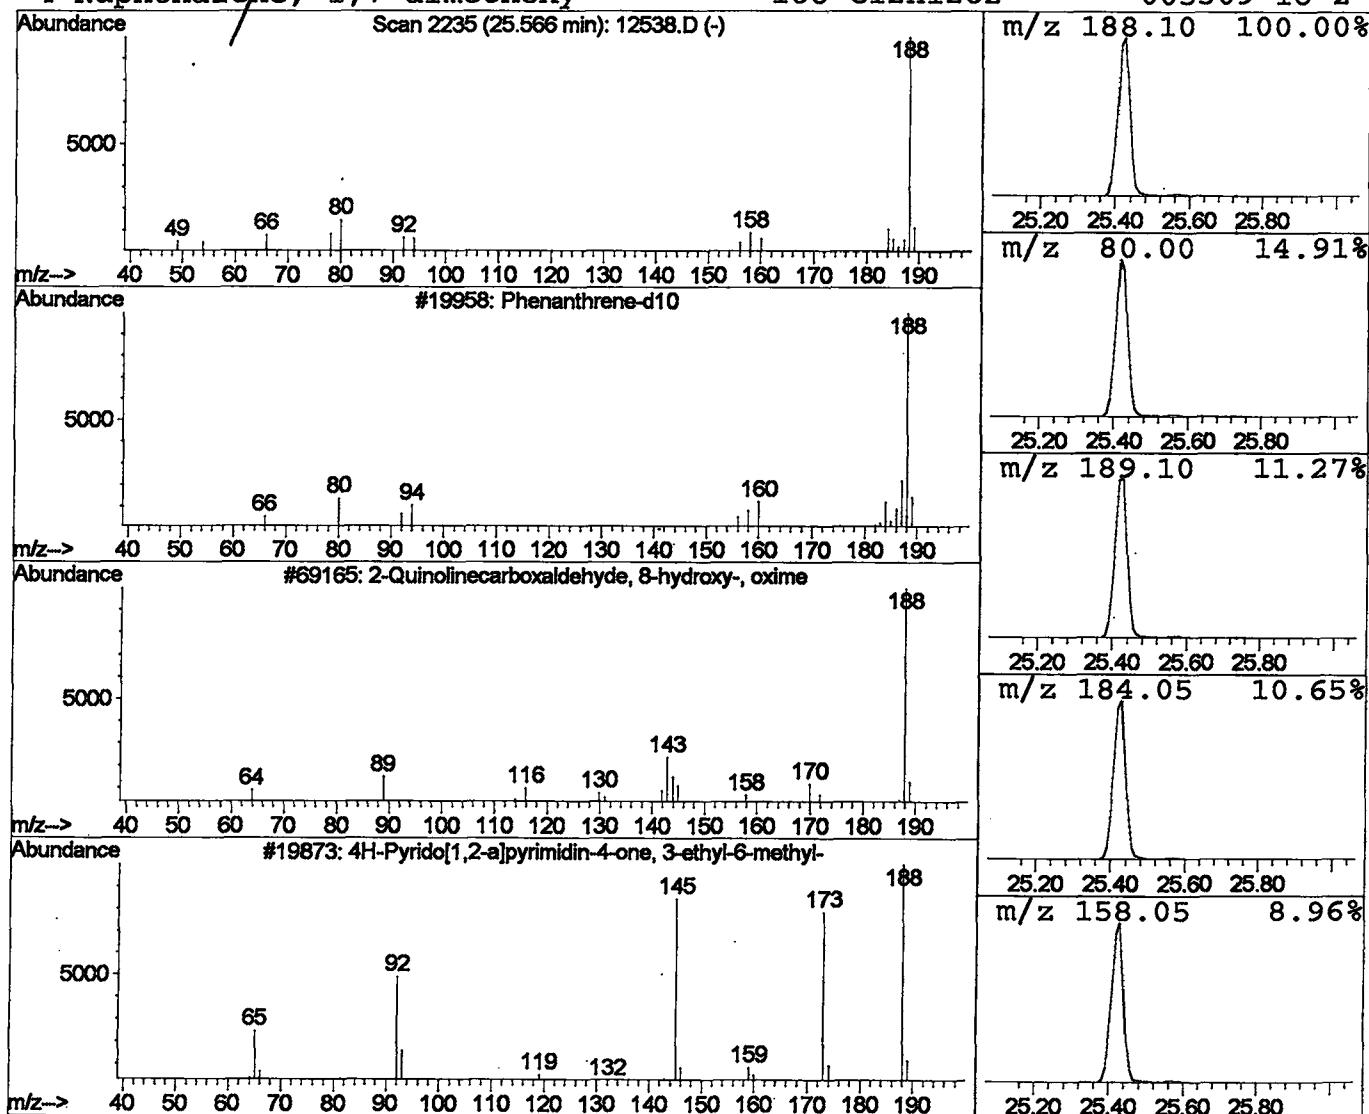

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 4 Jun 2002 2:57 am
Data File: C:\HPCHEM\1\DATA\JUN0302\12538.D
Name: gc/ms scan 5/28
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC / Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.07	1.1	ug/l	67894	ISTD01	12.07	2421310	40.0
Phenanthrene-d10	25.57	0.6	ug/l	47127	ISTD04	25.43	3415420	40.0

12538.D GCMS0531.M Tue Jun 04 11:52:07 2002