

Method 508 mod.

Date Extracted 5-29-02

Page 3

Ref

\$GCMS-18769

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
<u>LB</u>		<u>500ml</u>		<u>1ml</u>			<u>1ml</u>	<u>6B</u>	<u>7</u>			
<u>Ref</u>					<u>1ml</u>			<u>8A</u>				
<u>Ref</u>					<u>↓</u>			<u>7A</u>				
<u>120678</u>								<u>3A</u>				
<u>12099</u>	<u>FB</u>							<u>3B</u>				
<u>12151</u>								<u>2A</u>				
<u>12575</u>								<u>2B</u>				
<u>12576</u>								<u>7B</u>				
<u>12577</u>	<u>FB</u>							<u>8B</u>				
<u>12672</u>		<u>↓</u>		<u>↓</u>			<u>↓</u>	<u>6A</u>	<u>↓</u>			
Remarks Reviewed by, <u>CB 8/22/02</u> drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type <u>SEP Fun.</u> Solv. lot# <u>XD5E10</u> NaCl lot# <u>V46648</u> Na2SO4 lot# <u>V46648</u> STANDARD INT STD LOG# CALIBRATION <u>053102</u> <u>053002</u> REF/SPIKE <u>2297E</u> MDL/MDRF Q. CHECK INT. STD. <u>053102</u> SURROGATE <u>TCM X 2294 Q, R, S, E</u> <u>5/21/02</u> LPC ENDRIN/DDT												

Analyst B.H.
revision 4/12/01


Verified by my

Reviewed by DR
Date 6/6/02

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY3102\DFTPP.D
 Acq On : 31 May 2002 11:56 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: Morgan
 Inst : 209
 Multiplr: 1.00

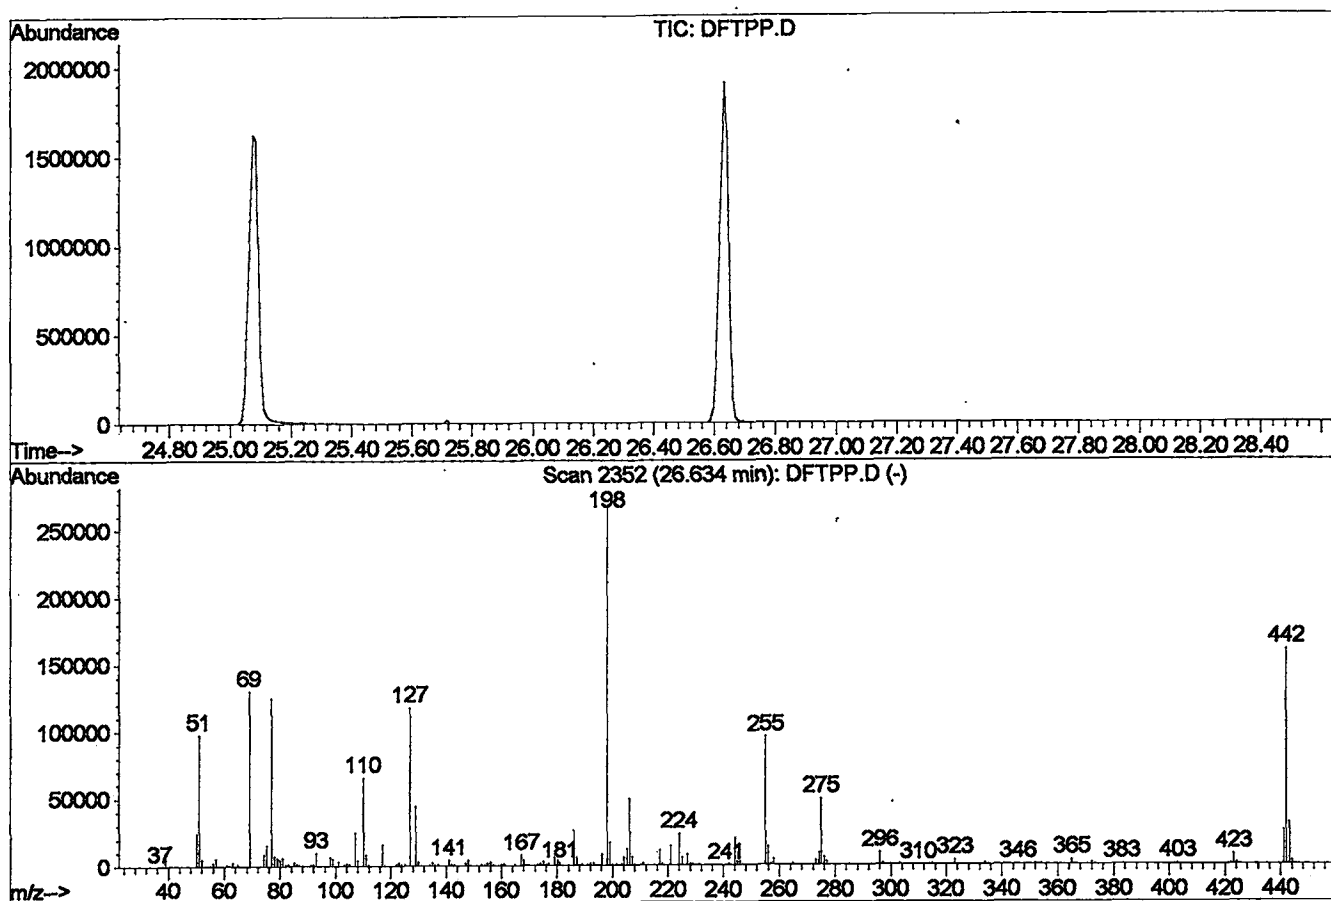

Spectrum Information: Scan 2352

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.6	98040	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.7	130624	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	44.1	118328	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	268160	PASS
199	198	5	9	6.7	17848	PASS
275	198	10	30	18.7	50232	PASS
365	198	1	100	1.5	4105	PASS
441	443	0.01	100	82.6	25368	PASS
442	198	40	110	59.7	160192	PASS
443	442	17	23	19.2	30728	PASS