


DFTPP

Data File : C:\HPCHEM\1\DATA\MAY3102\DFTPP.D
 Acq On : 31 May 2002 11:56 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: Morgan
 Inst : 209
 Multiplr: 1.00

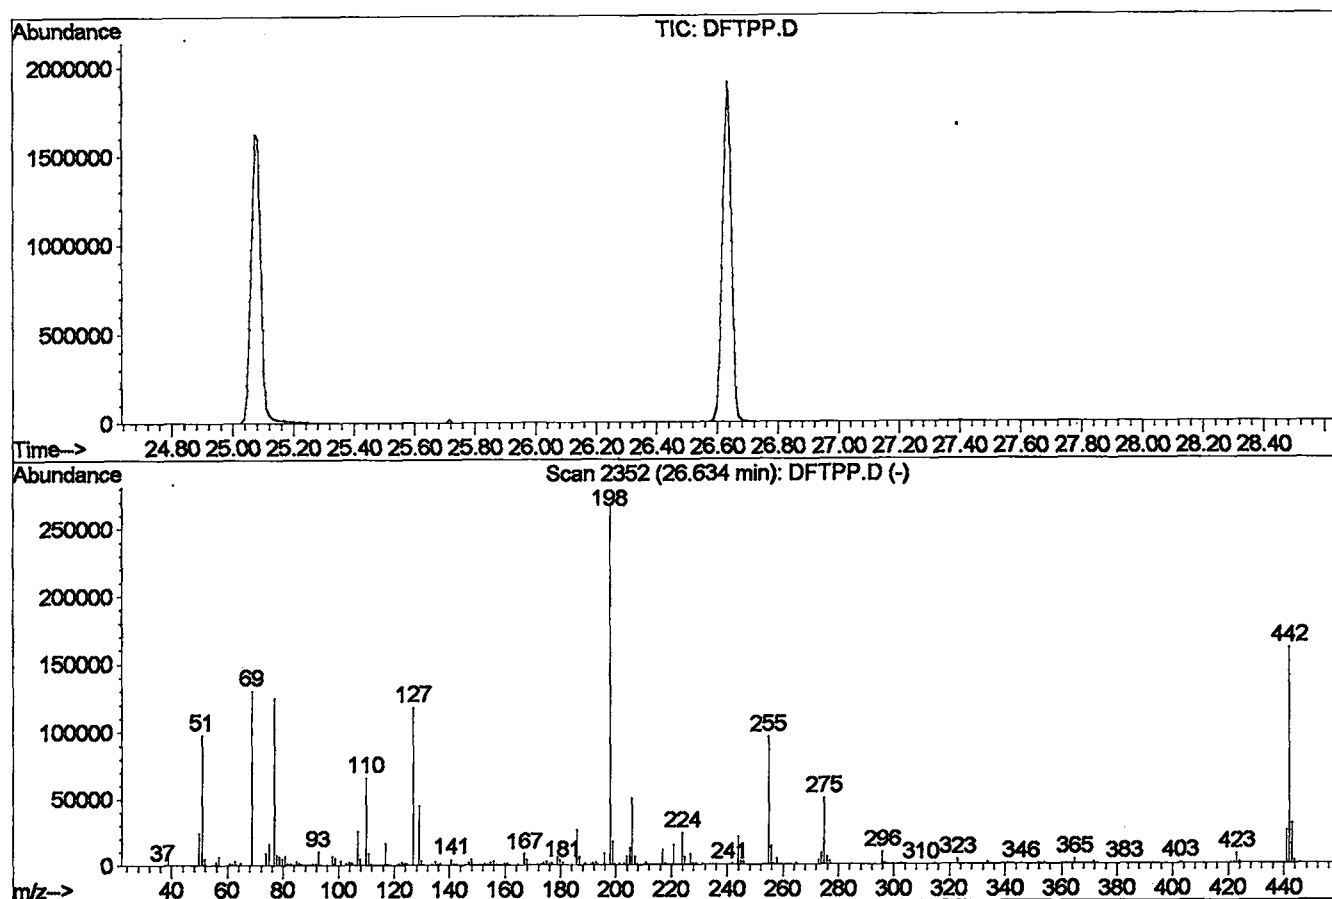

Spectrum Information: Scan 2352

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.6	98040	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.7	130624	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	44.1	118328	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	268160	PASS
199	198	5	9	6.7	17848	PASS
275	198	10	30	18.7	50232	PASS
365	198	1	100	1.5	4105	PASS
441	443	0.01	100	82.6	25368	PASS
442	198	40	110	59.7	160192	PASS
443	442	17	23	19.2	30728	PASS