

Method 508 MOD.Date Extracted 5/31/02Page 7

#GCMs - 18796

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
L.B.		500 mL		1 mL			1 mL	2B	7	
Ref 1					1 mL			2A		
Ref 2					1 mL			3B		
12224	Re-EXT.							9B		
12279	Re-EXT.							9A		
12285	Re-EXT. F.B. & Q							10A		
12286	Re-EXT.							10B		
12678								3A		
12679	F.B.							1A		
12734								4A		
Remarks NaOH WAS ADDED TO THE Q-SAMPLE (12285) TO BRING its PH TO NEUTRAL.										
Reviewed by, <i>[Signature]</i> 8/13/02										
drip rate must be between 5-15 ml/min for liq-liq extractors										
Extraction type - <u>SEP. Fun.</u> Solv. lot# <u>X07E07</u> NaCl lot# <u>V50603</u> Na2SO4 lot# <u>X04595</u>										
STANDARD	INT STD LOG#									
CALIBRATION	053002									
(RE) SPIKE	021902 (5/30/02)									
MDL/MDRF										
Q CHECK										
INT STD.	053102									
SURROGATE	2284 (5/21/02)									
IPC										
ENDRINDT										

Analyst A.D.
Revision 4/12/01Verified by mqReviewed by Dr
Date 6/11/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\jun0302.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\jun0302\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

☒ Full Method☐ Reprocessing Only

On A Barcode Mismatch


☒ Inject Anyway☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0531	
2	Sample	2	CAL10	GCMS0531	
3	Sample	3	LB	GCMS0531	gc/ms scan 5/31
4	Sample	4	REF1	GCMS0531	gc/ms scan 5/31
5	Sample	5	REF2	GCMS0531	gc/ms scan 5/31
6	Sample	6	12224	GCMS0531	re-ext
7	Sample	7	12279	GCMS0531	re-ext
8	Sample	8	12285	GCMS0531	re-ext
9	Sample	9	12286	GCMS0531	re-ext
10	Sample	10	12678	GCMS0531	gc/ms scan 5/31
11	Sample	11	12679	GCMS0531	gc/ms scan 5/31 fb
12	Sample	12	12734	GCMS0531	gc/ms scan 5/31
13	Sample	13	LBA	GCMS0531	gc/ms scan 5/28
14	Sample	14	REFA1	GCMS0531	gc/ms scan 5/28
15	Sample	15	REFA2	GCMS0531	gc/ms scan 5/28
16	Sample	16	12535	GCMS0531	gc/ms scan 5/28 fb
17	Sample	17	12536	GCMS0531	gc/ms scan 5/28
18	Sample	18	12537	GCMS0531	gc/ms scan 5/28
19	Sample	19	12538	GCMS0531	gc/ms scan 5/28
20	Sample	20	12539	GCMS0531	gc/ms scan 5/28 fb
21	Sample	21	12570	GCMS0531	gc/ms scan 5/28
22	Sample	22	12571	GCMS0531	gc/ms scan 5/28
23	Sample	23	12572	GCMS0531	gc/ms scan 5/28
24	Sample	24	12573	GCMS0531	gc/ms scan 5/28
25	Sample	25	12574	GCMS0531	gc/ms scan 5/28

DFTPP

Data File : C:\HPCHEM\1\DATA\JUN0302\DFTPP.D
 Acq On : 3 Jun 2002 8:41 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0531.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: Morgan
 Inst : 209
 Multiplr: 1.00

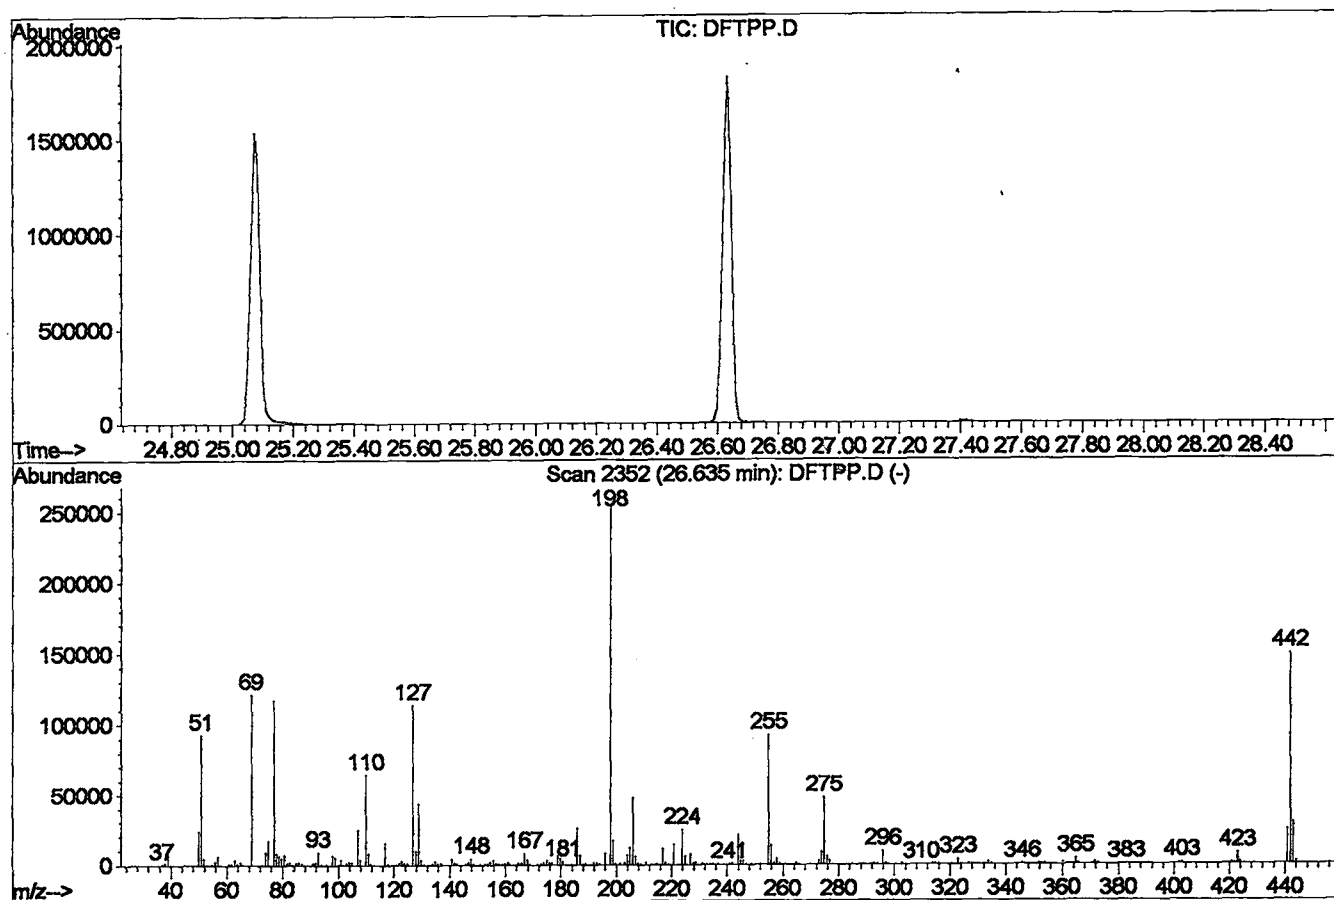

Spectrum Information: Scan 2352

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.5	93048	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.6	121424	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	44.7	113896	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	254976	PASS
199	198	5	9	6.8	17248	PASS
275	198	10	30	18.6	47448	PASS
365	198	1	100	1.6	4084	PASS
441	443	0.01	100	82.0	24120	PASS
442	198	40	110	58.5	149120	PASS
443	442	17	23	19.7	29416	PASS