

NYC-WTC\_000015649

## DFTPP

Data File : C:\MSDCHEM\1\DATA\061002\DFTPP.D

Vial: 1

Acq On : 10 Jun 2002 10:05 am

Operator:

Sample :

Inst : Instrume


Misc :

Multiplr: 1.00

MS Integration Params: EVENTS.E

Method : C:\MSDCHEM\1\METHODS\060302.M (Chemstation Integrator)

Title : 508 Modified GC/MS scan

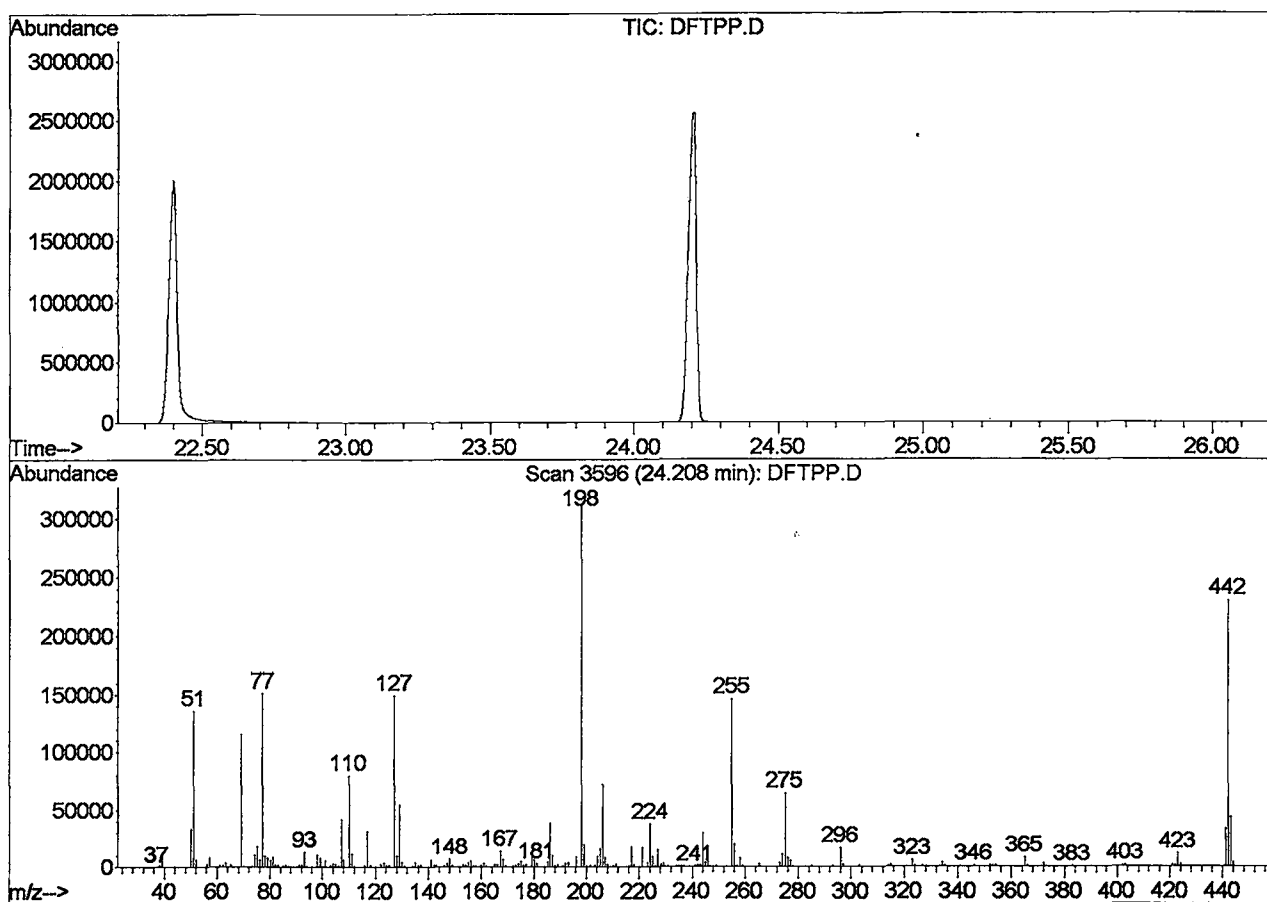

## Spectrum Information: Scan 3596

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 30           | 60           | 43.7      | 136640  | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 37.1      | 116016  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 646     | PASS             |
| 127         | 198          | 40           | 60           | 47.9      | 149824  | PASS             |
| 197         | 198          | 0.00         | 1            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 312896  | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 20424   | PASS             |
| 275         | 198          | 10           | 30           | 20.7      | 64720   | PASS             |
| 365         | 198          | 1            | 99           | 2.7       | 8410    | PASS             |
| 441         | 443          | 1            | 100          | 77.0      | 33824   | PASS             |
| 442         | 198          | 40           | 110          | 73.6      | 230144  | PASS             |
| 443         | 442          | 17           | 23           | 19.1      | 43944   | PASS             |

DFTPP.D 060302.M

Tue Jun 11 08:13:50 2002