

DFTPP

Data File : C:\MSDCHEM\1\DATA\061102\DFTPP.D

Vial: 1

Acq On : 11 Jun 2002 10:30 am

Operator:

Sample :

Inst : Instrume


Misc :

Multiplr: 1.00

MS Integration Params: EVENTS.E

Method : C:\MSDCHEM\1\METHODS\060302.M (Chemstation Integrator)

Title : 508 Modified GC/MS scan

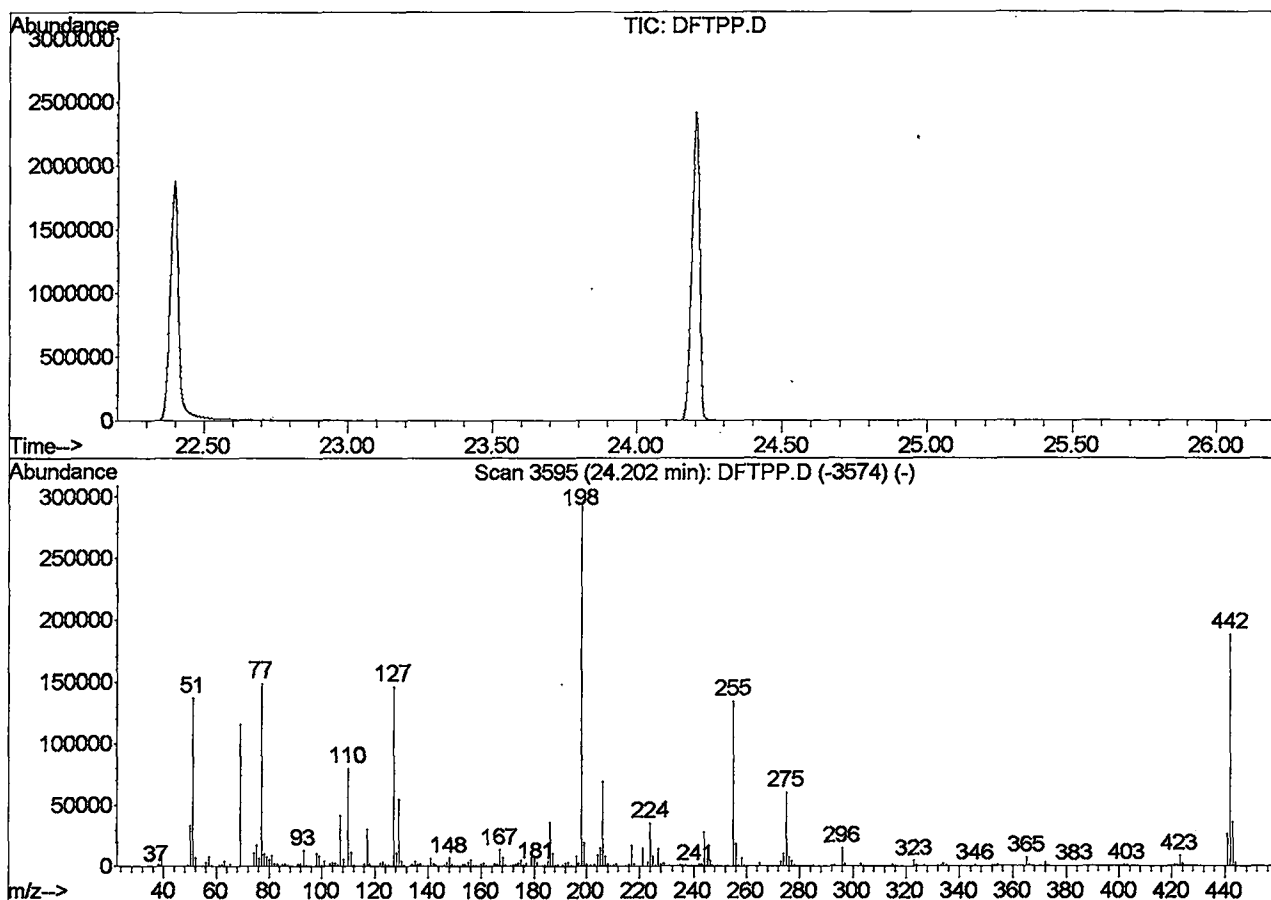

Spectrum Information: Scan 3595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	46.7	137600	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.4	116168	PASS
70	69	0.00	2	0.4	451	PASS
127	198	40	60	49.8	146688	PASS
197	198	0.00	1	1.0	2872	PASS
198	198	100	100	100.0	294592	PASS
199	198	5	9	6.7	19824	PASS
275	198	10	30	20.6	60632	PASS
365	198	1	99	2.5	7256	PASS
441	443	1	100	74.4	27344	PASS
442	198	40	110	64.0	188416	PASS
443	442	17	23	19.5	36752	PASS

DFTPP.D 060302.M

Tue Jun 11 14:03:22 2002