


User: Bohlk, Ted
Westchester Dept. of Labs & Research
Date: 05/14/2002 Time: 14:41:30

Sample: AE11755
Analysis: SLP525 Organic Extractables
Units: ug
Started: 5/13/02 14:40 Ended: 5/13/02 14:40 Analyst: TB
Page: 1

	Component Name	Viol	Result
1	DFTPP		PASSED
2	ENDRIN		5.1
3	DDT		0

File : C:\MSDCHEM\1\DATA\051302\DFTA0513.D
 Operator : Bohlk / Inst 213
 Acquired : 13 May 2002 2:43 pm using AcqMethod 050802
 Instrument : Instrumen
 Sample Name: DFTPP/ENDRIN
 Misc Info :
 Vial Number: 4

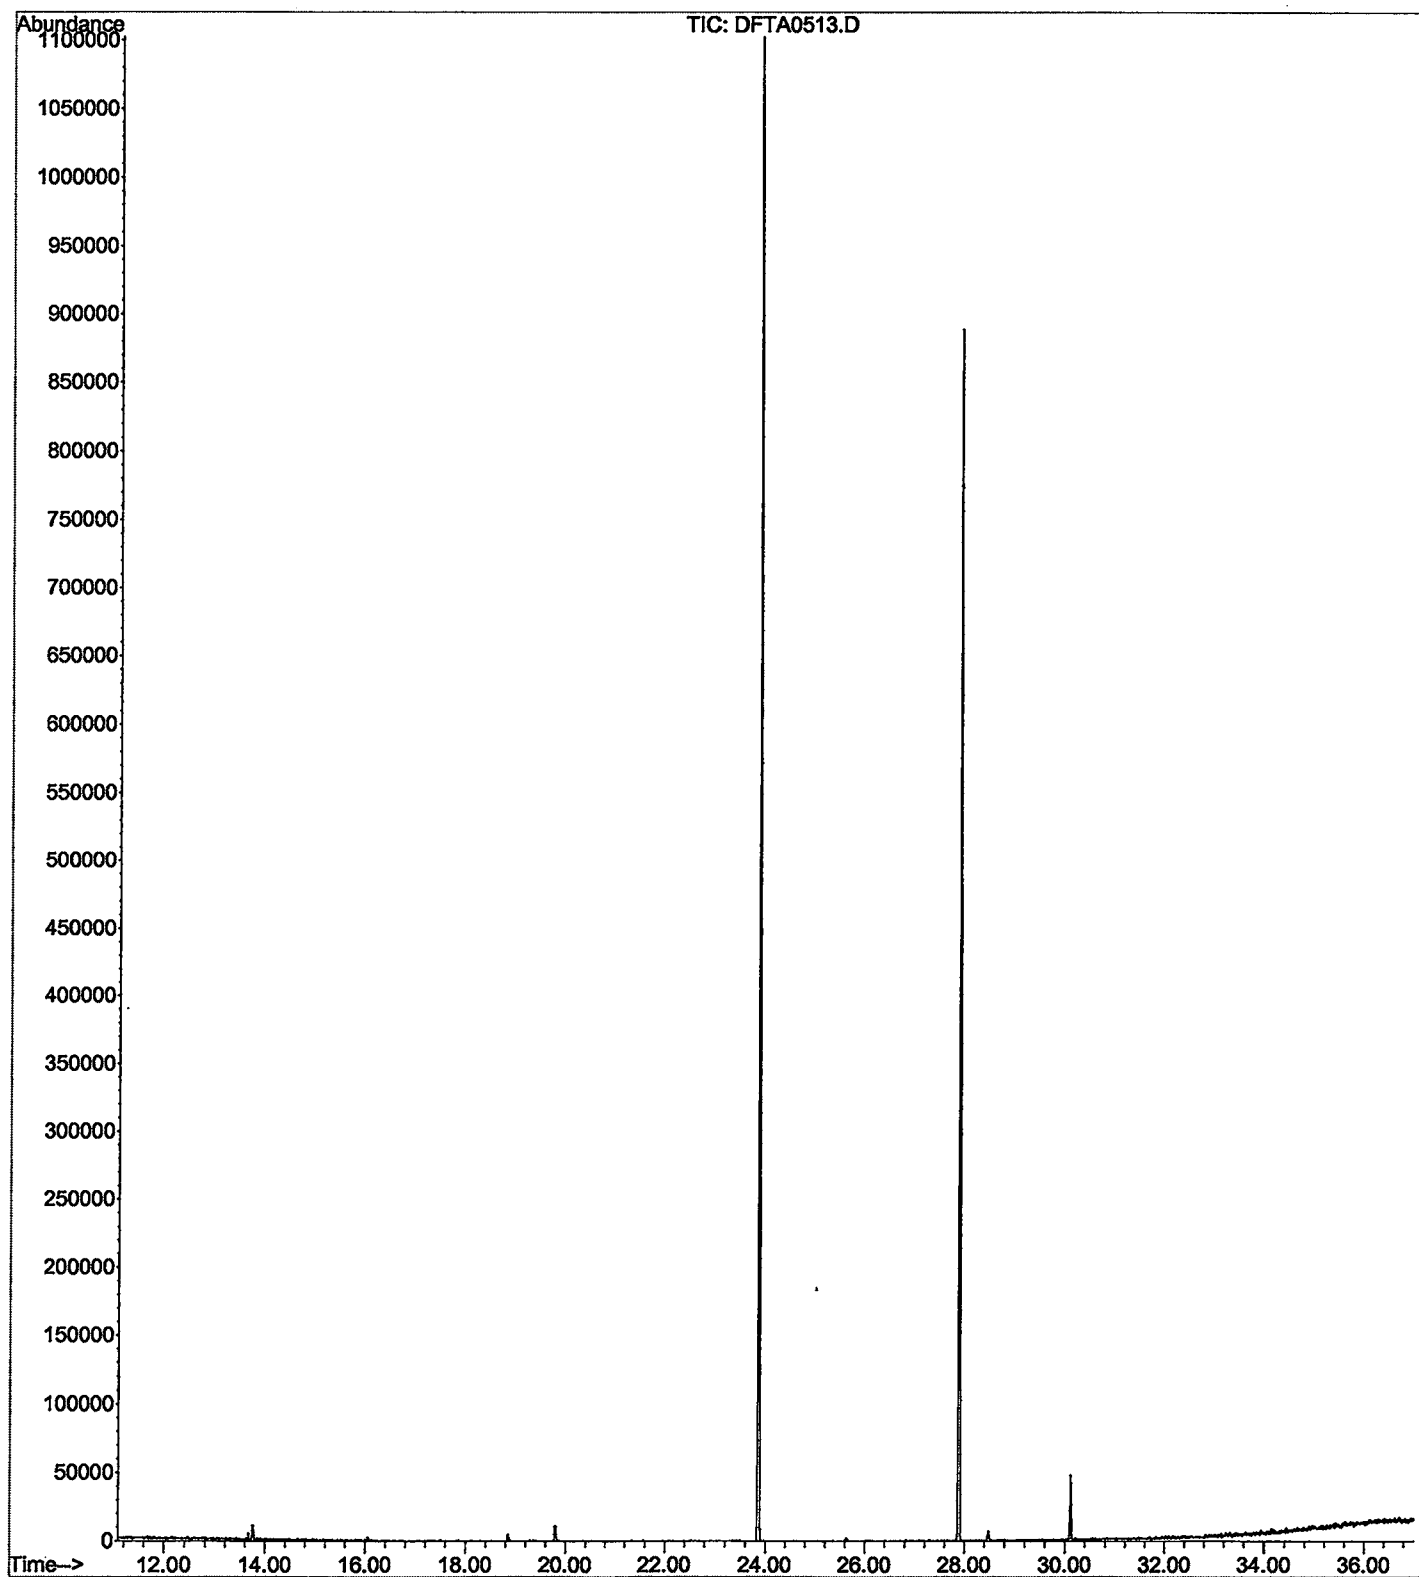

DFTPP

Data File : C:\MSDCHEM\1\DATA\051302\DFTA0513.D

Vial: 4

Acq On : 13 May 2002 2:43 pm

Operator: Bohlk / Inst 213

Sample : DFTPP/ENDRIN

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: rteint.p

Method : C:\MSDCHEM\1\5973N\050802.M (RTE Integrator)

Title : Quantitation For Method 525.2

Spectrum Information: Average of 23.811 to 23.910 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	11732	PASS
68	69	0.00	2	1.0	136	PASS
69	198	0.00	100	39.5	14050	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.3	20417	PASS
197	198	0.00	2	0.4	152	PASS
198	198	50	100	100.0	35602	PASS
199	198	5	9	6.7	2400	PASS
275	198	10	60	18.4	6539	PASS
365	198	1	100	1.8	630	PASS
441	443	0.01	100	67.9	3328	PASS
442	198	50	100	72.3	25725	PASS
443	442	15	24	19.0	4899	PASS

DFTA0513.D 050802.M

Mon May 13 15:32:49 2002

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\051302\DFTA0513.D
 Acq On : 13 May 2002 2:43 pm
 Sample : DFTPP/ENDRIN
 Misc :
 MS Integration Params: rteint.p

Vial: 4
 Operator: Bohlk / Inst 213
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\050802.M (RTE Integrator)
 Title : Quantitation For Method 525.2
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 5000 Area counts
 Start Thrs: 0.2 Max Peaks: 10
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5


Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	27.892	1849	1854	1857	rM	888849	1560612	100.00%	94.929%
2	28.491	1916	1920	1923	rM	6512	10513	0.67%	0.639%
3	30.114	2096	2099	2103	rM 2	47331	72856	4.67%	4.432%

Sum of corrected areas: 1643981

5.1 ⁷/₂
 Endrin
 Breakdown

File : C:\MSDCHEM\1\DATA\051302\DDTA0513.D
 Operator : Bohlk / Inst 213
 Acquired : 13 May 2002 3:29 pm using AcqMethod 050802
 Instrument : Instrumen
 Sample Name: DDT
 Misc Info :
 Vial Number: 5

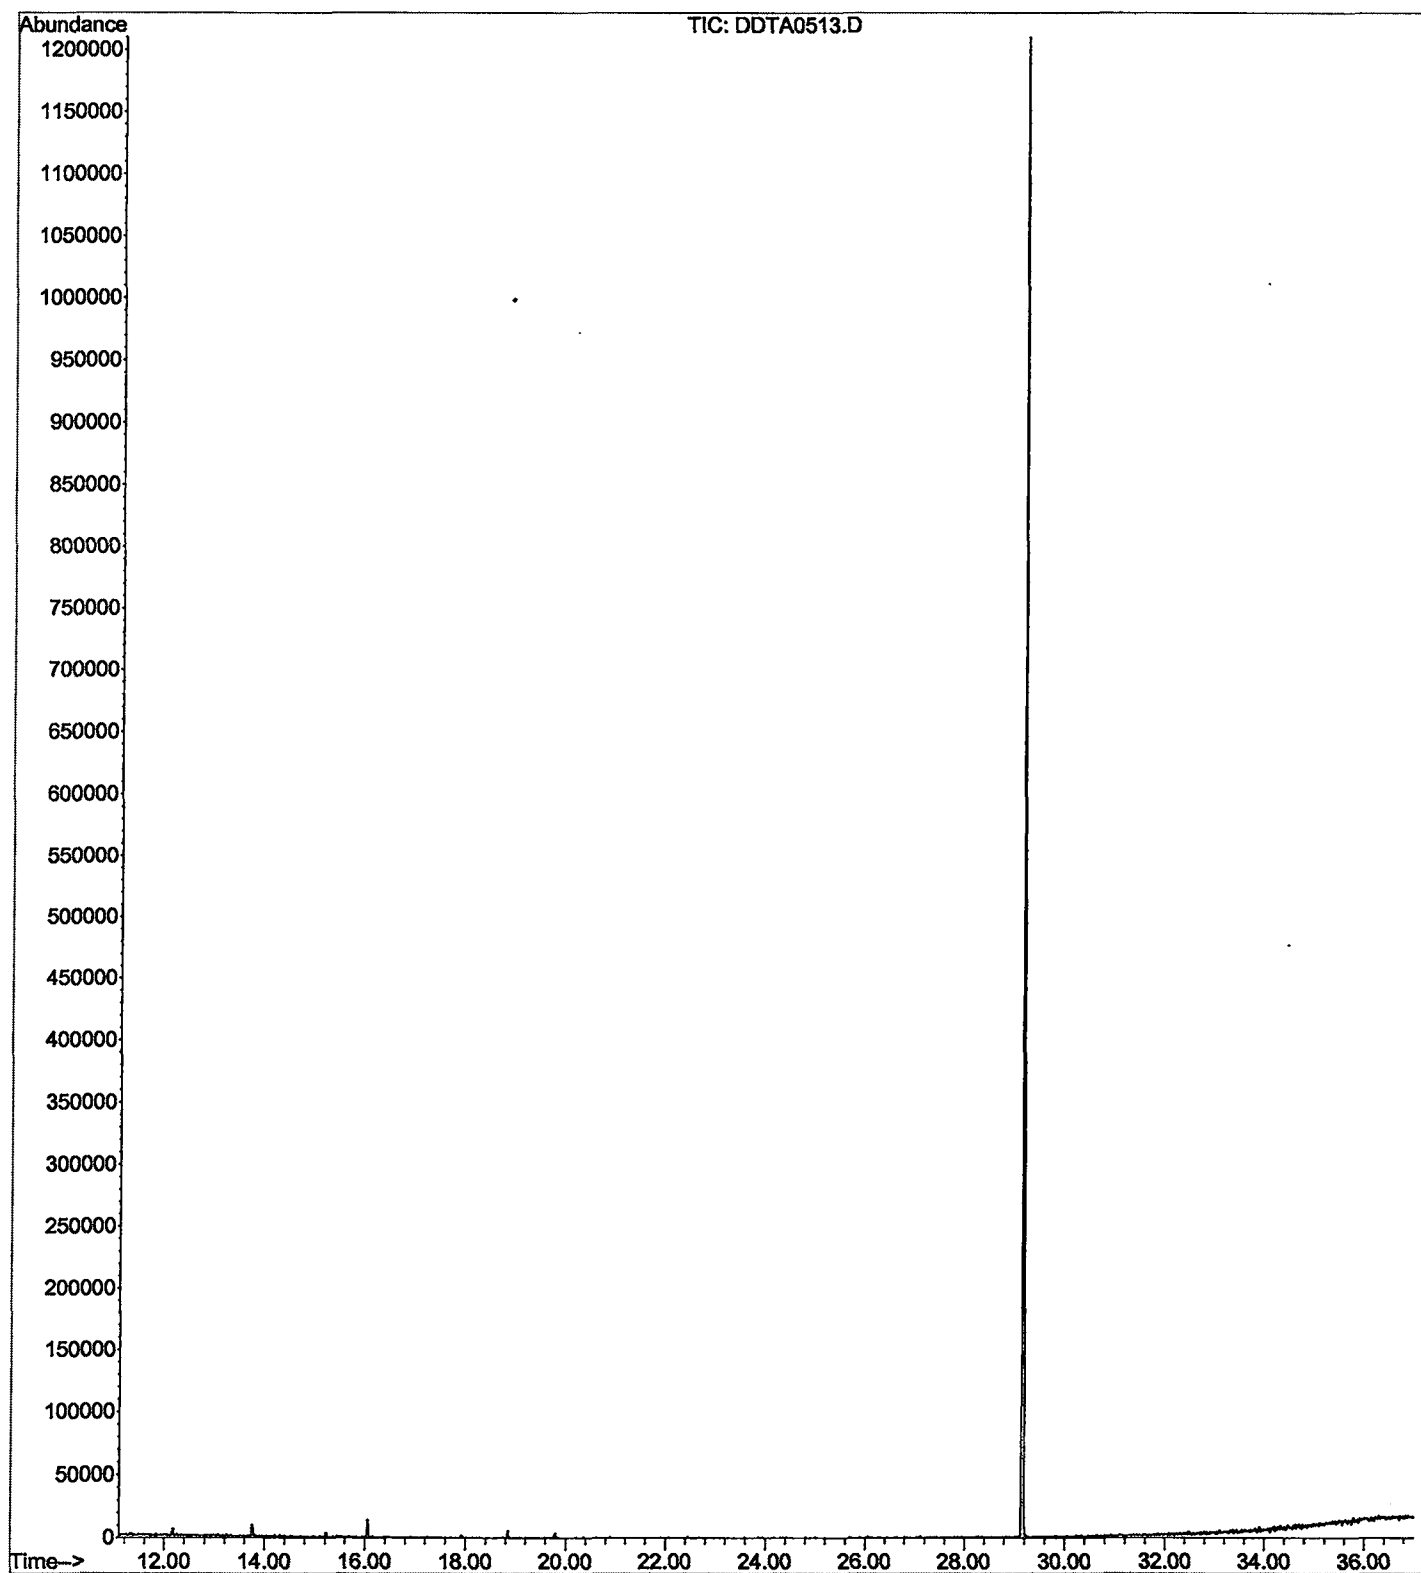

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\051302\DDTA0513.D Vial: 5
 Acq On : 13 May 2002 3:29 pm Operator: Bohlk / Inst 213
 Sample : DDT Inst : Instrumen
 Misc : Multiplr: 1.00
 MS Integration Params: rteint.p

Method : C:\MSDCHEM\1\5973N\050802.M (RTE Integrator)
 Title : Quantitation For Method 525.2
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 5000 Area counts
 Start Thrs: 0.2 Max Peaks: 10
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	29.153	1988	1993	2003	rM	1209198	2108632	100.00%	100.000%

Sum of corrected areas: 2108632