

Method 508 modified Date Extracted 12/12/01Page 59

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Sol add	IS add	Final vol.	T.V. pos.	pH	Count		
REF		500ml		1ml			1ml		7			
✓ 300922		↓		↓	0.5ml		↓	8A	↓			
✓ 300921		↓		↓			↓	8B	↓			
✓ 30113		↓		↓			↓	7A	↓			
✓ 30112		↓		↓			↓	8B	↓			
✓ 30087		↓		↓			↓	6A	↓			
✓ 30086		↓		↓			↓	6B	↓			
✓ 30118		↓		↓			↓	6A	↓			
✓ 30117		↓		↓			↓	8A	↓			
✓ 30116		↓		↓			↓	7B	↓			
✓ 30257		↓		↓			↓	7A	↓			
								6B				
Remarks												
Reviewed by: <u>LB</u> 5/15/02												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type - <u>Sep fun</u> Solv. lot# <u>V39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V3 H00</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	<u>91759</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>CREMS 12-11-01</u>											
LPC												
ENDRIN/DDT												

Analyst gheith
revision 4/12/01

Verified by _____

Reviewed by DN
Date 1/9/02

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC1801\DFTPP1.D

Acq On : 19 Dec 2001 8:42 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

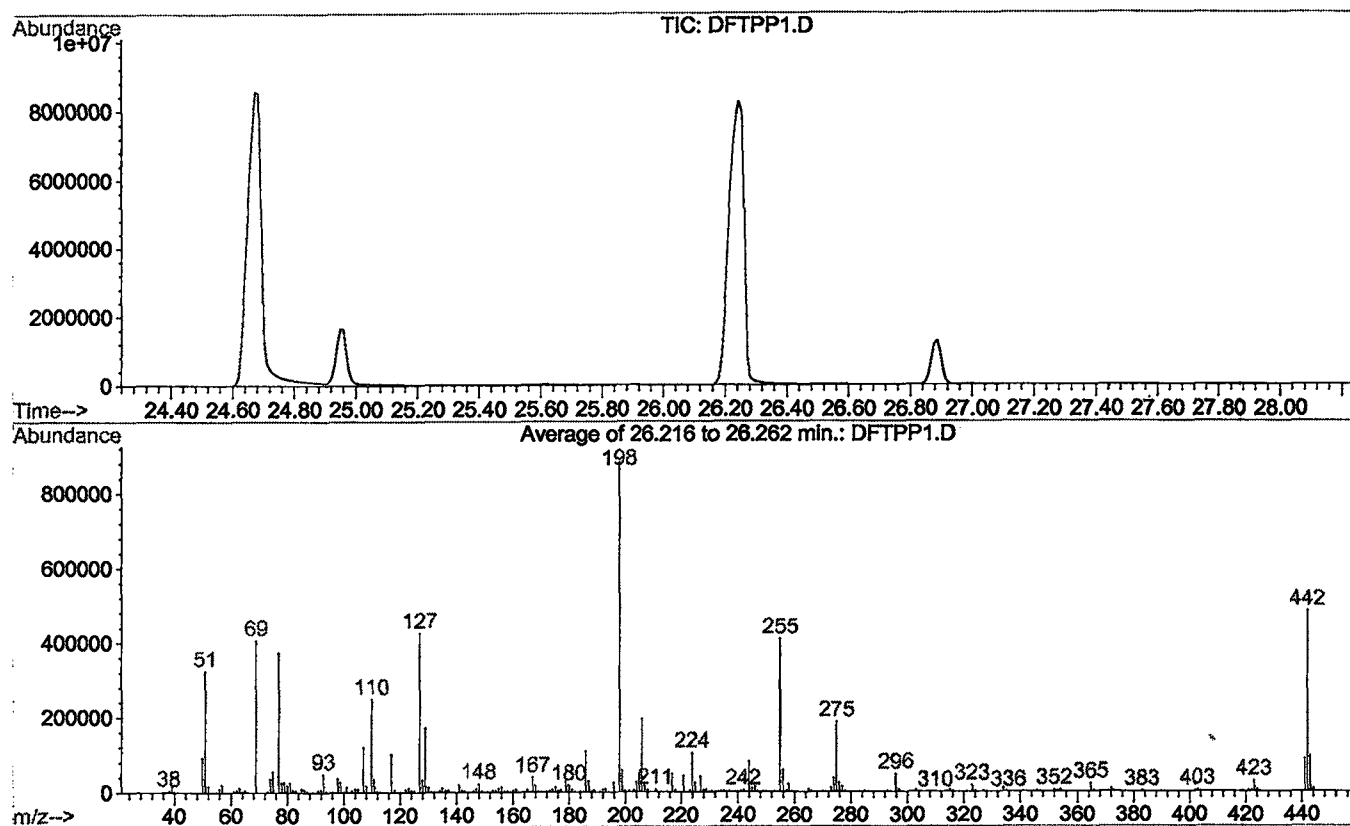

Spectrum Information: Average of 26.216 to 26.262 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.9	325045	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.2	406955	PASS
70	69	0.00	2	0.0	56	PASS
127	198	40	60	48.4	426496	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	881184	PASS
199	198	5	9	6.6	58321	PASS
275	198	10	30	21.1	185931	PASS
365	198	1	100	2.5	21764	PASS
441	443	0.01	100	92.7	86832	PASS
442	198	40	110	54.7	481835	PASS
443	442	17	23	19.4	93632	PASS

DFTPP1.D GCMS1126.M

Thu Jan 03 10:06:05 2002